


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050115\
 Data File : BG016841.D
 Acq On : 1 May 2015 11:59
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 01 13:58:29 2015

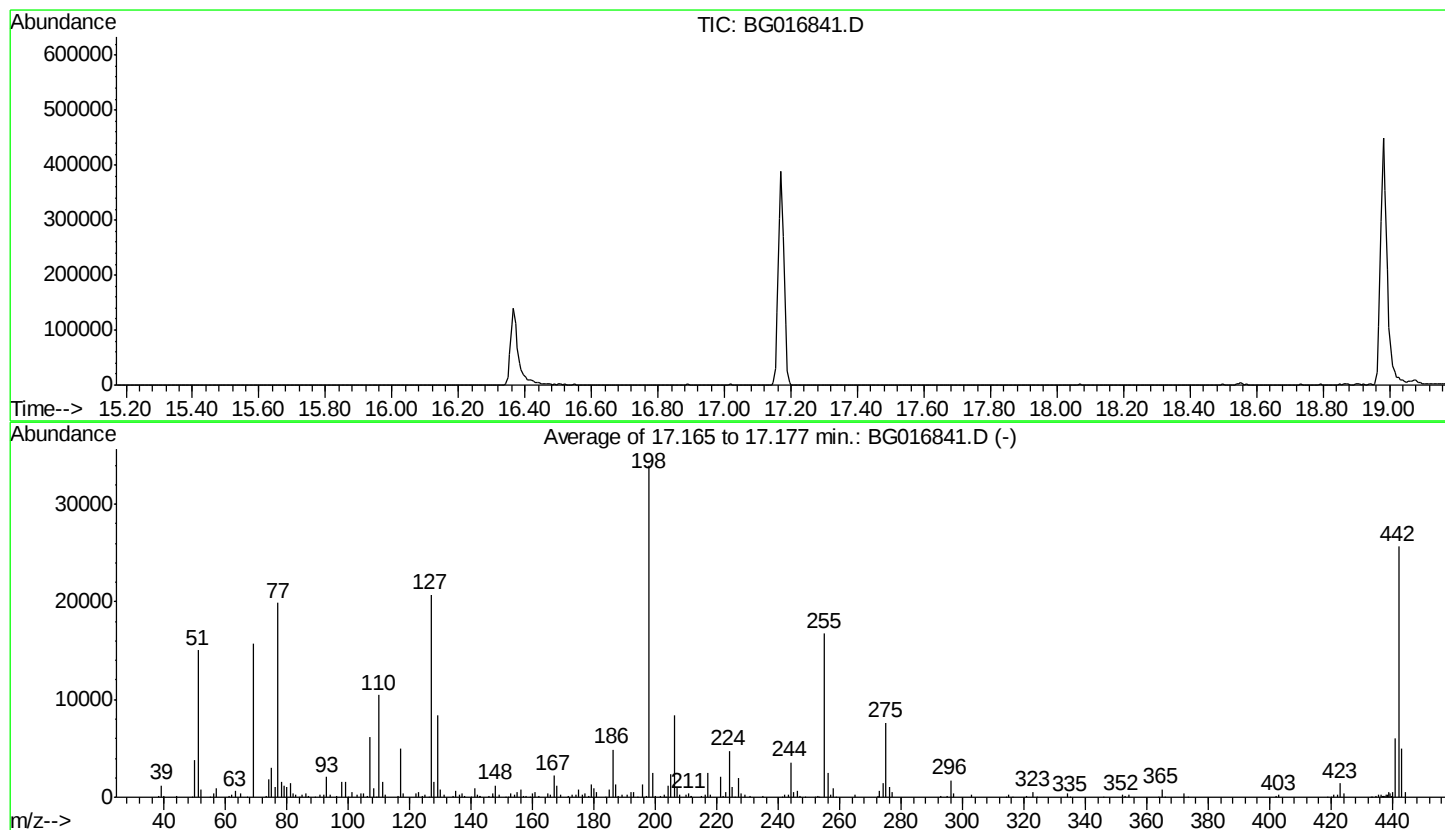

AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	15054	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.5	15788	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	61.1	20749	PASS
197	198	0.00	2	0.5	168	PASS
198	198	100	100	100.0	33946	PASS
199	198	5	9	7.3	2485	PASS
275	198	10	60	22.5	7621	PASS
365	198	1	100	2.5	845	PASS
441	442	0.01	24	23.3	5973	PASS
442	198	50	100	75.5	25624	PASS
443	442	15	24	19.3	4955	PASS