

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050115\
 Data File : BG016849.D
 Acq On : 1 May 2015 17:38
 Operator : TP/IZ
 Sample : G2012-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FYMW-04

Quant Time: May 02 00:04:26 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 01 23:47:41 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.26	152	53656	20.00	ng	0.00
21) Naphthalene-d8	10.03	136	242459	20.00	ng	0.00
38) Acenaphthene-d10	13.94	164	143555	20.00	ng	0.00
63) Phenanthrene-d10	16.70	188	294159	20.00	ng	0.00
75) Chrysene-d12	20.91	240	261971	20.00	ng	0.00
86) Perylene-d12	22.98	264	237963	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	4.87	112	171349	58.82	ng	0.00
7) Phenol-d6	6.48	99	138006	33.75	ng	0.00
23) Nitrobenzene-d5	8.42	82	337582	90.70	ng	0.00
41) 2,4,6-Tribromophenol	15.45	330	155199	145.16	ng	0.00
44) 2-Fluorobiphenyl	12.55	172	823587	88.83	ng	0.00
78) Terphenyl-d14	19.36	244	824023	75.87	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050115\
Data File : BG016849.D
Acq On : 1 May 2015 17:38
Operator : TP/IZ
Sample : G2012-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FYMW-04

Quant Time: May 02 00:04:26 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 01 23:47:41 2015
Response via : Initial Calibration

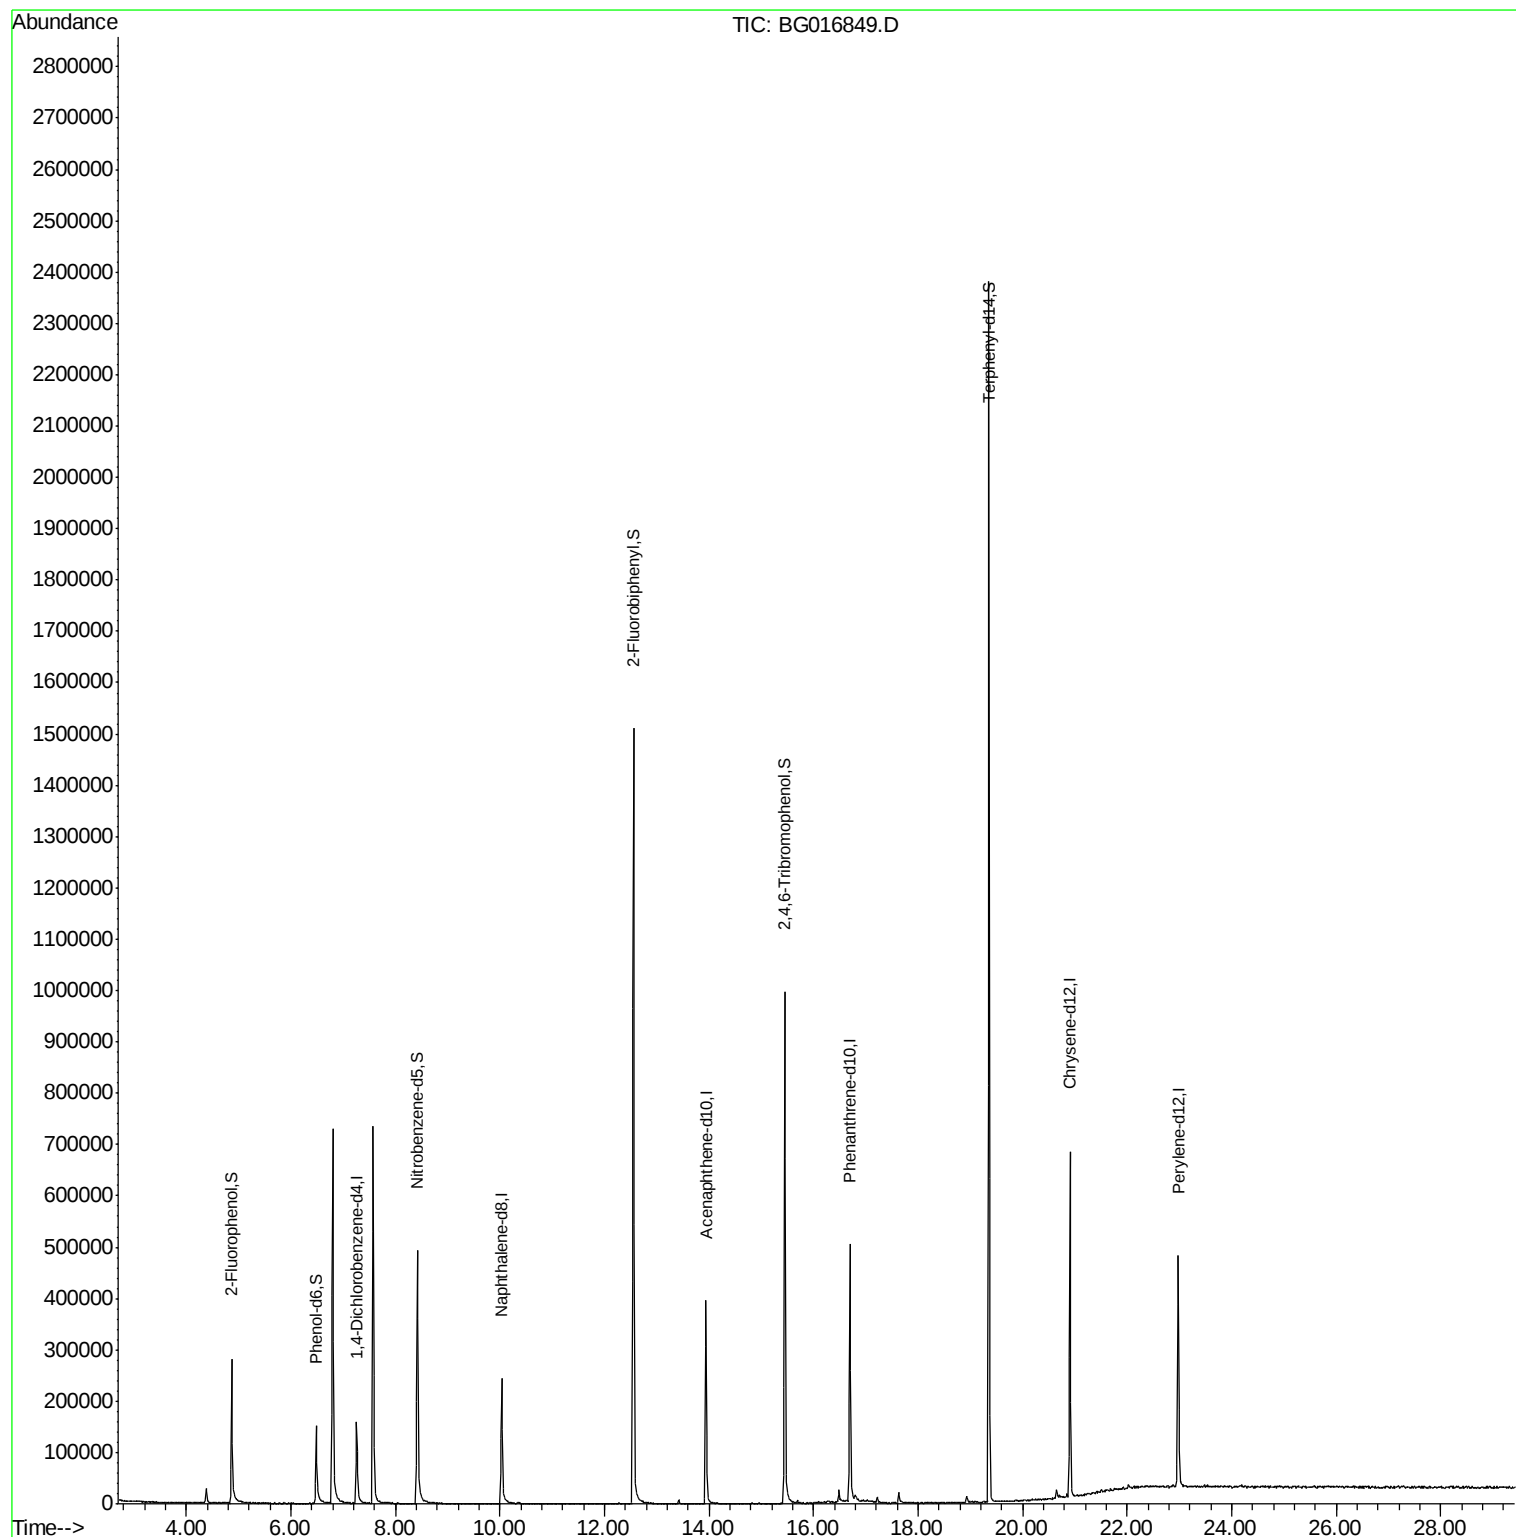

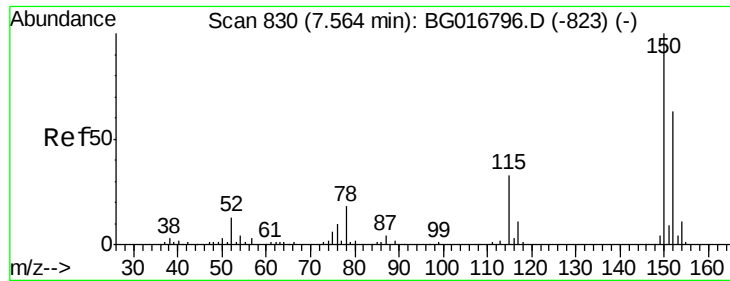


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.26 min Scan# 778
Delta R.T. 0.00 min
Lab File: BG016849.D
Acq: 1 May 2015 17:38

Instrument :
BNA_G
ClientSampleId :
FYMW-04

Tot Ion:152 Resp: 53656
Ion Ratio Lower Upper
152 100
150 144.0 126.2 189.4
115 51.2 41.1 61.7

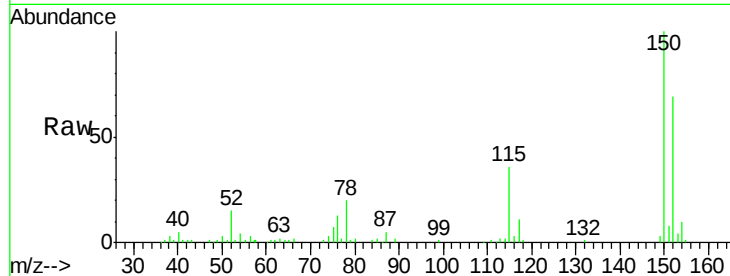


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

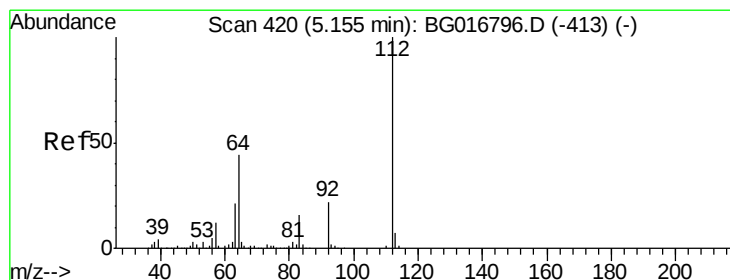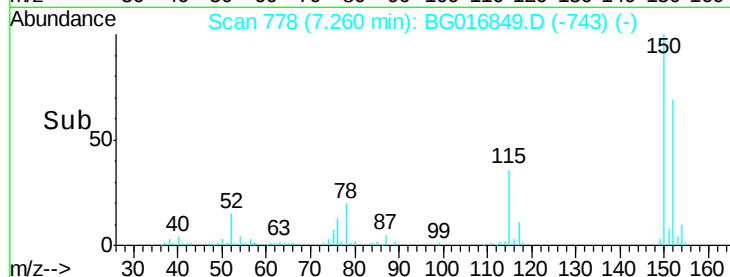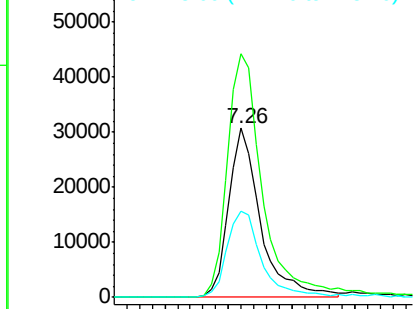



#5


2-Fluorophenol
Concen: 58.82 ng
RT: 4.87 min Scan# 371
Delta R.T. 0.01 min
Lab File: BG016849.D
Acq: 1 May 2015 17:38

Tgt Ion:112 Resp: 171349
Ion Ratio Lower Upper
112 100
64 46.9 35.5 53.3
63 24.2 17.2 25.8

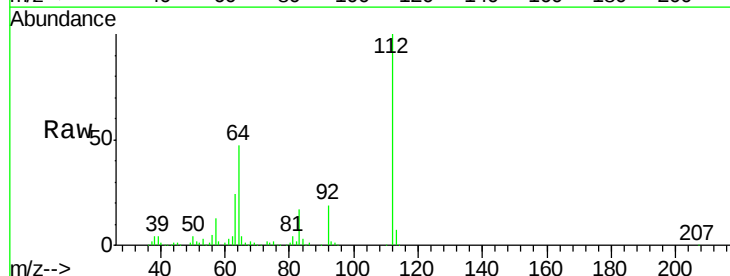

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

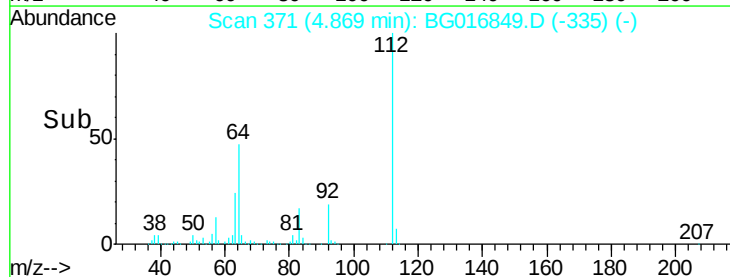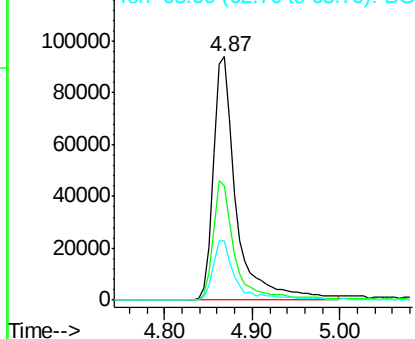

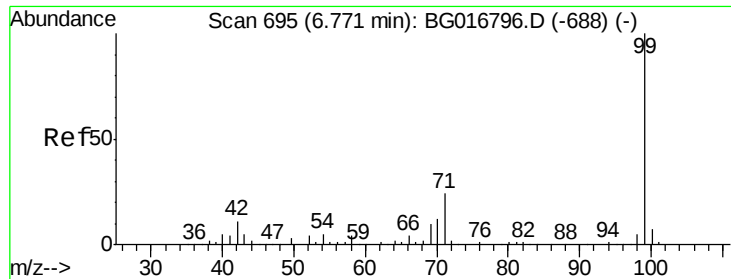

#7

Phenol-d6

Concen: 33.75 ng

RT: 6.48 min Scan# 646

Delta R.T. 0.01 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38

Instrument :

BNA_G

ClientSampleId :

FYMW-04


Tot Ion: 99 Resp: 138006

Ion Ratio Lower Upper




99 100

42 11.8 8.9 13.3

71 25.5 19.0 28.6

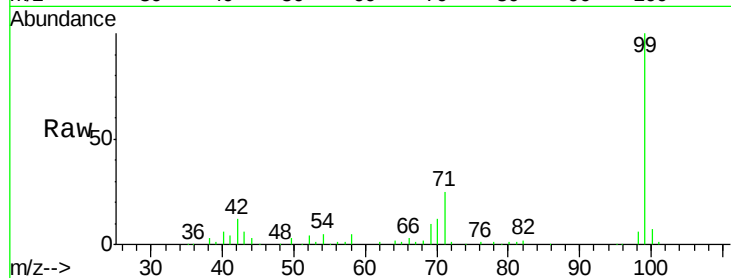

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

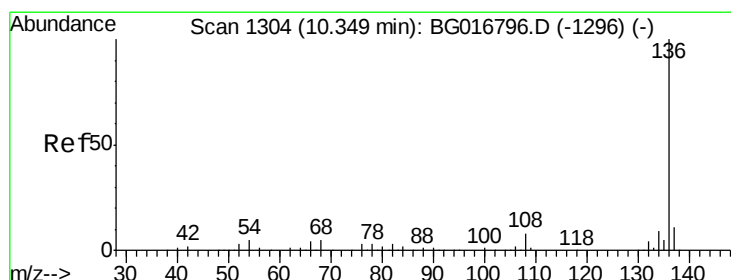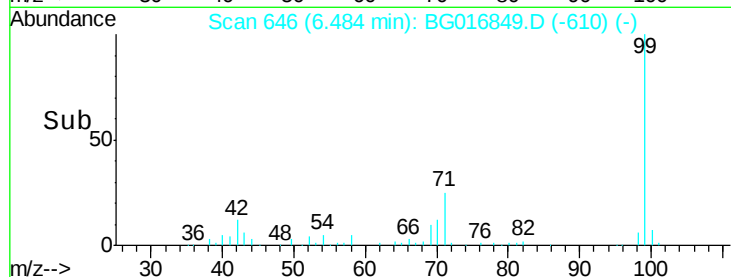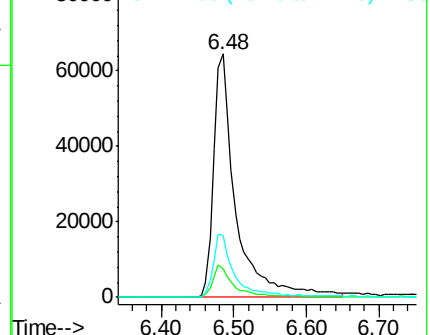

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.03 min Scan# 1250

Delta R.T. 0.00 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38

Tgt Ion: 136 Resp: 242459


Ion Ratio Lower Upper

136 100



137 10.8 8.6 12.8


54 5.7 4.3 6.5

68 5.6 4.3 6.5

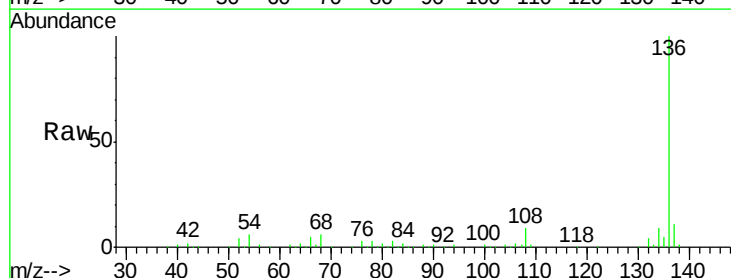

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



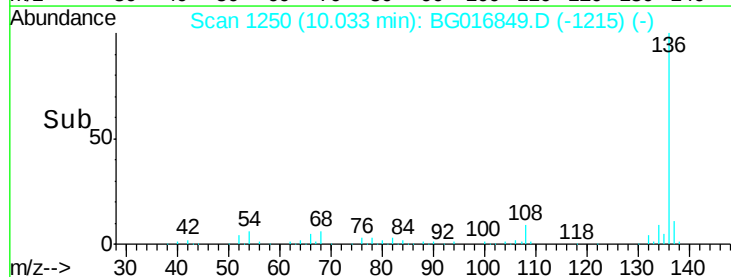
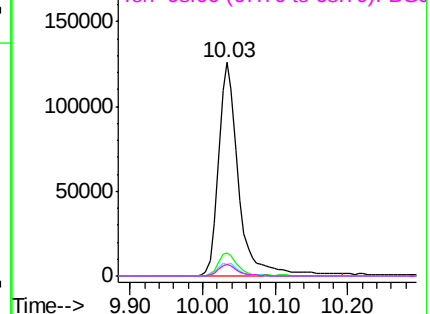


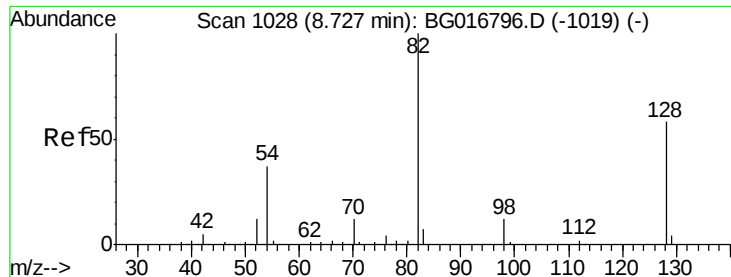

#23
Nitrobenzene-d5
Concen: 90.70 ng
RT: 8.42 min Scan# 976
Delta R.T. 0.00 min
Lab File: BG016849.D
Acq: 1 May 2015 17:38




Instrument :
BNA_G
ClientSampleId :
FYMW-04


Tot Ion: 82 Resp: 337582
Ion Ratio Lower Upper
82 100
128 54.6 46.3 69.5
54 39.9 30.0 45.0

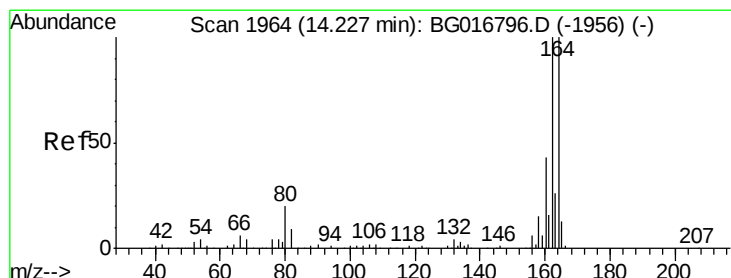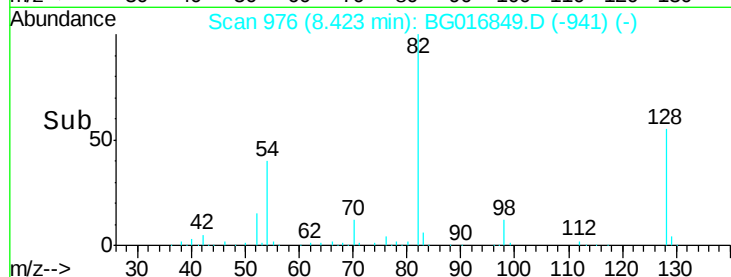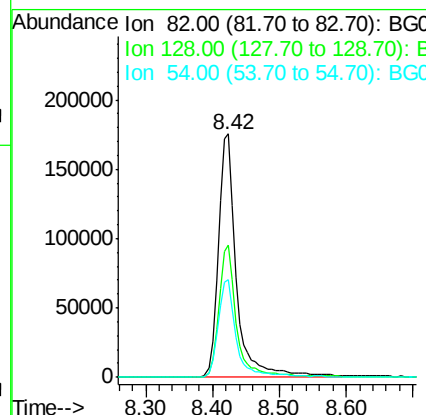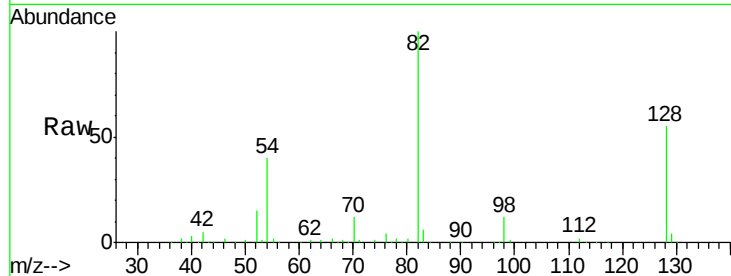

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 13.94 min Scan# 1915
Delta R.T. -0.00 min
Lab File: BG016849.D
Acq: 1 May 2015 17:38

Tgt Ion:164 Resp: 143555
Ion Ratio Lower Upper
164 100
162 97.1 80.2 120.4
160 43.1 34.8 52.2


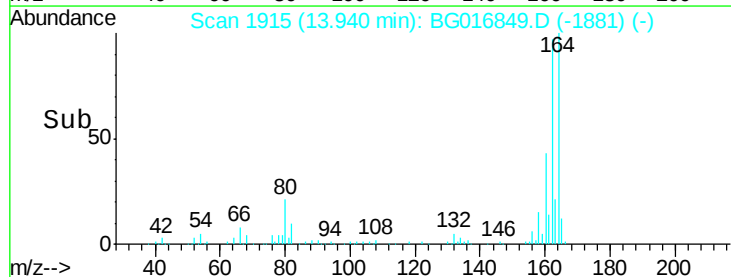
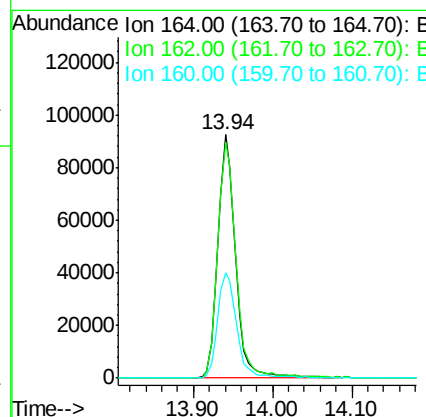
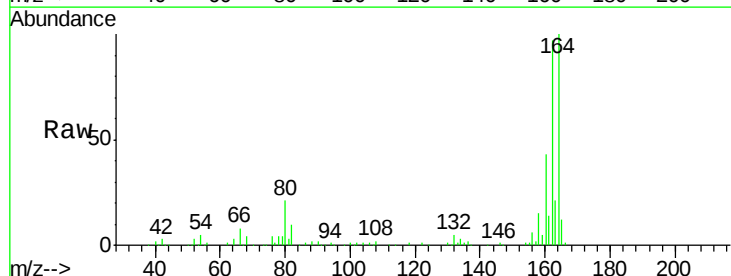


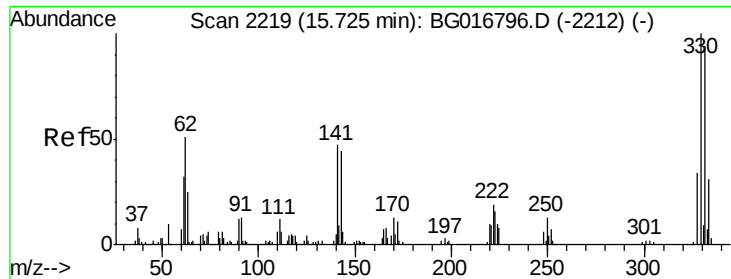

#41
 2,4,6-Tribromophenol
 Concen: 145.16 ng
 RT: 15.45 min Scan# 2172
 Delta R.T. -0.00 min
 Lab File: BG016849.D
 Acq: 1 May 2015 17:38




Instrument :
 BNA_G
 ClientSampleId :
 FYMW-04


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	75.3	112.9
141	52.6	40.7	61.1

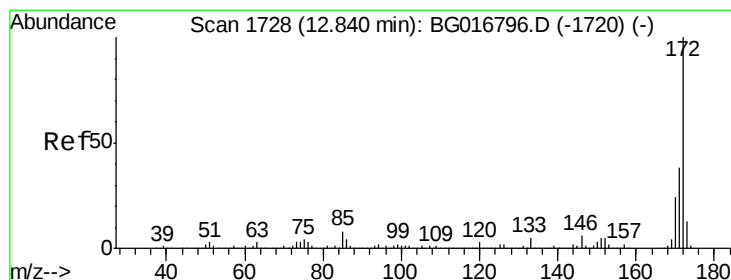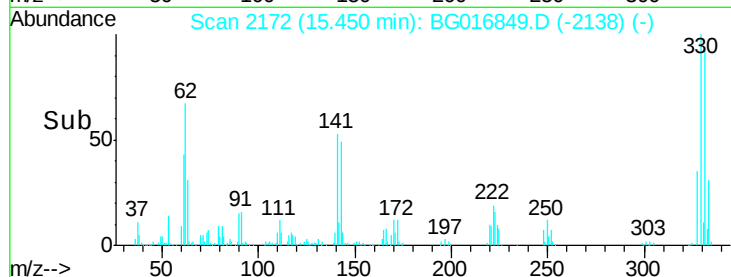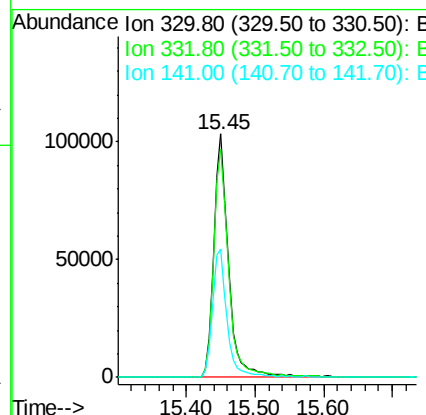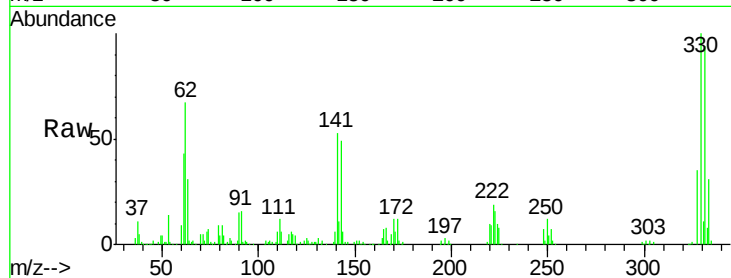

#44
 2-Fluorobiphenyl
 Concen: 88.83 ng
 RT: 12.55 min Scan# 1679
 Delta R.T. 0.00 min
 Lab File: BG016849.D
 Acq: 1 May 2015 17:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.9	30.2	45.4
170	24.5	19.4	29.0

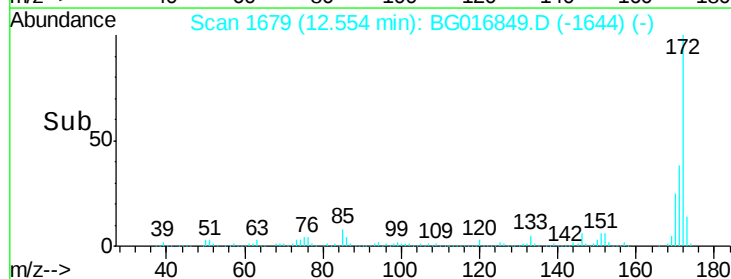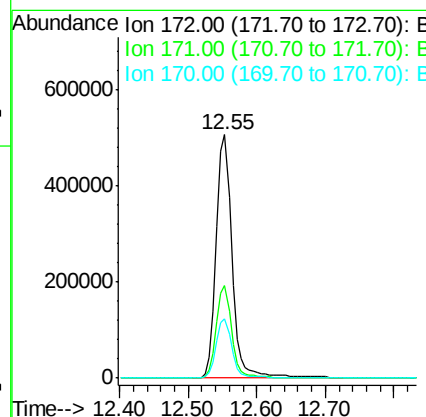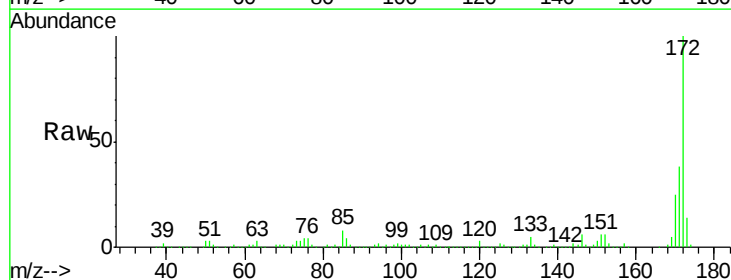

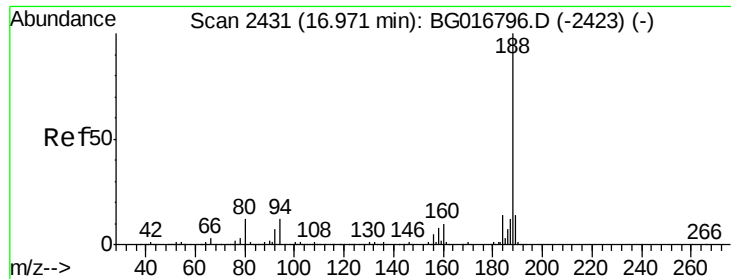

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 16.70 min Scan# 2384

Delta R.T. -0.00 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38

Instrument :

BNA_G

ClientSampleId :

FYMW-04


Tot Ion:188 Resp: 294159

Ion Ratio Lower Upper

188 100

94 11.2 9.5 14.3




80 12.0 9.2 13.8

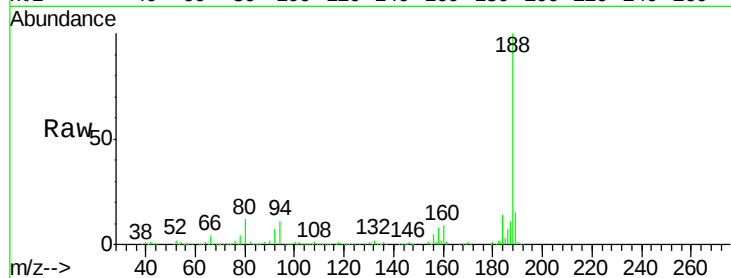

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

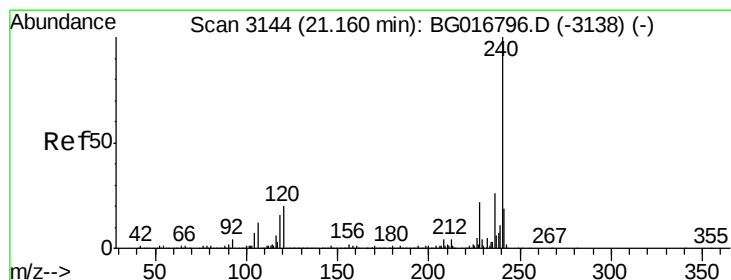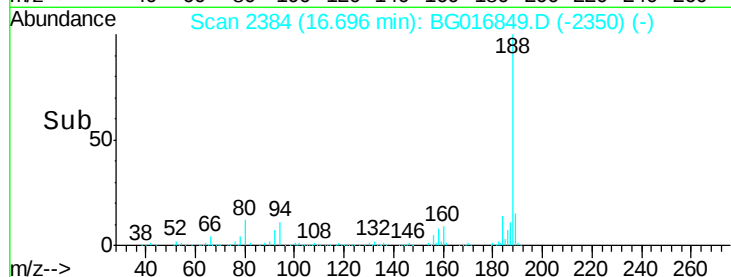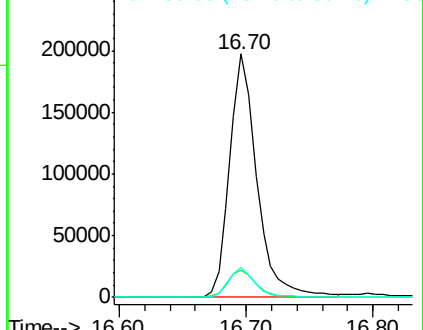

#75

Chrysene-d12

Concen: 20.00 ng

RT: 20.91 min Scan# 3101

Delta R.T. -0.01 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38


Tgt Ion:240 Resp: 261971

Ion Ratio Lower Upper

240 100

120 17.4 16.1 24.1



236 27.6 21.0 31.6

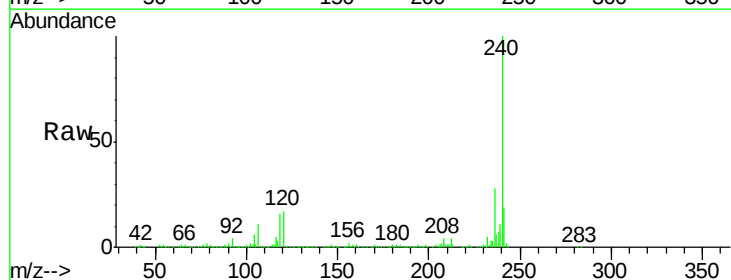


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

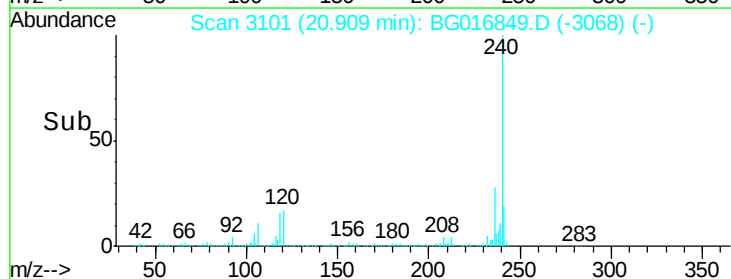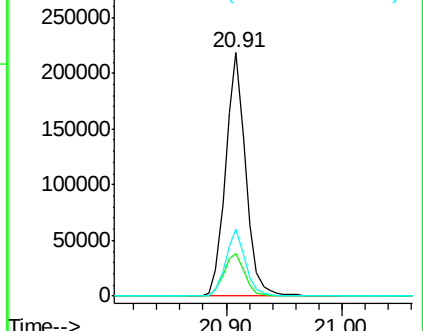

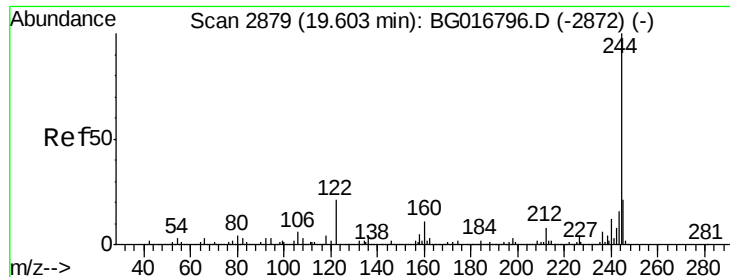

#78

Terphenyl-d14

Concen: 75.87 ng

RT: 19.36 min Scan# 2837

Delta R.T. -0.00 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38

Instrument :

BNA_G

ClientSampleId :

FYMW-04


Tot Ion:244 Resp: 824023

Ion Ratio Lower Upper

244 100

212 8.1 6.4 9.6




122 19.5 16.4 24.6

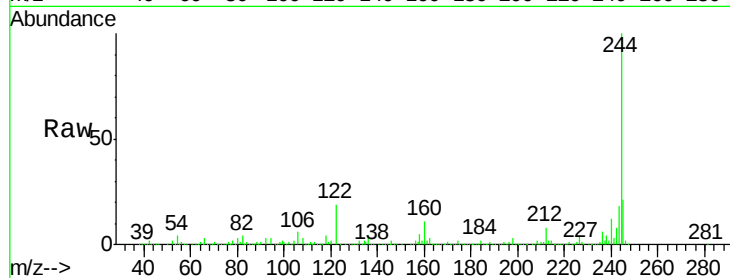

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

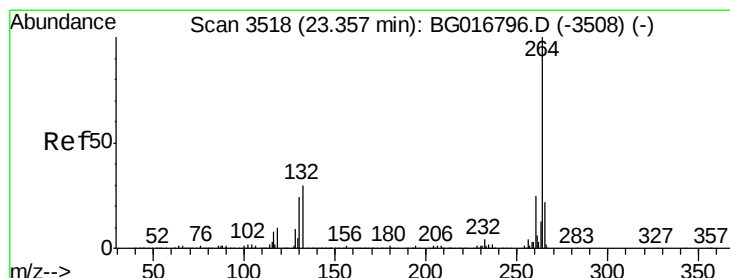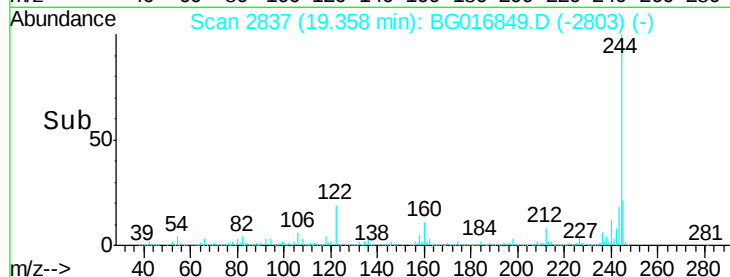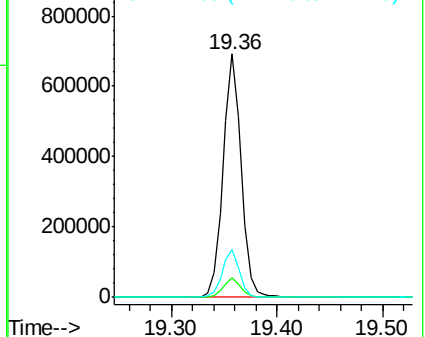

#86

Perylene-d12

Concen: 20.00 ng

RT: 22.98 min Scan# 3453

Delta R.T. -0.01 min

Lab File: BG016849.D

Acq: 1 May 2015 17:38


Tgt Ion:264 Resp: 237963

Ion Ratio Lower Upper

264 100

260 25.3 19.7 29.5

265 21.8 17.4 26.2

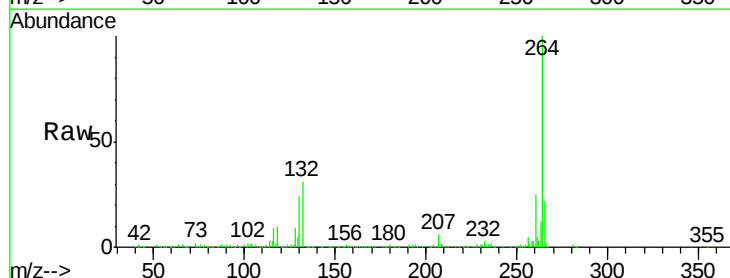

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

