

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report

(QT Reviewed)

Data File : BG026819.D

Acq On : 1 May 2017 23:09

Operator : SJ/MA

Sample : I2850-15

Misc :

ALS Vial : 17 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampled :

JHSY5

Manual Integrations

APPROVED

mohammad

5/3/2017 12:12:47 PM


Quant Time: May 02 03:23:45 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue May 02 03:22:01 2017

Response via : Initial Calibration

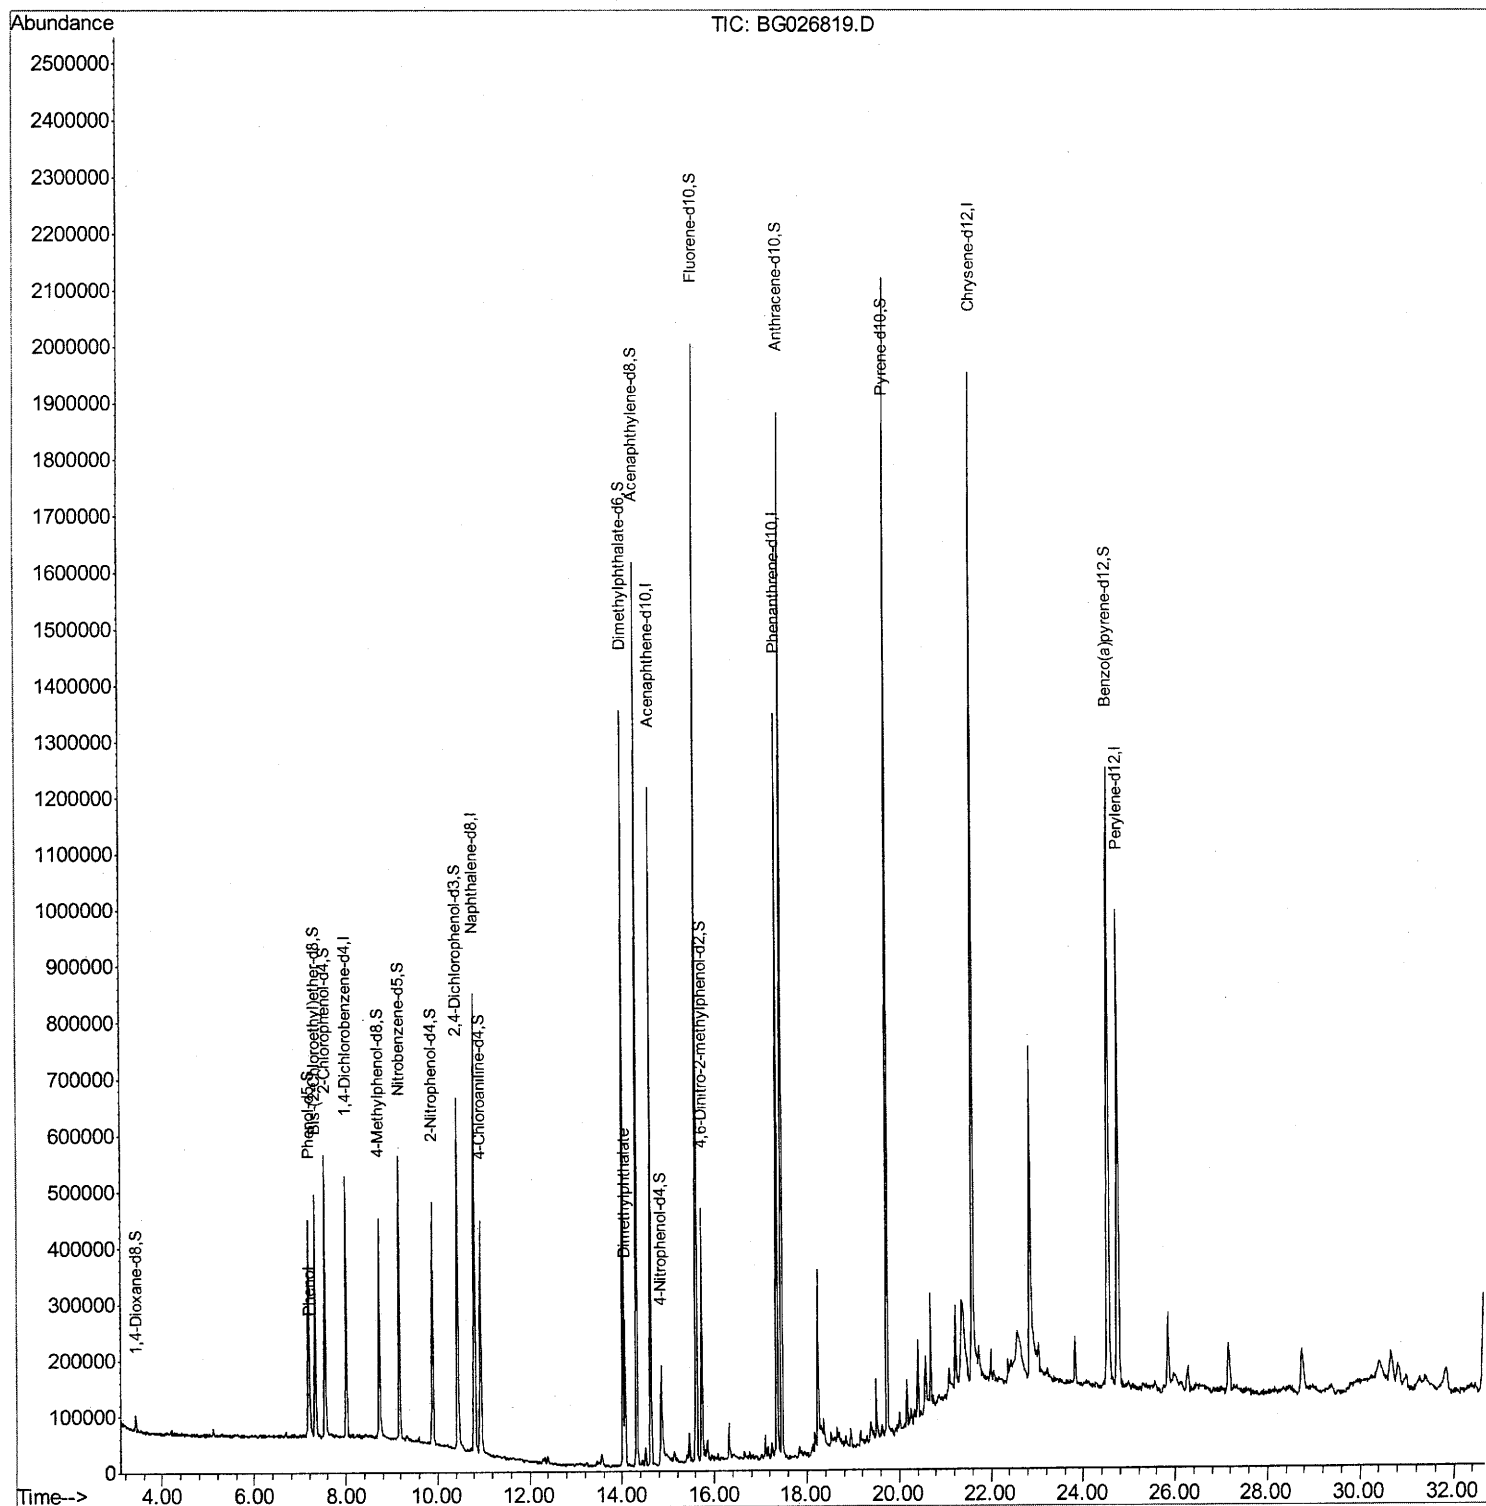

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report (Qedit)

Data File : BG026819.D

Acq On : 1 May 2017 23:09

Operator : SJ/MA

Sample : I2850-15

Misc :

ALS Vial : 17 Sample Multiplier: 1

Quant Time: May 02 03:21:59 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue May 02 03:22:01 2017

Response via : Initial Calibration

Instrument :




BNA_G

ClientSampleId :

JHSY5

Manual Integrations
APPROVED

mohammad
5/3/2017 12:12:47 PM

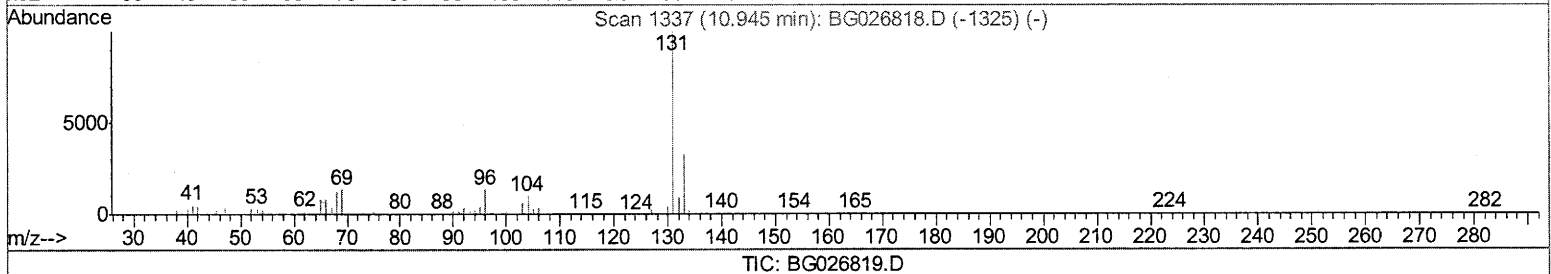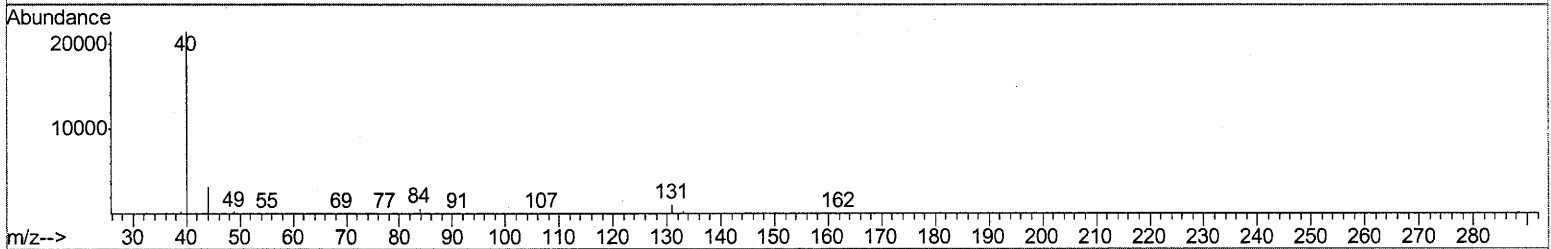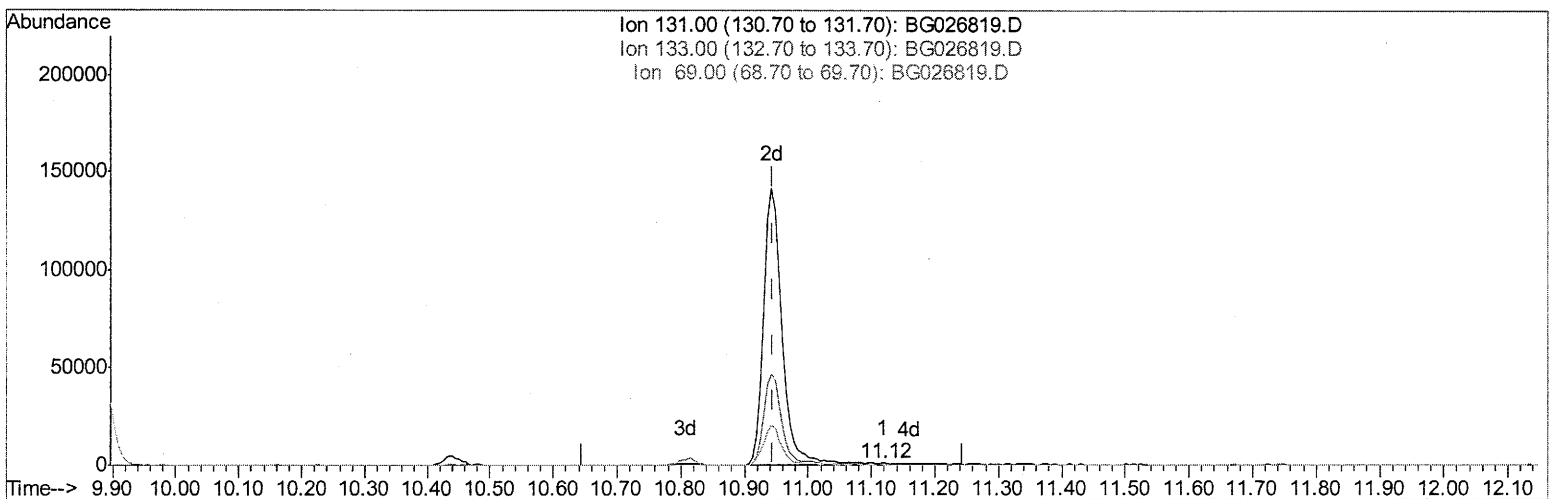

(29) 4-Chloroaniline-d4 (S)

11.119min (+0.174) 0.02ng/ul

response 323

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	35.46
69.00	23.80	22.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report (Qedit)

Data File : BG026819.D

Acq On : 1 May 2017 23:09

Operator : SJ/MA

Sample : I2850-15

Misc :

ALS Vial : 17 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

JHSY5

Manual Integrations
APPROVED

mohammad

5/3/2017 12:12:47 PM




Quant Time: May 02 03:21:59 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue May 02 03:22:01 2017

Response via : Initial Calibration

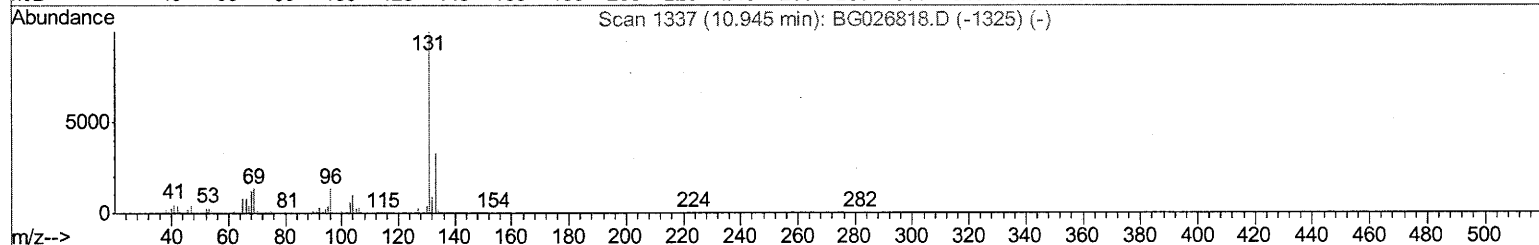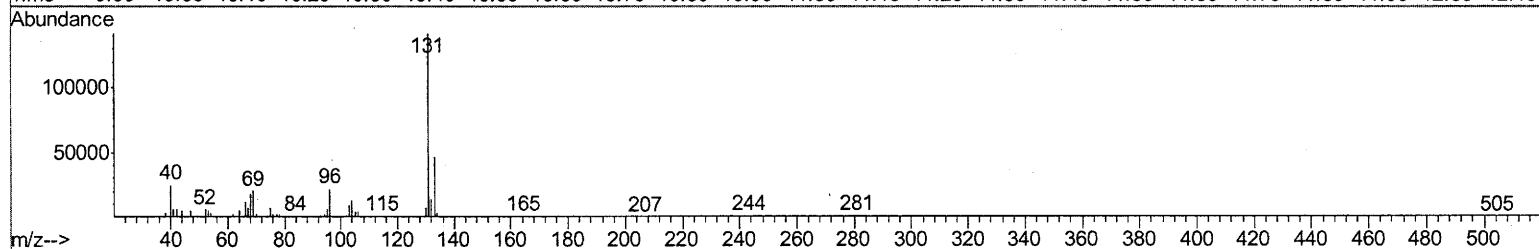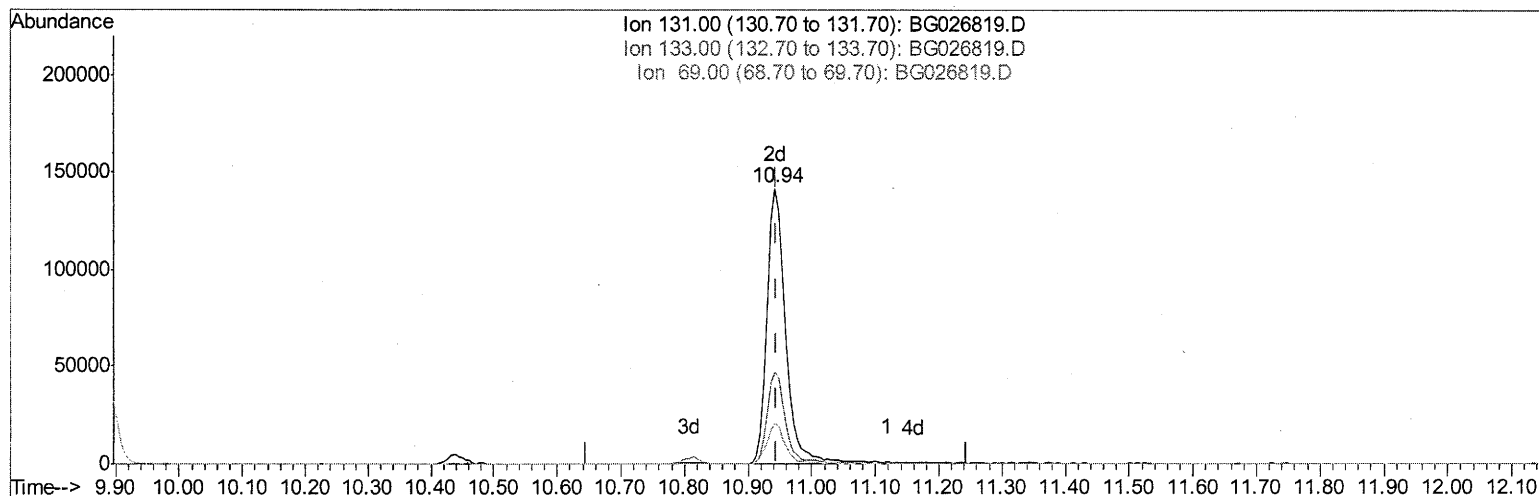

TIC: BG026819.D

(29) 4-Chloroaniline-d4 (S)

10.943min (-0.003) 20.52ng/ul m

SJ 5/5/17

response 291183

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	33.30
69.00	23.80	14.36#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\
Quantitation Report (QT Reviewed)

Data File : BG026819.D
Acq On : 1 May 2017 23:09
Operator : SJ/MA
Sample : I2850-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
JHSY5

Manual Integrations
APPROVED

mohammad
5/3/2017 12:12:47 PM

Quant Time: May 02 03:23:45 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 02 03:22:01 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	141933	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	733853	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	409453	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	767757	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	702273	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	730785	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	14007	4.44	ng/uL	0.00
5) Phenol-d5	7.19	99	292552	23.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	212649	28.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	273100	25.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	198828	18.91	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	159162	25.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	174180	26.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	278115	26.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	291183m	20.52	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	928612	28.18	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1195117	28.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	93103	15.67	ng/ul	0.00
57) Fluorene-d10	15.61	176	786727	27.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	101506	21.77	ng/ul	0.00
70) Anthracene-d10	17.45	188	1061542	28.49	ng/ul	0.00
76) Pyrene-d10	19.73	212	1043381	28.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1002474	29.01	ng/ul	0.00

SJ 5/5/17

Target Compounds

						Qvalue
6) Phenol	7.22	94	25819	2.01	ng/ul#	80
44) Dimethylphthalate	14.07	163	174146	5.40	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed