


Data File : BG026835.D
Acq On : 2 May 2017 9:37
Operator : SJ/MA
Sample : I2867-12
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
JHT77

Manual Integrations
APPROVED

mohammad
5/3/2017 12:13:08 PM

Quant Time: May 03 01:01:39 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 03 00:58:45 2017
Response via : Initial Calibration

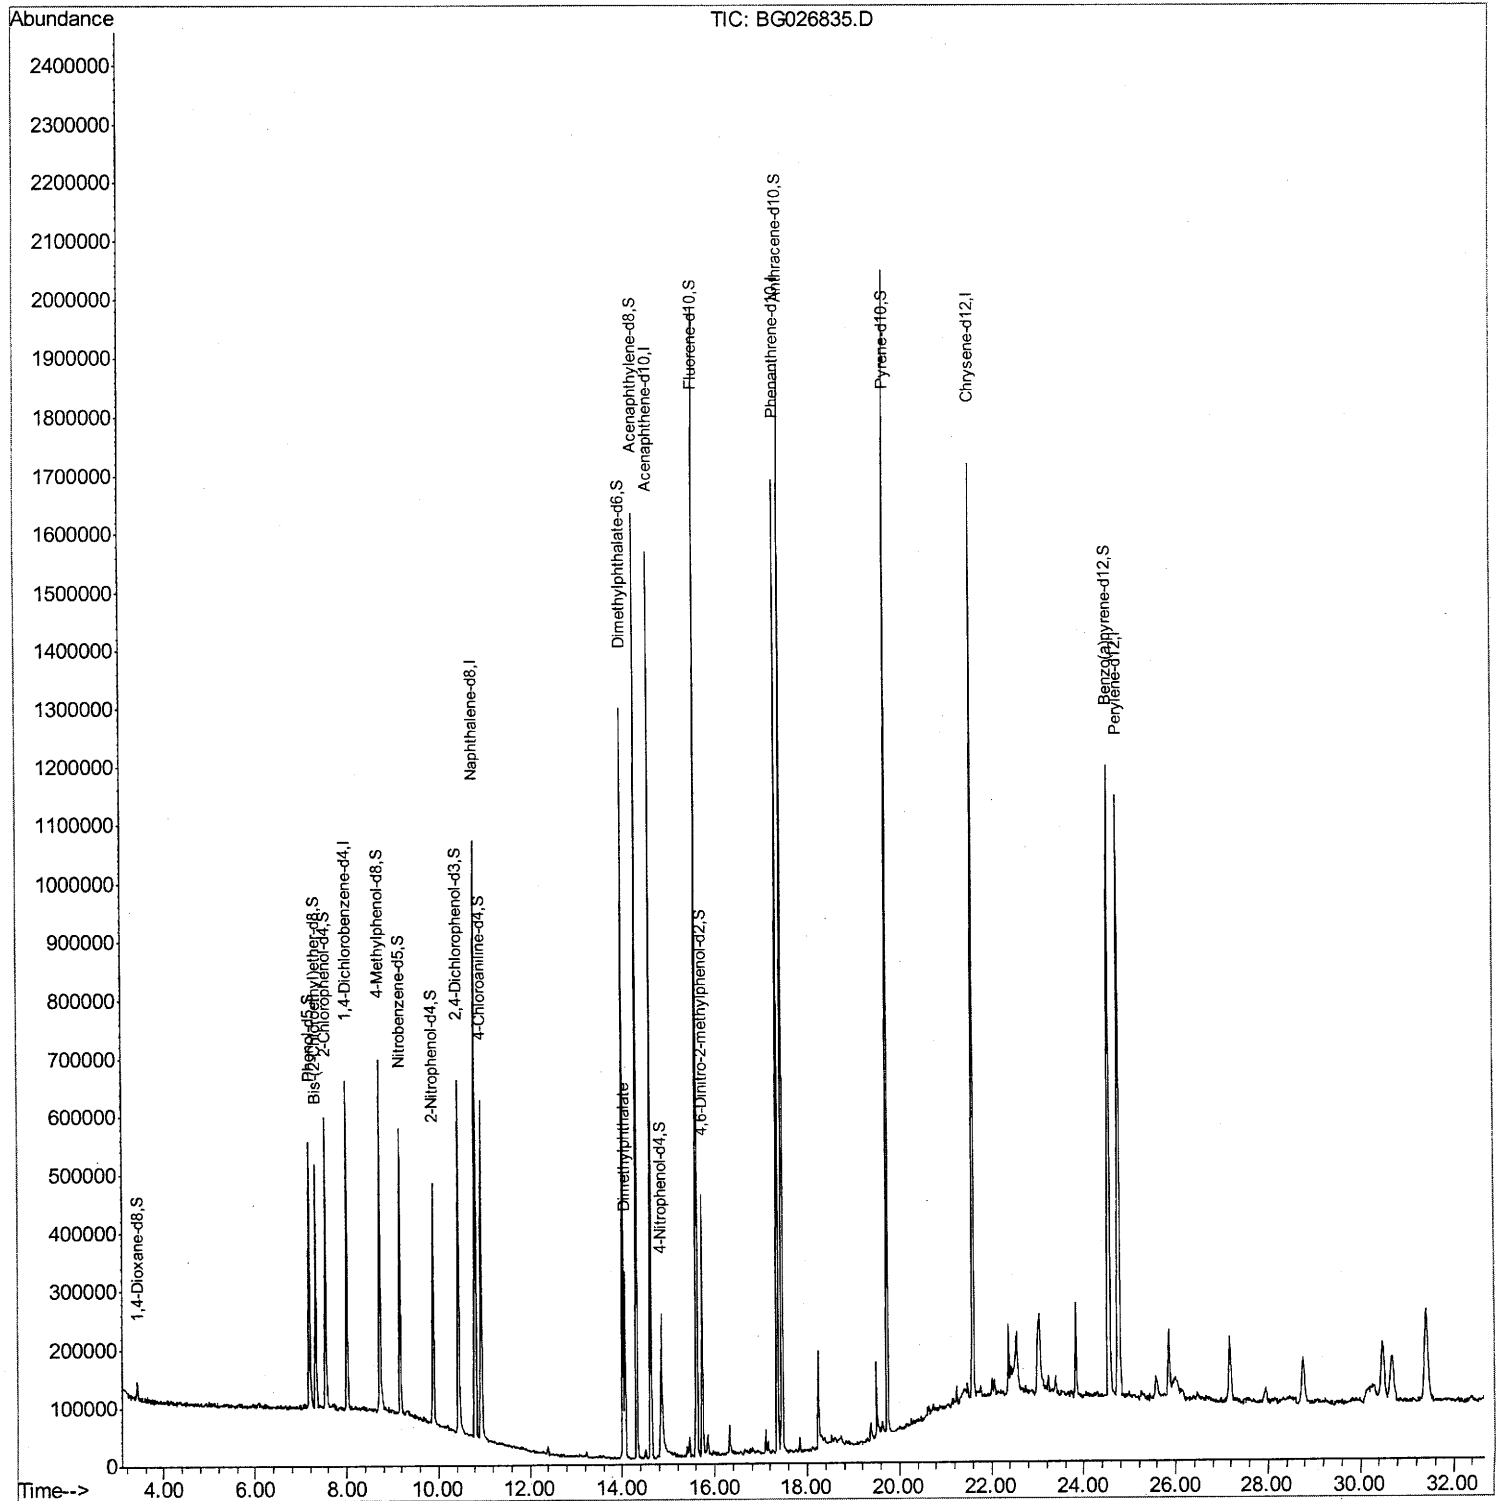

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report (Qedit)

Data File : BG026835.D

Acq On : 2 May 2017 9:37

Operator : SJ/MA

Sample : I2867-12

Misc :

ALS Vial : 33 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampled :

JHT77

Manual Integrations
APPROVED

mohammad
5/3/2017 12:13:08 PM




Quant Time: May 03 00:58:41 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 03 00:58:45 2017

Response via : Initial Calibration

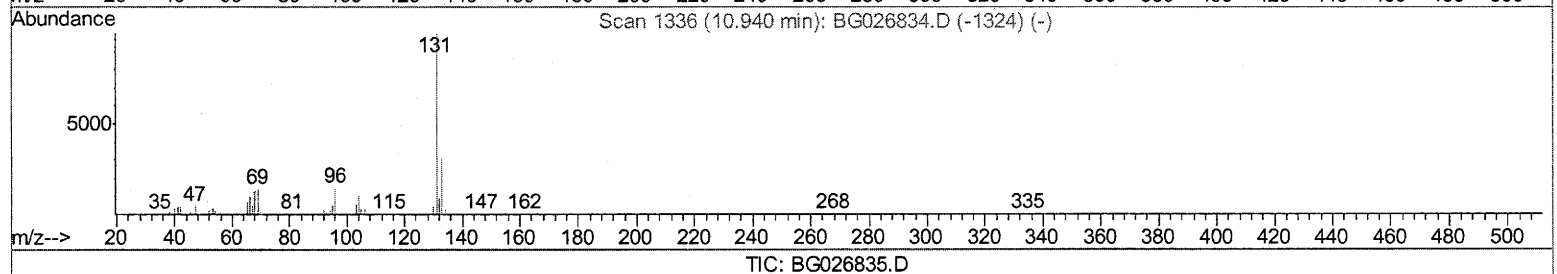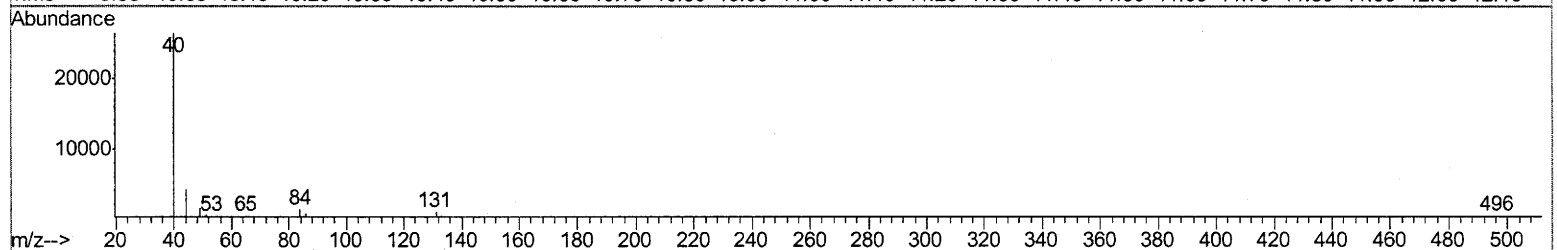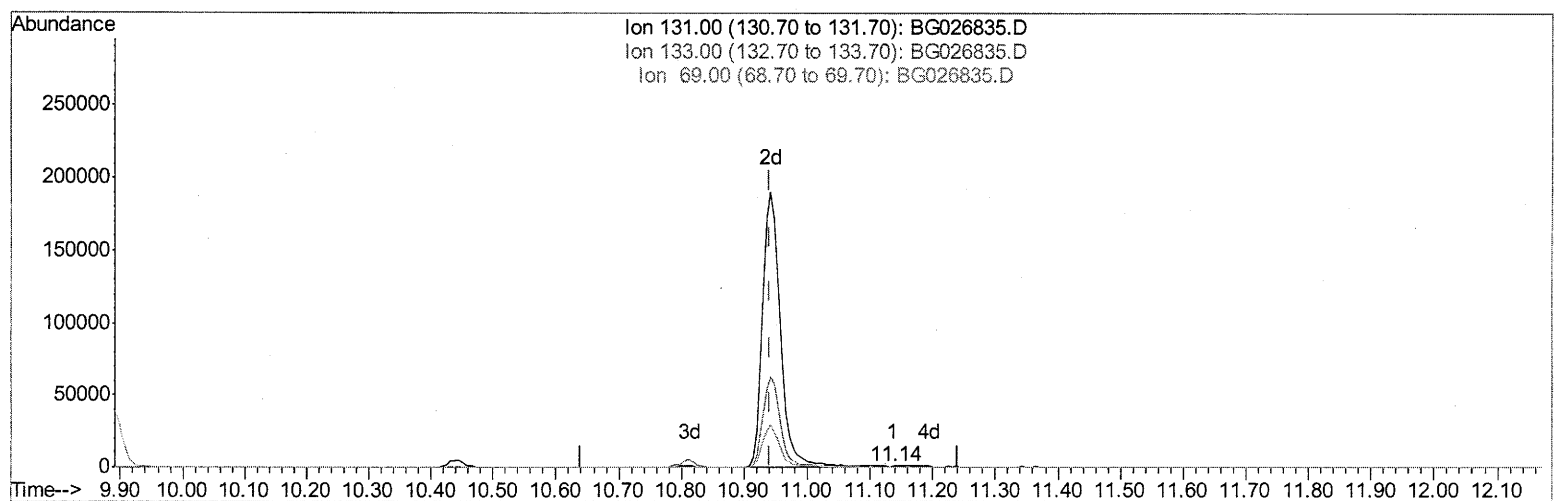

(29) 4-Chloroaniline-d4 (S)

11.137min (+0.196) 0.04ng/ul

response 699

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	31.95
69.00	23.80	20.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report (Qedit)

Data File : BG026835.D

Acq On : 2 May 2017 9:37

Operator : SJ/MA

Sample : I2867-12

Misc :

ALS Vial : 33 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

JHT77

Manual Integrations
APPROVED

mohammad

5/3/2017 12:13:08 PM




Quant Time: May 03 00:58:41 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 03 00:58:45 2017

Response via : Initial Calibration

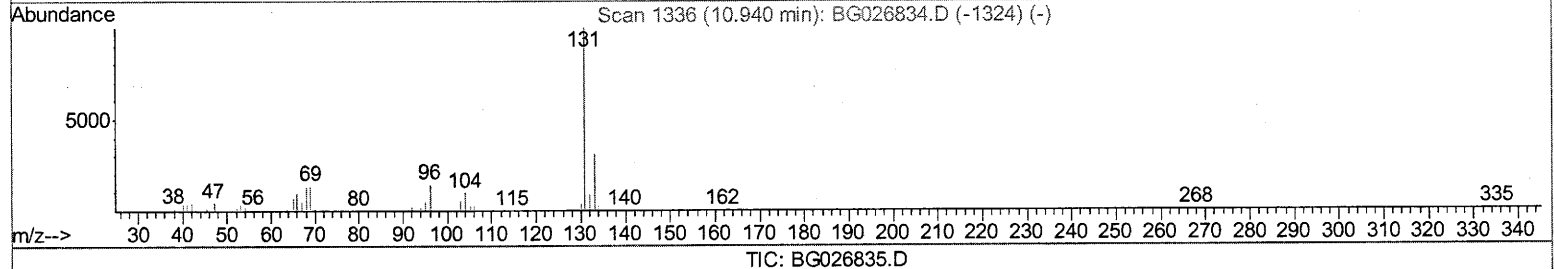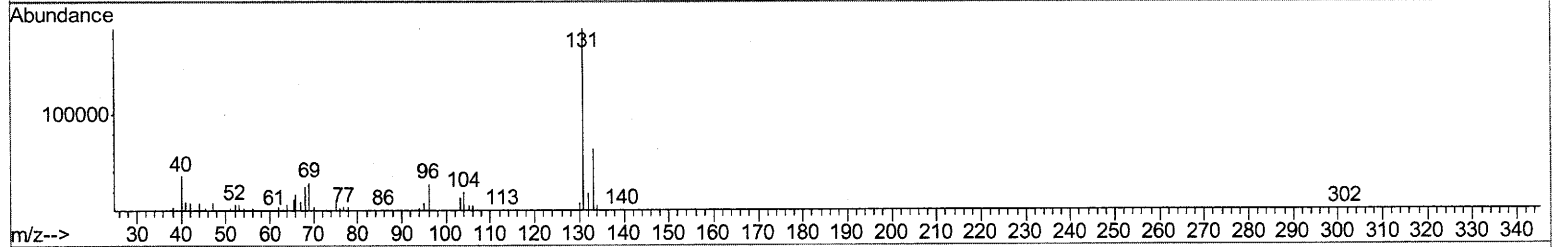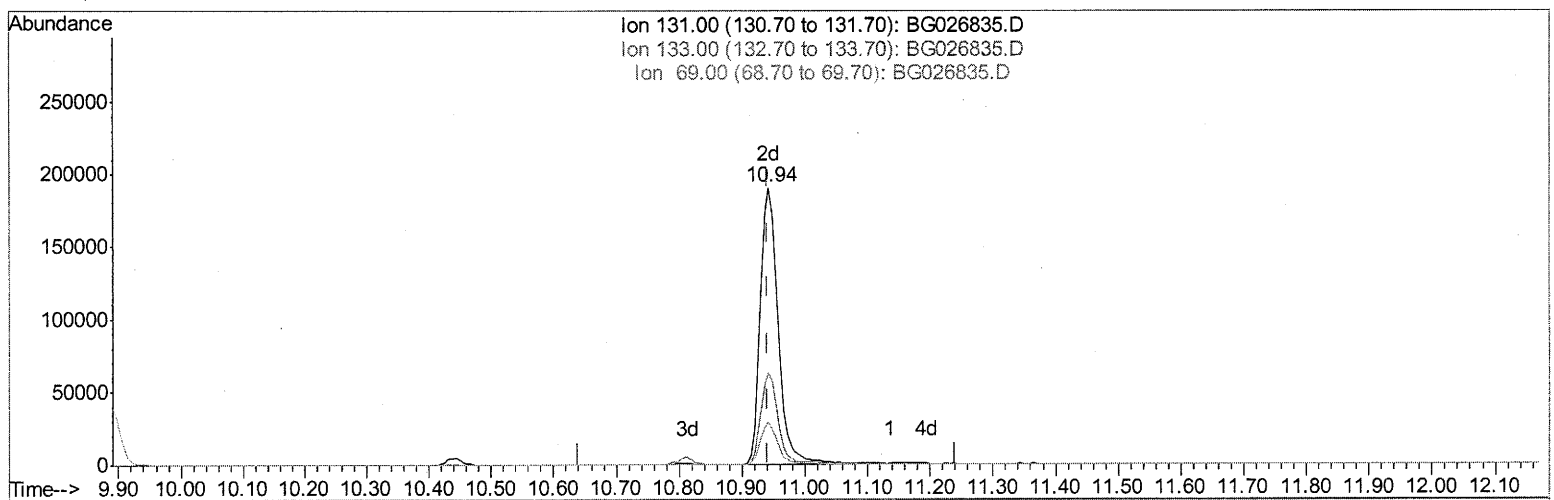

(29) 4-Chloroaniline-d4 (S)

10.943min (+0.003) 21.72ng/ul m

SJ 5/5/17

response 377789

Ion	Exp%	Act%
131.00	100	100
133.00	35.40	33.33
69.00	23.80	15.39#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050117\

Quantitation Report (QT Reviewed)

Data File : BG026835.D

Acq On : 2 May 2017 9:37

Operator : SJ/MA

Sample : I2867-12

Misc :

ALS Vial : 33 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampled :

JHT77

Manual Integrations
APPROVED

mohammad
5/3/2017 12:13:08 PM

Quant Time: May 03 01:01:39 2017

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed May 03 00:58:45 2017

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	164719	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	899359	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	520452	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.36	188	976951	20.00	ng/ul	0.00
75) Chrysene-d12	21.61	240	880781	20.00	ng/ul	0.00
83) Perylene-d12	24.77	264	921862	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	13978	3.82	ng/uL	0.00
5) Phenol-d5	7.19	99	344103	23.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	208640	24.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	268910	21.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	290186	23.78	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	152624	20.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	163010	19.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	267792	20.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	377789m	21.72	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	909560	21.71	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1162006	22.08	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	120257	15.93	ng/ul	0.00
57) Fluorene-d10	15.61	176	768794	21.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	97981	16.52	ng/ul	0.00
70) Anthracene-d10	17.45	188	1047282	22.09	ng/ul	0.00
76) Pyrene-d10	19.73	212	1005812	21.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	906850	20.81	ng/ul	0.00

SJ 5/5/17

Target Compounds					Qvalue
44) Dimethylphthalate	14.07	163	211753	5.16	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed