
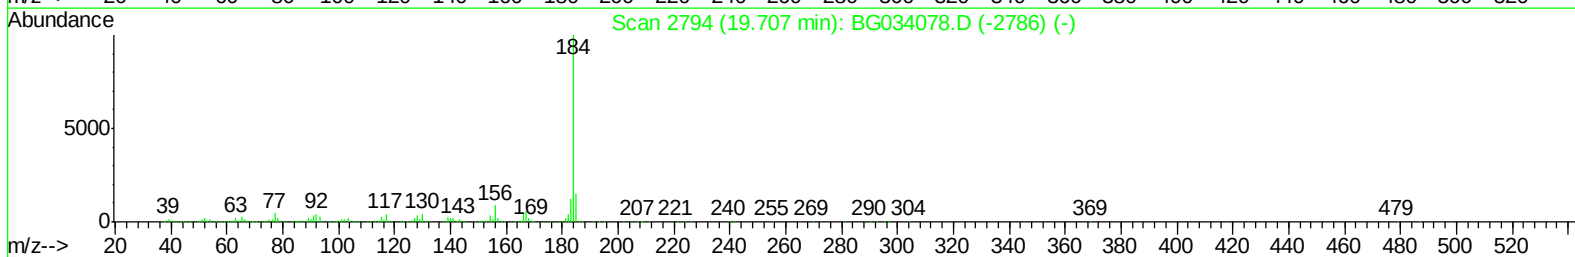
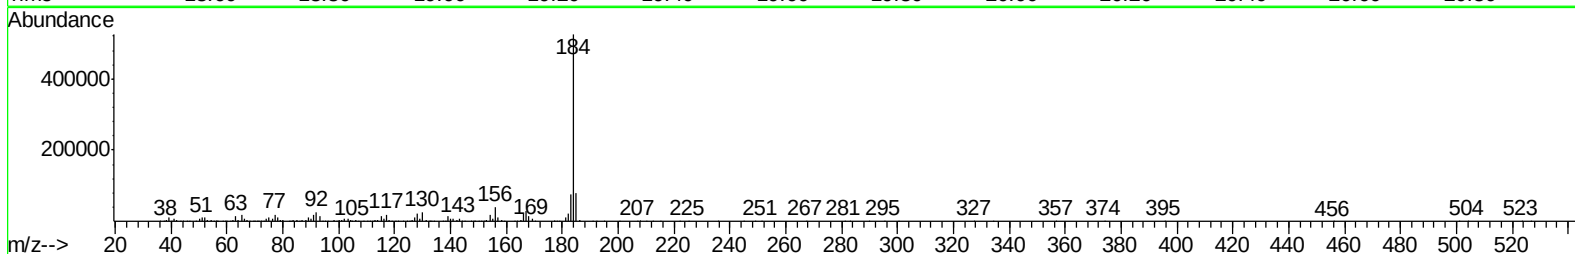


Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034074.D
Acq On : 1 May 2018 11:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:21:04 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

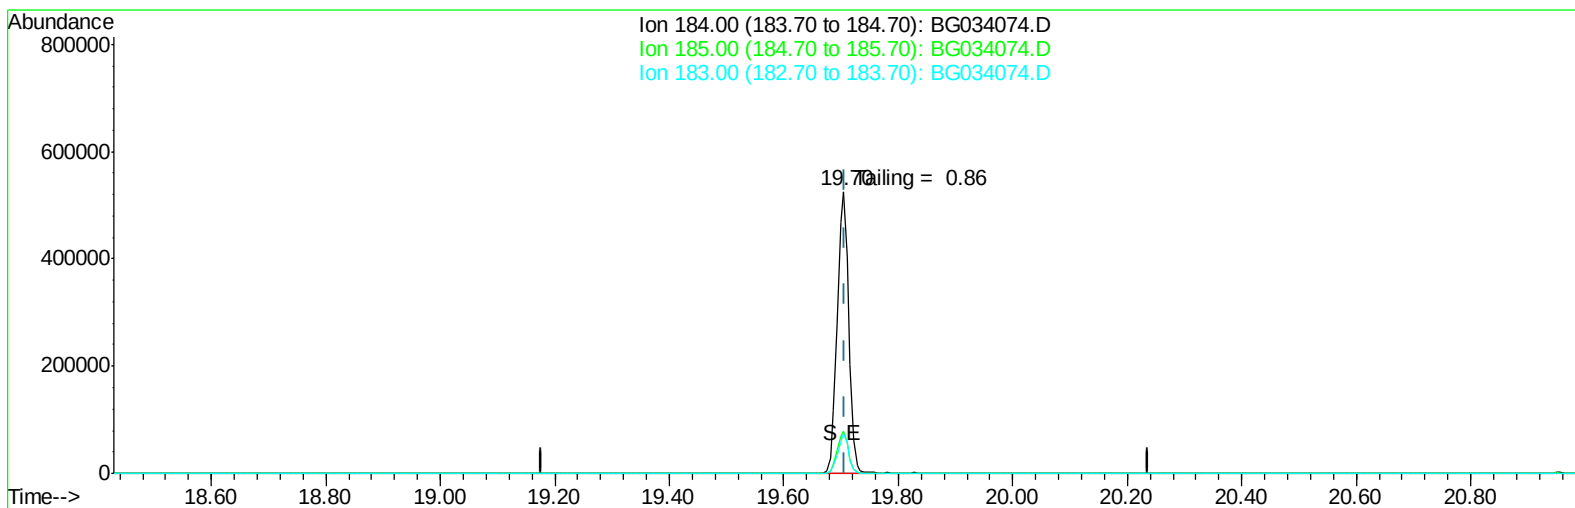

TIC: BG034074.D

(76) Benzidine




19.704min (-0.003) 498528.18ng

response 744814

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.99
183.00	13.30	14.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034074.D
Acq On : 1 May 2018 11:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:21:04 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

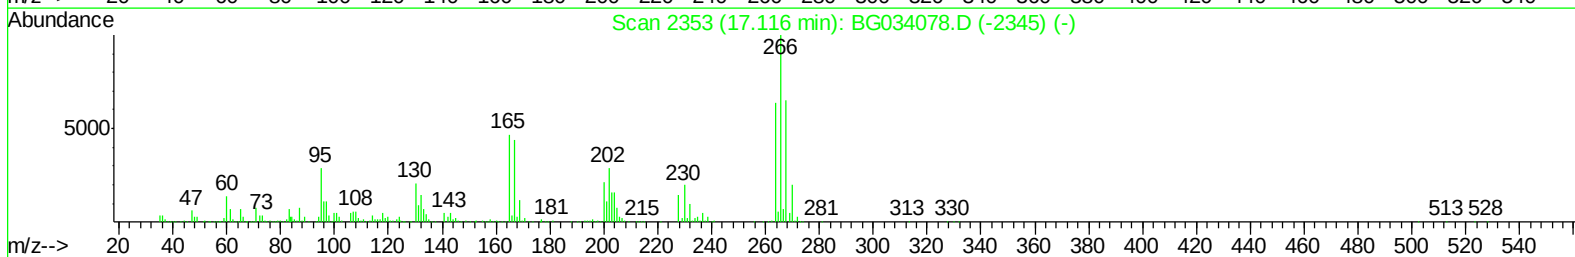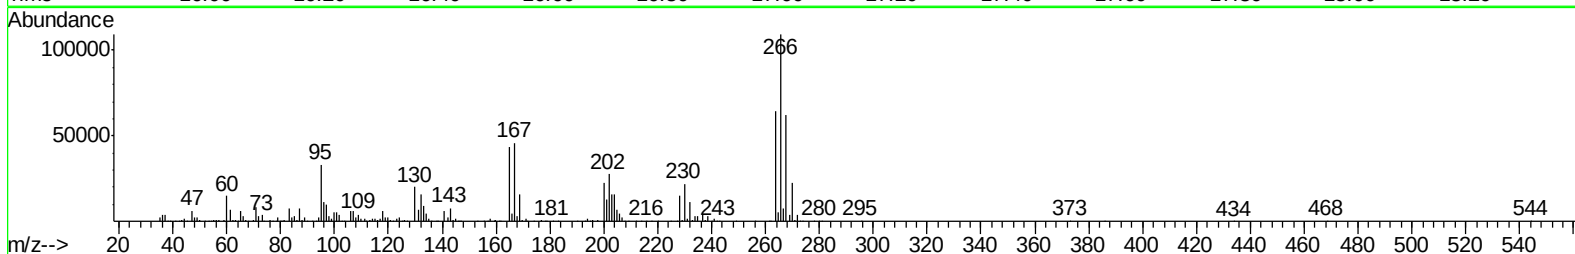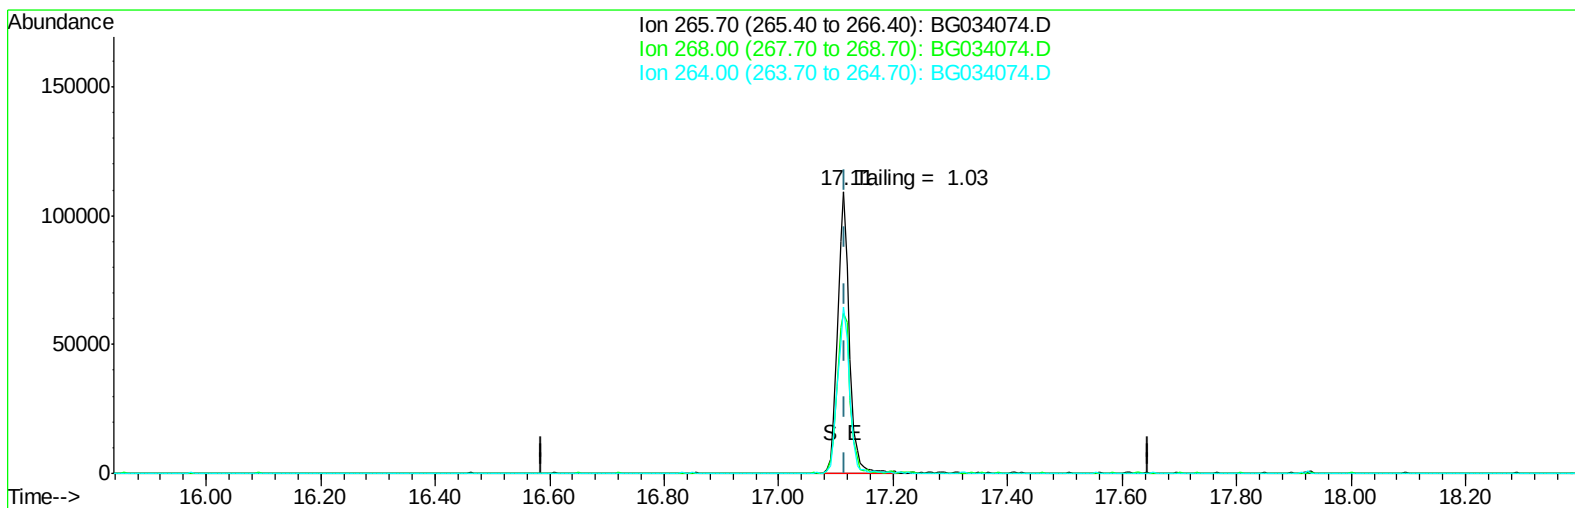

TIC: BG034074.D

(69) Pentachlorophenol (C)

17.113min (-0.003) 118720.34ng

response 155387

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	56.69
264.00	62.00	59.06
0.00	0.00	0.00