
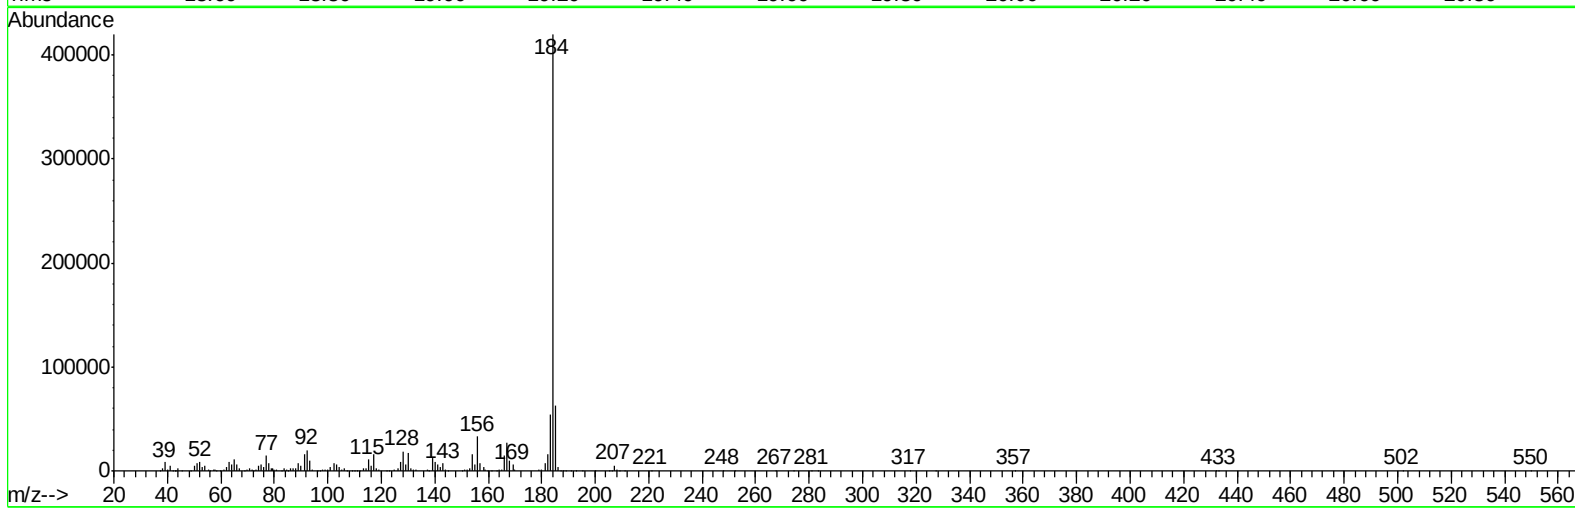


Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034083.D
Acq On : 1 May 2018 17:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:23:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

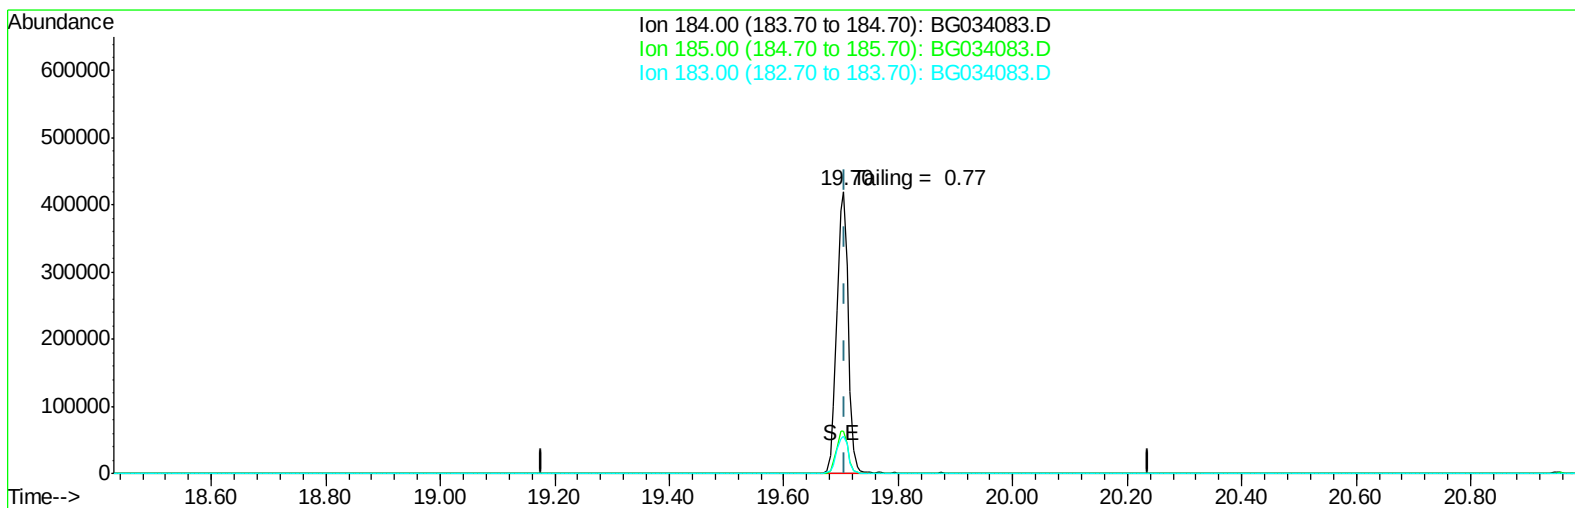

TIC: BG034083.D

(76) Benzidine



19.705min (-0.003) 332287.67ng

response 590600

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.04
183.00	13.30	13.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034083.D
Acq On : 1 May 2018 17:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:23:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

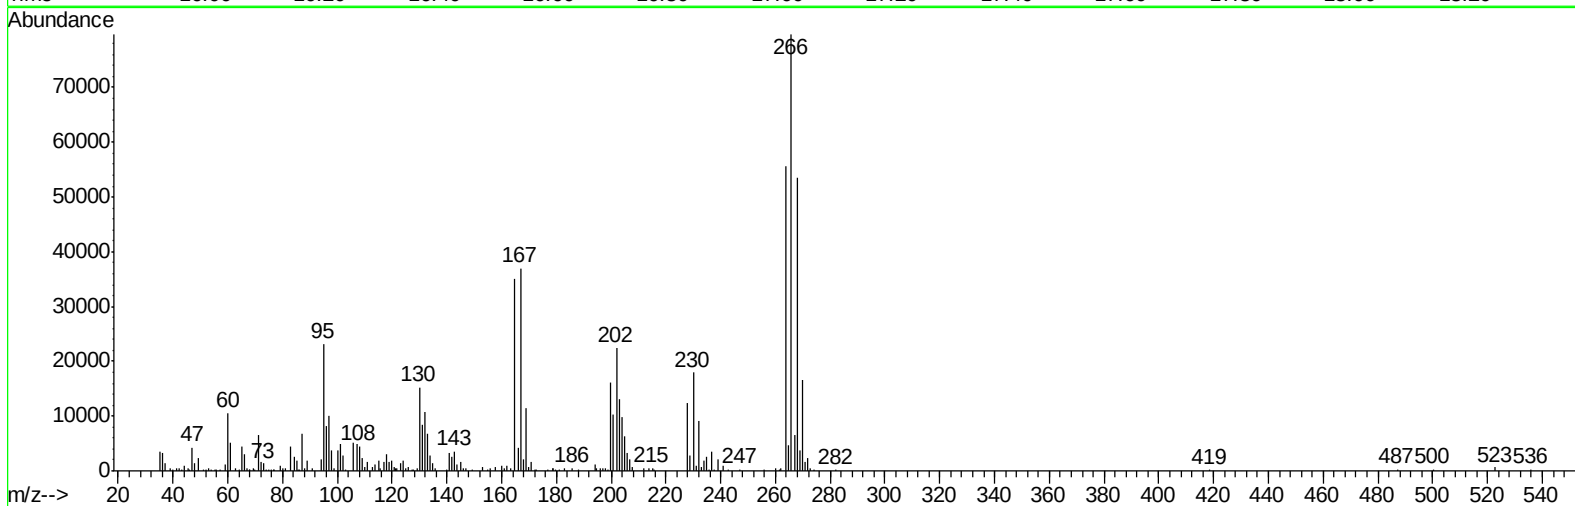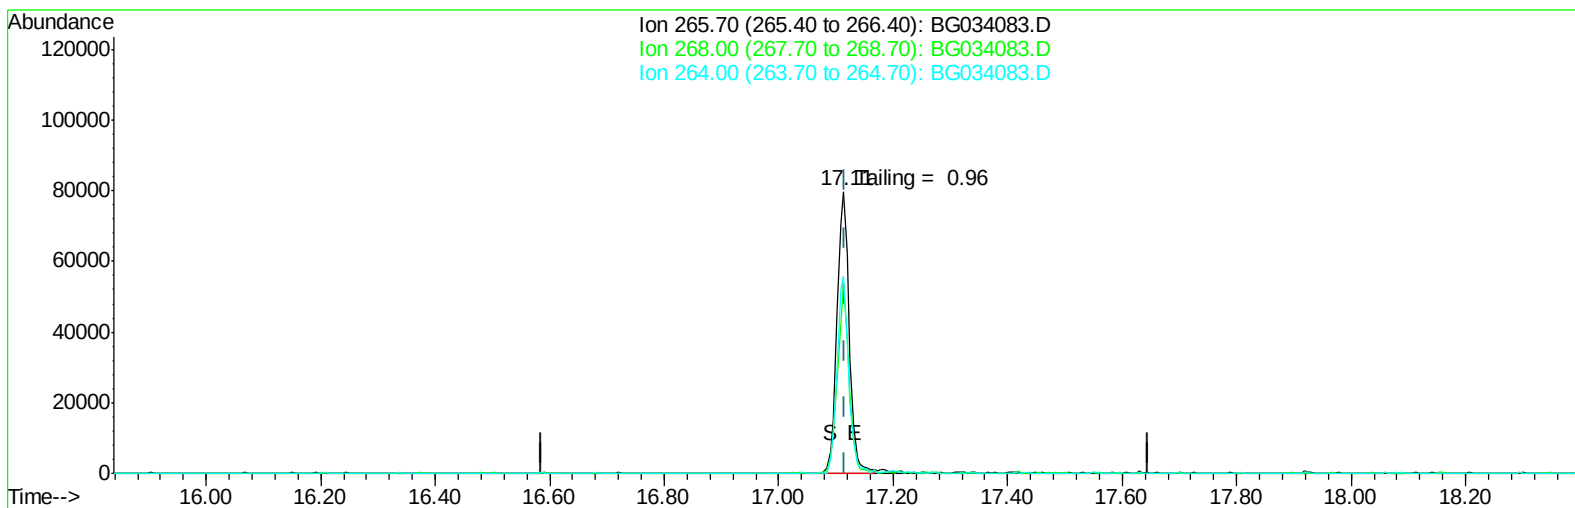

TIC: BG034083.D

(69) Pentachlorophenol (C)

17.114min (-0.003) 100526.13ng

response 120977

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.11
264.00	62.00	69.91
0.00	0.00	0.00