
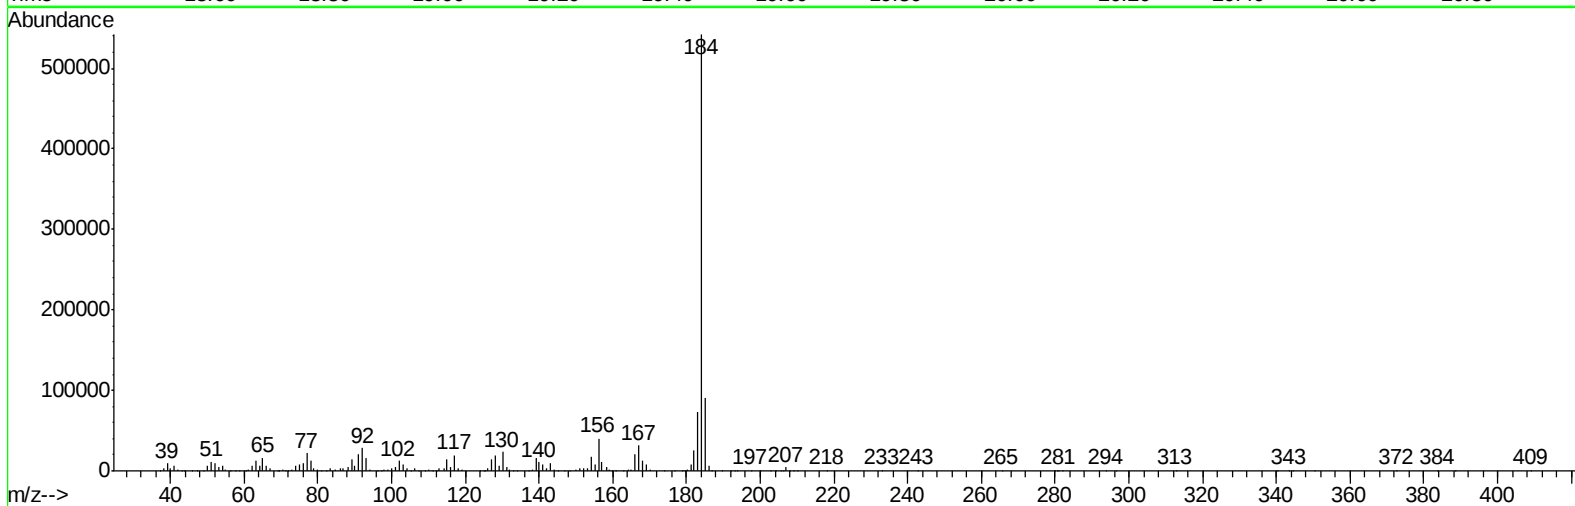


Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034102.D
Acq On : 2 May 2018 6:02
Operator : SJ/JU
Sample : DFTPP
Misc : 20PPM L00
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:24:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

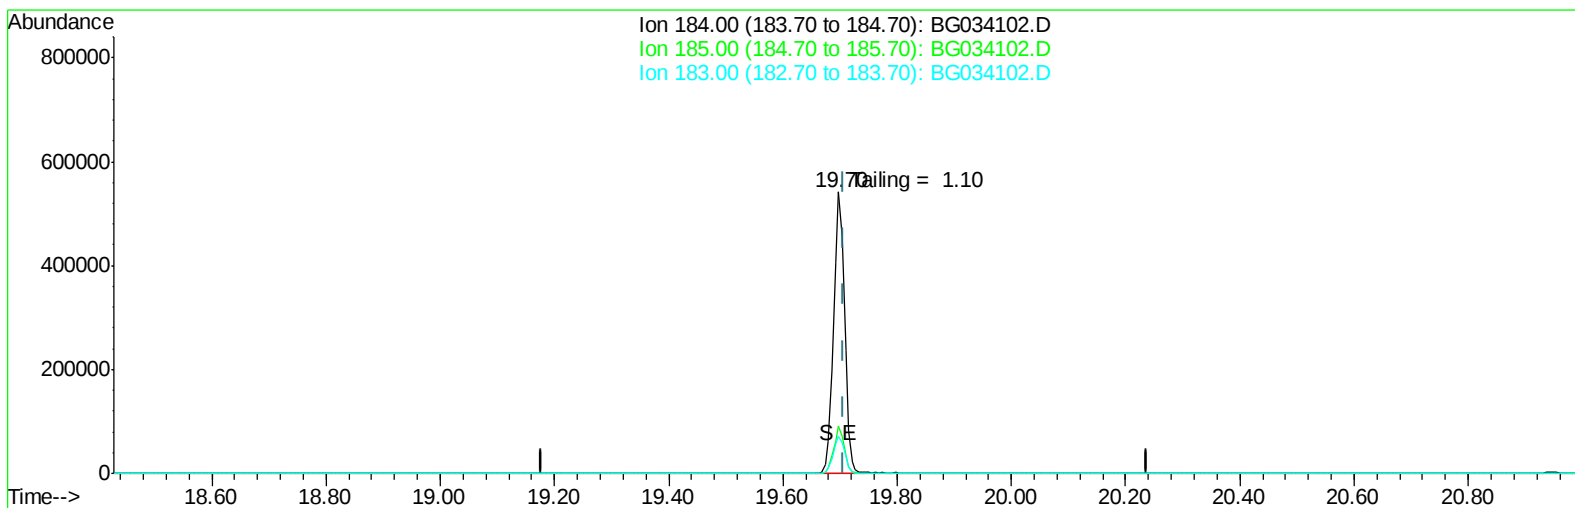

TIC: BG034102.D

(76) Benzidine



19.698min (-0.010) 392310.93ng

response 717495

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.78#
183.00	13.30	13.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG050118\
Data File : BG034102.D
Acq On : 2 May 2018 6:02
Operator : SJ/JU
Sample : DFTPP
Misc : 20PPM L00
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:24:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

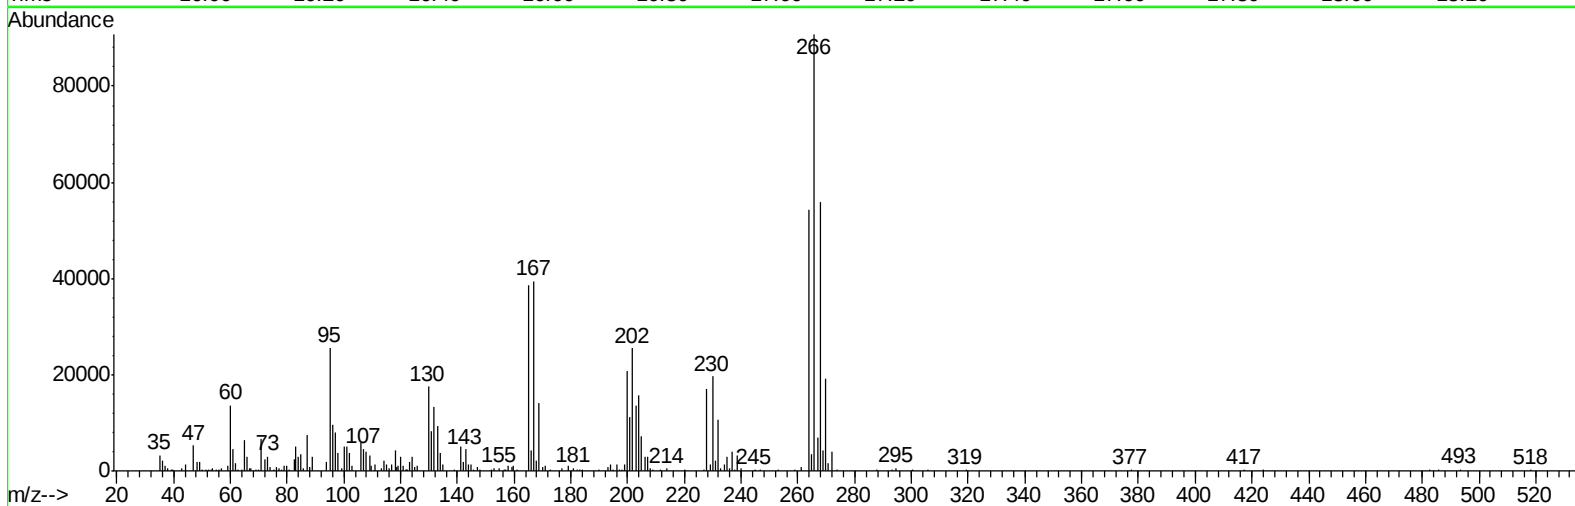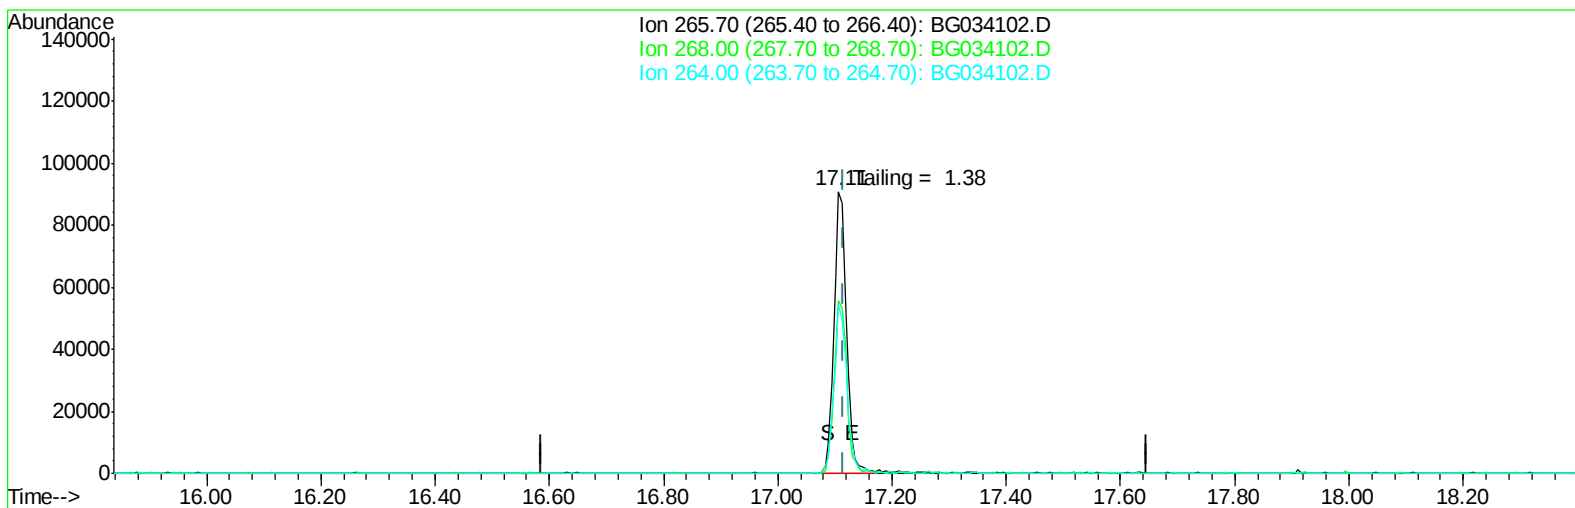

TIC: BG034102.D

(69) Pentachlorophenol (C)

17.107min (-0.010) 255771.56ng

response 137052

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.57
264.00	62.00	59.93
0.00	0.00	0.00