


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050118\
 Data File : BG034074.D
 Acq On : 1 May 2018 11:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 19:08:03 2018

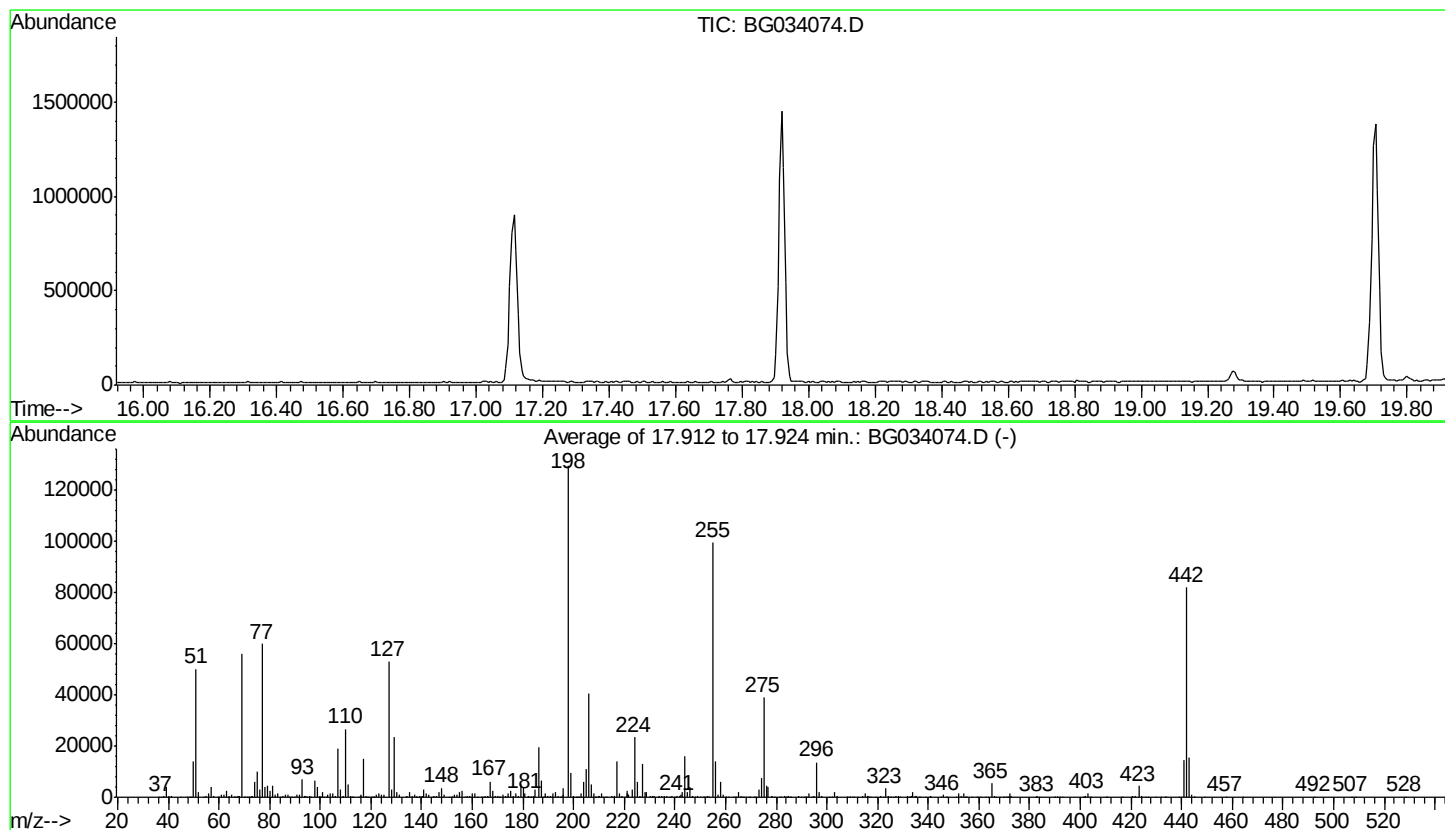

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	50280	PASS
68	69	0.00	2	1.2	667	PASS
69	198	0.00	100	43.1	55961	PASS
70	69	0.00	2	0.4	219	PASS
127	198	10	80	40.9	53002	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129746	PASS
199	198	5	9	7.4	9567	PASS
275	198	10	60	30.1	39005	PASS
365	198	1	100	4.2	5416	PASS
441	443	0.01	100	92.6	14326	PASS
442	198	50	100	63.2	81965	PASS
443	442	15	24	18.9	15476	PASS