


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050118\
Data File : BG034083.D
Acq On : 1 May 2018 17:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 01 19:08:03 2018

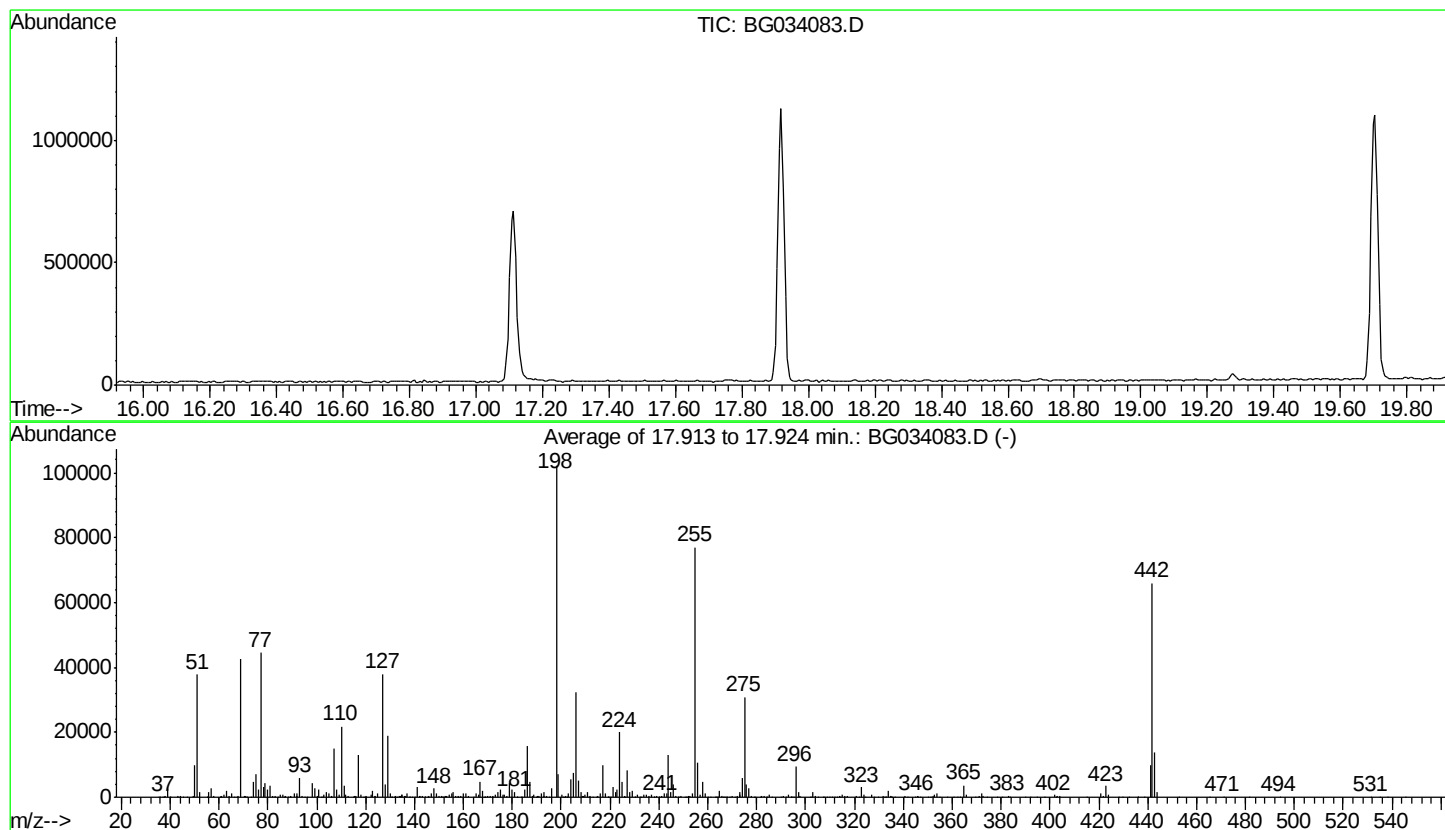

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	37734	PASS
68	69	0.00	2	0.9	369	PASS
69	198	0.00	100	41.7	42610	PASS
70	69	0.00	2	1.0	447	PASS
127	198	10	80	37.2	38045	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102192	PASS
199	198	5	9	7.1	7282	PASS
275	198	10	60	30.1	30808	PASS
365	198	1	100	3.6	3667	PASS
441	443	0.01	100	72.3	10055	PASS
442	198	50	100	64.6	66029	PASS
443	442	15	24	21.1	13909	PASS