


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050118\
 Data File : BG034102.D
 Acq On : 2 May 2018 6:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc : 20PPM LOQ
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 19:08:03 2018

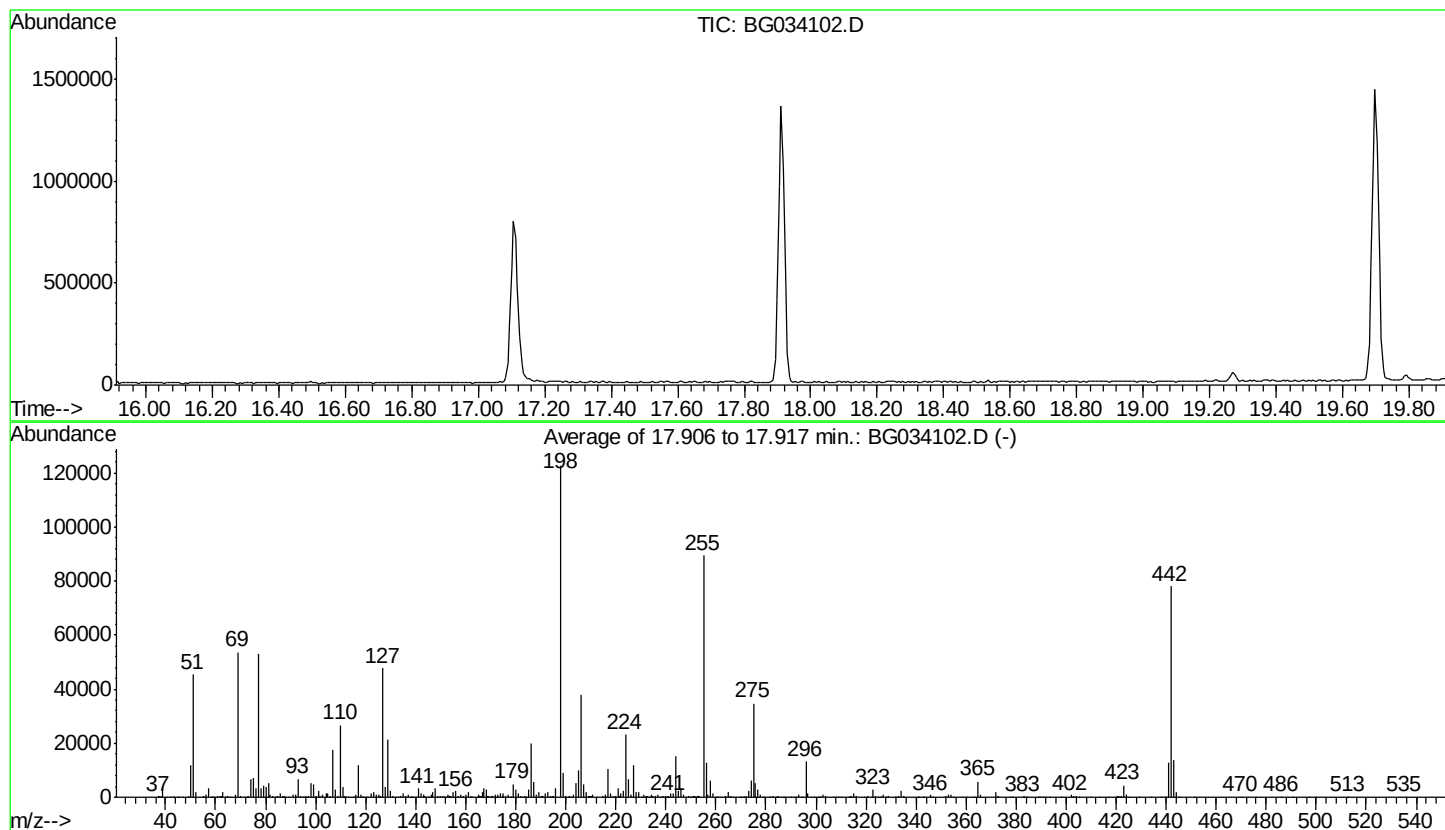

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	45465	PASS
68	69	0.00	2	1.7	892	PASS
69	198	0.00	100	43.6	53533	PASS
70	69	0.00	2	0.8	425	PASS
127	198	10	80	39.0	47802	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	122688	PASS
199	198	5	9	7.4	9028	PASS
275	198	10	60	28.4	34794	PASS
365	198	1	100	4.8	5912	PASS
441	443	0.01	100	94.2	12927	PASS
442	198	50	100	63.5	77962	PASS
443	442	15	24	17.6	13726	PASS