

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050124\
 Data File : BG061071.D
 Acq On : 1 May 2024 11:06
 Operator : MA/JU
 Sample : PB160621BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: May 01 12:38:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 05:11:25 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.956	152	17015	20.000	ng	# 0.00
21) Naphthalene-d8	10.753	136	65232	20.000	ng	# 0.00
39) Acenaphthene-d10	14.584	164	59974	20.000	ng	0.00
64) Phenanthrene-d10	17.328	188	174465	20.000	ng	0.00
76) Chrysene-d12	21.581	240	213390	20.000	ng	-0.01
86) Perylene-d12	24.713	264	238983	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.547	112	132092	157.884	ng	0.00
7) Phenol-d6	7.134	99	179041	144.662	ng	0.00
23) Nitrobenzene-d5	9.114	82	122675	93.225	ng	0.00
42) 2,4,6-Tribromophenol	16.070	330	177080	147.717	ng	0.00
45) 2-Fluorobiphenyl	13.209	172	369889	91.200	ng	0.00
79) Terphenyl-d14	19.948	244	1219937	95.081	ng	0.00
Target Compounds						
9) Benzaldehyde	7.134	77	351	Below Cal		Qvalue # 3
19) n-Nitroso-di-n-propyla...	9.114	70	18668	20.155	ng	# 66
51) 2,6-Dinitrotoluene	14.584	165	7250	7.317	ng	# 15
57) 2,4-Dinitrotoluene	14.584	165	7250	4.946	ng	# 17
67) 4-Bromophenyl-phenylether	16.070	248	10844	5.276	ng	# 1
77) Benzidine	19.948	184	18789	7.153	ng	# 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050124\
Data File : BG061071.D
Acq On : 1 May 2024 11:06
Operator : MA/JU
Sample : PB160621BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: May 01 12:38:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration




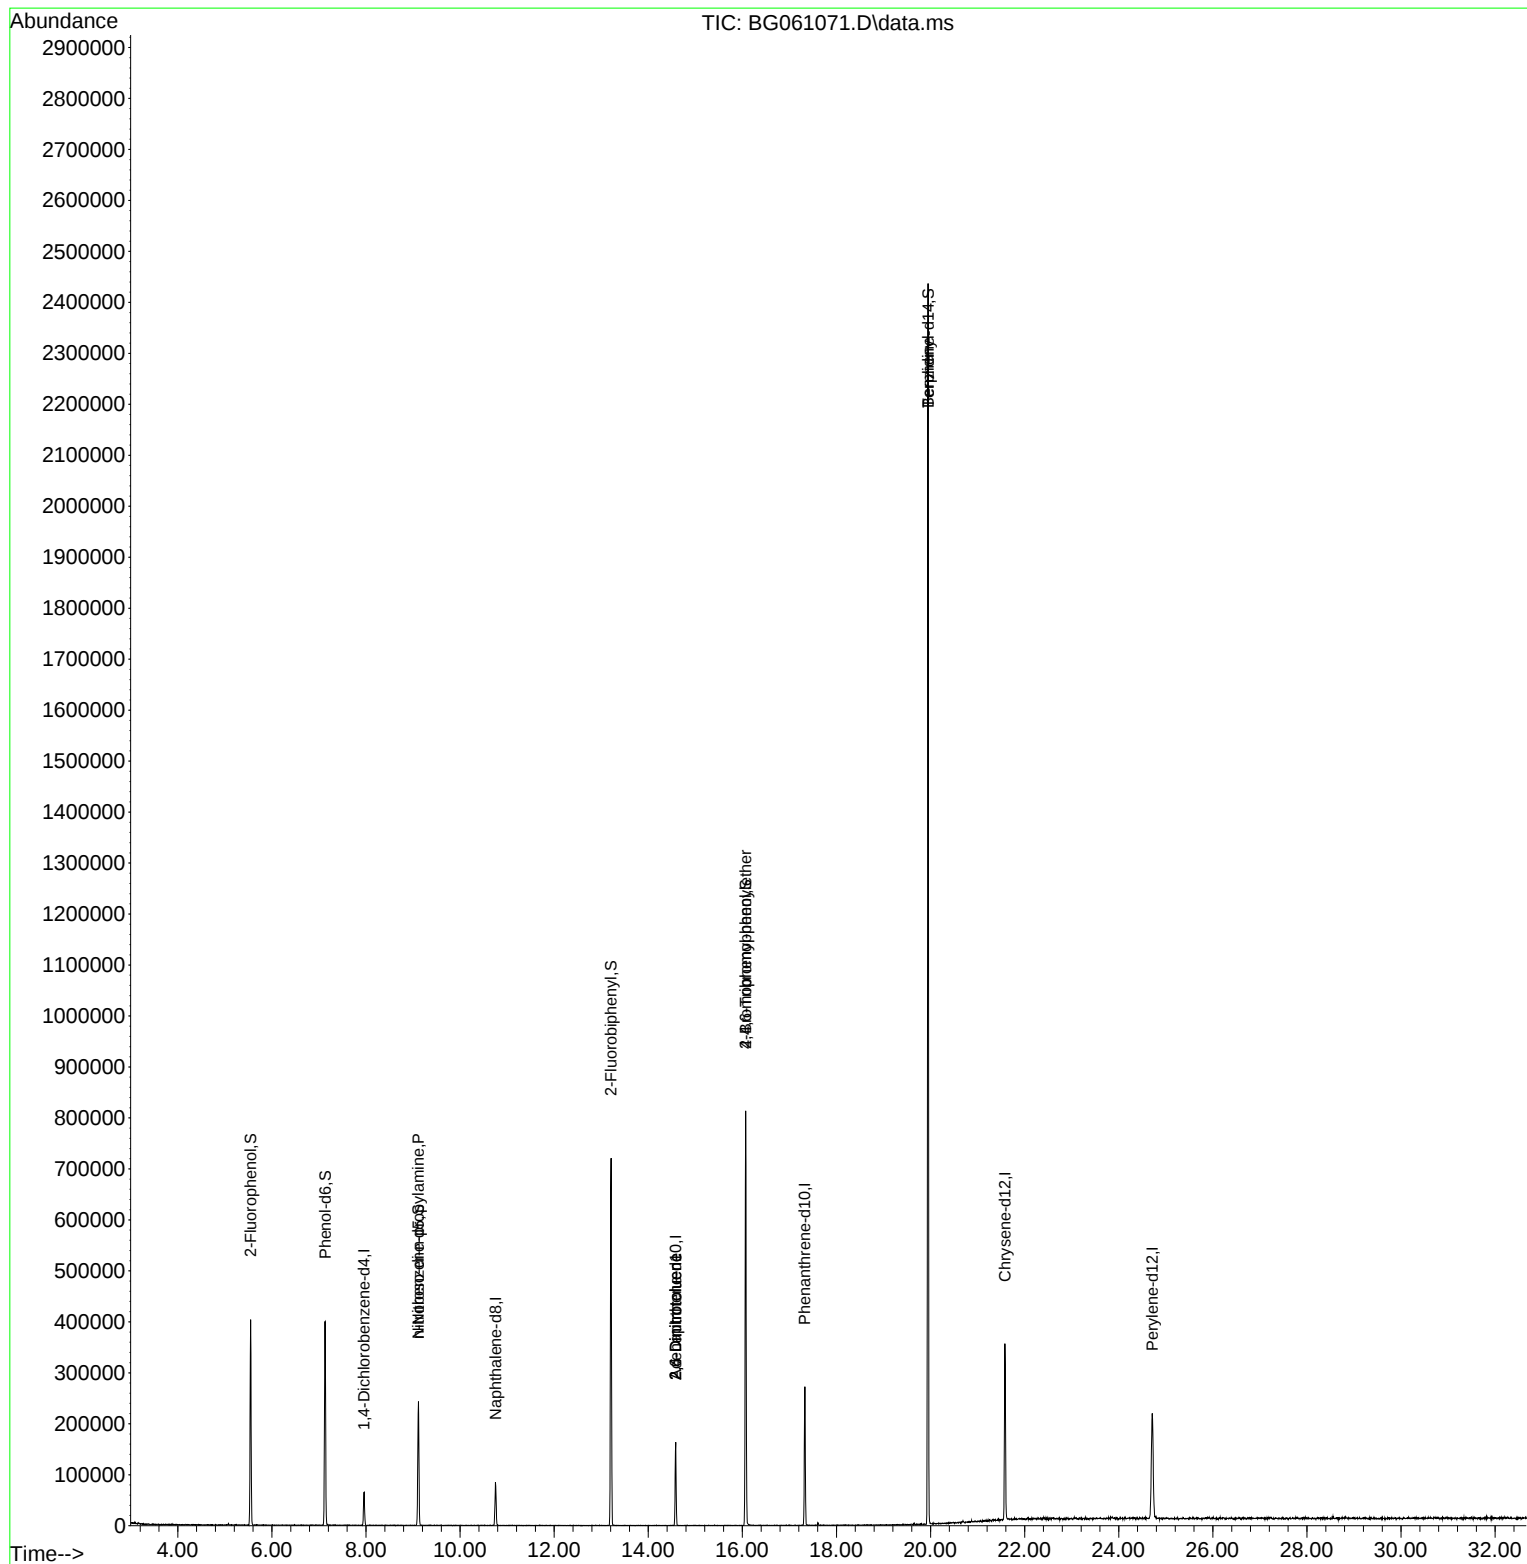


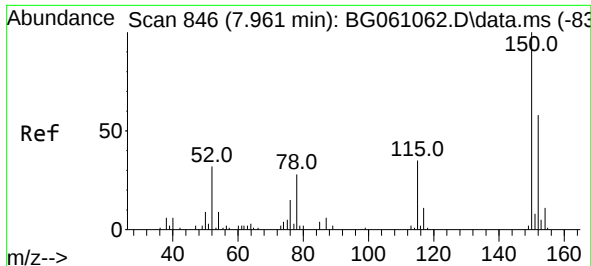

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.956 min Scan# 846
Delta R.T. -0.005 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:152 Resp: 17015
Ion Ratio Lower Upper
152 100
150 137.7 138.3 207.5#
115 60.8 48.0 72.0

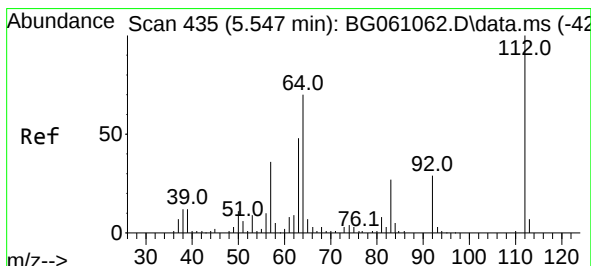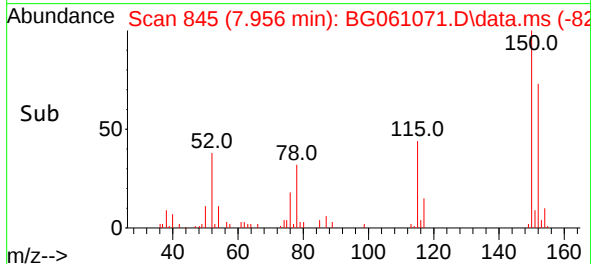

#5
2-Fluorophenol
Concen: 157.884 ng
RT: 5.547 min Scan# 435
Delta R.T. 0.001 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

Tgt Ion:112 Resp: 132092
Ion Ratio Lower Upper
112 100
64 70.8 55.7 83.5
63 45.9 38.1 57.1


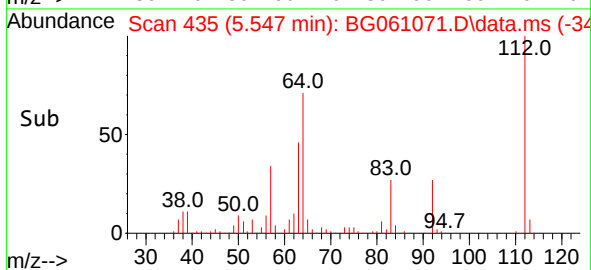

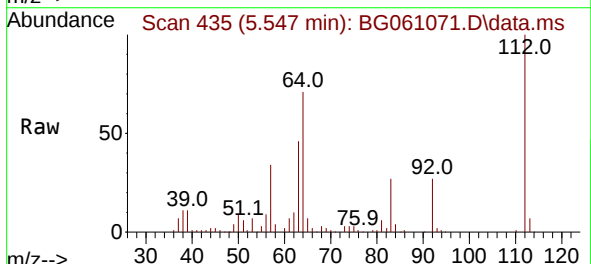


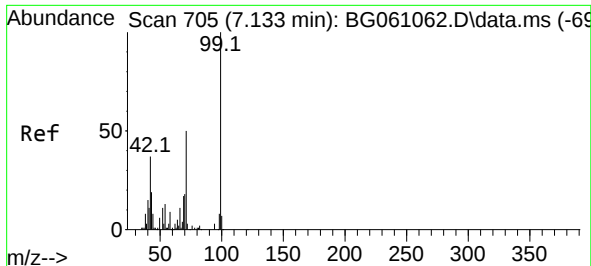

#7
Phenol-d6
Concen: 144.662 ng
RT: 7.134 min Scan# 705
Delta R.T. 0.001 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06




Instrument :
BNA_G
ClientSampleId :


Tgt Ion: 99 Resp: 179041
Ion Ratio Lower Upper
99 100
42 34.9 29.2 43.8
71 49.2 39.7 59.5

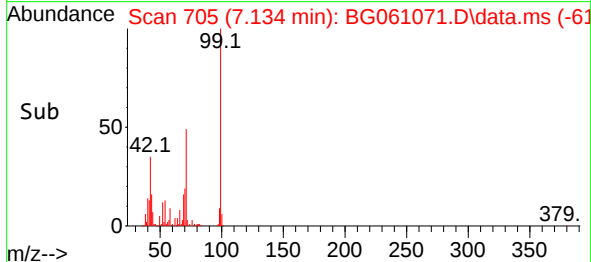

#19
n-Nitroso-di-n-propylamine
Concen: 20.155 ng
RT: 9.114 min Scan# 1042
Delta R.T. 0.347 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

Tgt Ion: 70 Resp: 18668
Ion Ratio Lower Upper
70 100
42 73.5 86.4 129.6#
101 0.0 7.8 11.8#
130 2.0 19.0 28.4#

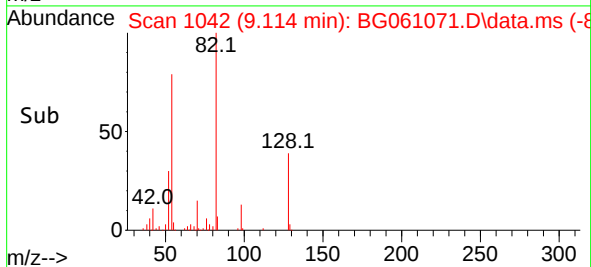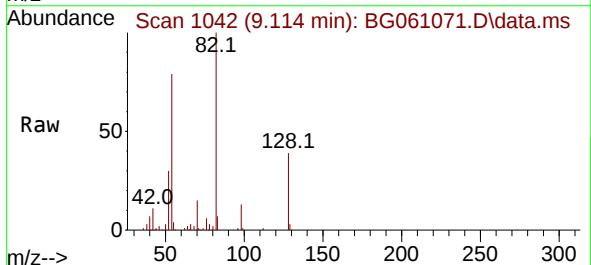



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.753 min Scan# 11

Delta R.T. -0.005 min


Lab File: BG061071.D

Acq: 1 May 2024 11:06



Instrument :

BNA_G

ClientSampleId :

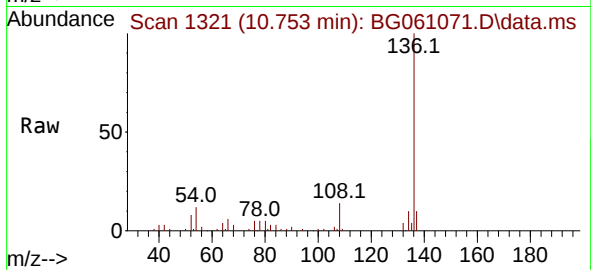

Tgt Ion:	136	Resp:	65232
Ion Ratio	Lower	Upper	
136	100		
137	9.7	7.8	11.6
54	11.9	8.1	12.1
68	2.9	3.0	4.4

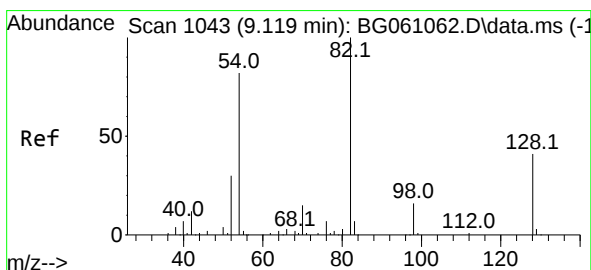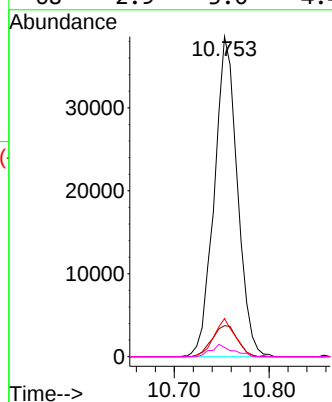

#23

Nitrobenzene-d5

Concen: 93.225 ng




RT: 9.114 min Scan# 1042


Delta R.T. -0.005 min

Lab File: BG061071.D

Acq: 1 May 2024 11:06


Tgt Ion:	82	Resp:	122675
Ion Ratio	Lower	Upper	
82	100		
128	39.4	32.7	49.1
54	78.8	65.6	98.4

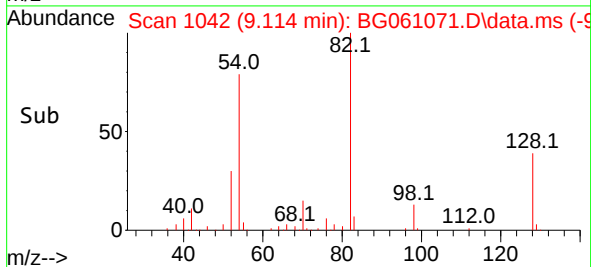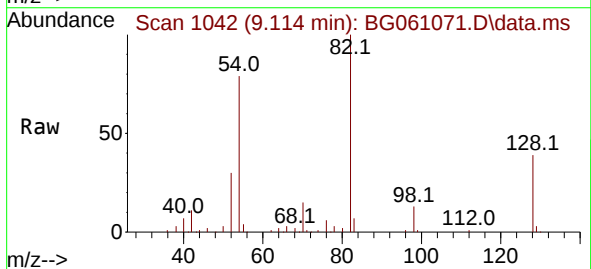



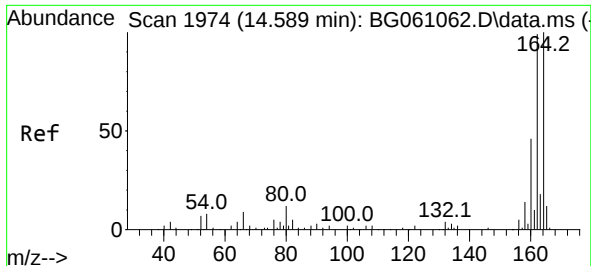


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.584 min Scan# 1974
Delta R.T. -0.005 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06


Instrument :
BNA_G
ClientSampleId :





Tgt Ion:164 Resp: 59974
Ion Ratio Lower Upper
164 100
162 96.8 79.4 119.2
160 40.9 37.0 55.6

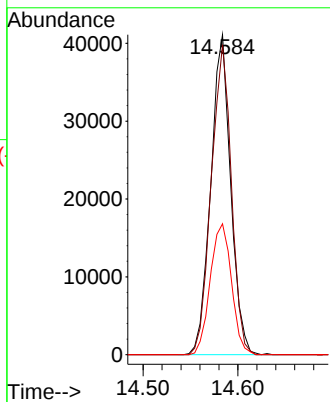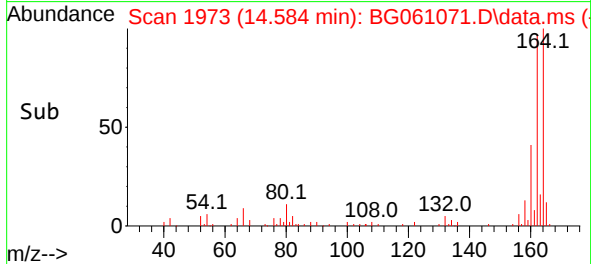


#42
2,4,6-Tribromophenol
Concen: 147.717 ng
RT: 16.070 min Scan# 2226
Delta R.T. -0.005 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

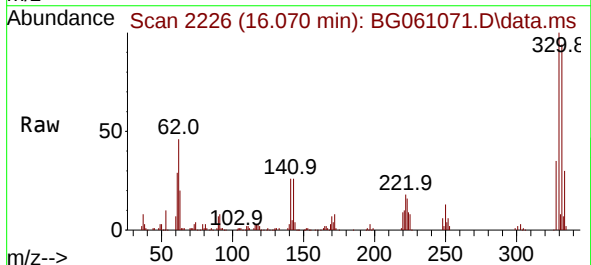


Tgt Ion:330 Resp: 177080
Ion Ratio Lower Upper
330 100
332 96.7 78.6 117.8
141 25.2 20.5 30.7

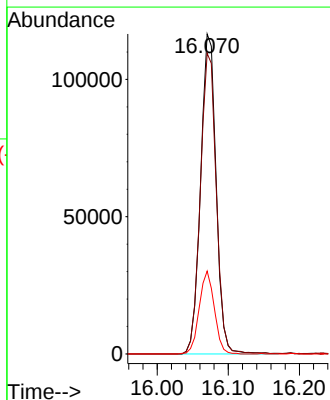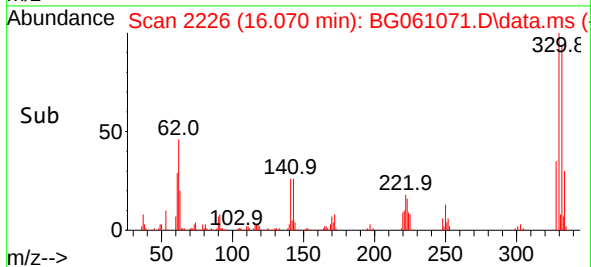



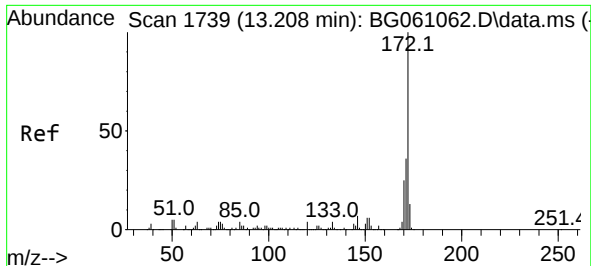


#45
2-Fluorobiphenyl
Concen: 91.200 ng
RT: 13.209 min Scan# 1
Delta R.T. 0.001 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

Instrument :
BNA_G
ClientSampleId :







Tgt Ion:172 Resp: 369889
Ion Ratio Lower Upper
172 100
171 36.2 29.0 43.6
170 23.7 20.2 30.4

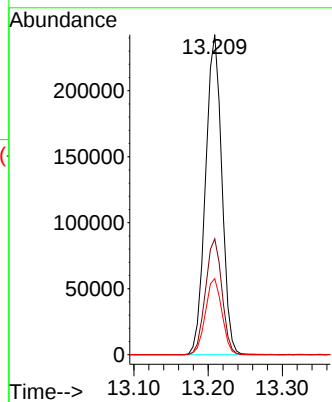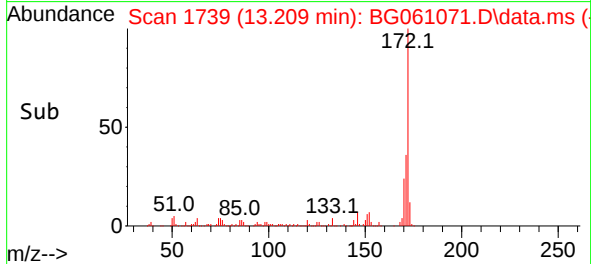

#51
2,6-Dinitrotoluene
Concen: 7.317 ng
RT: 14.584 min Scan# 1973
Delta R.T. 0.424 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

Tgt Ion:165 Resp: 7250
Ion Ratio Lower Upper
165 100
63 0.0 60.0 90.0#
89 0.0 50.9 76.3#

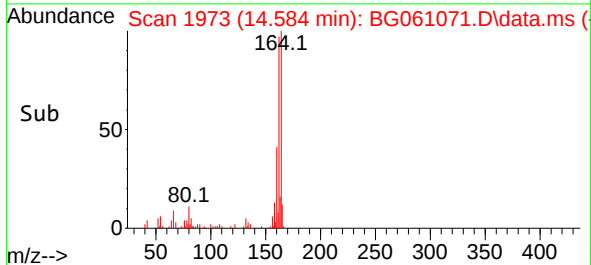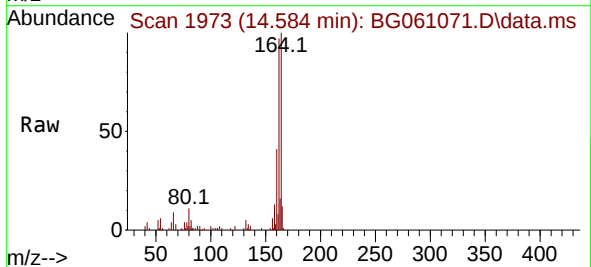

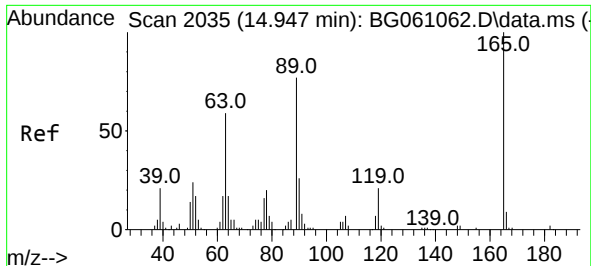

#57

2,4-Dinitrotoluene

Concen: 4.946 ng

RT: 14.584 min Scan# 1973

Delta R.T. -0.364 min


Lab File: BG061071.D

Acq: 1 May 2024 11:06

Instrument :

BNA_G

ClientSampleId :

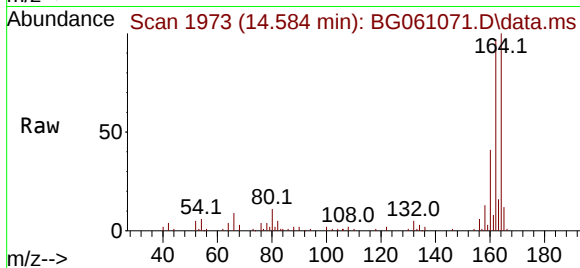

Tgt Ion:165 Resp: 7250




Ion Ratio Lower Upper

165 100

63 0.0 47.3 70.9#

89 0.0 61.8 92.8#

182 0.0 1.8 2.6#

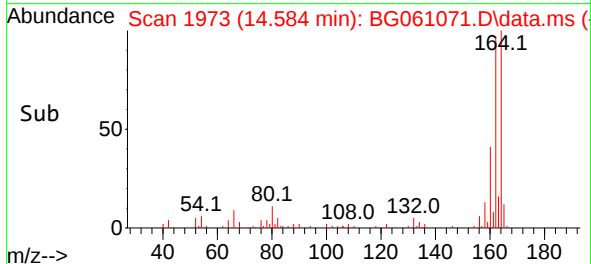

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.328 min Scan# 2440

Delta R.T. -0.005 min

Lab File: BG061071.D

Acq: 1 May 2024 11:06




Tgt Ion:188 Resp: 174465


Ion Ratio Lower Upper

188 100

94 4.6 3.6 5.4

80 5.8 4.2 6.2


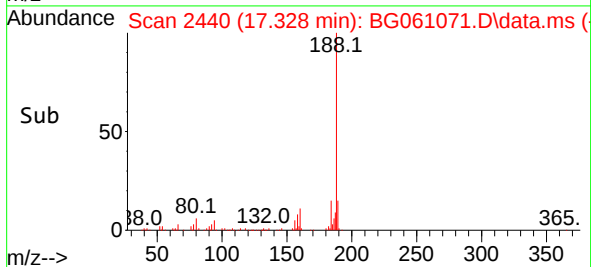
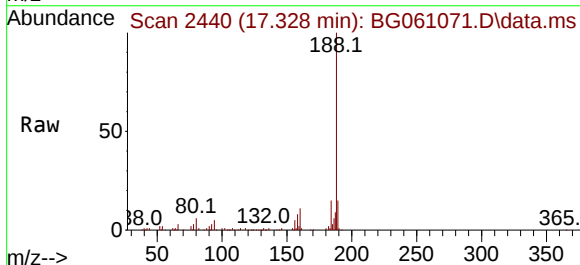



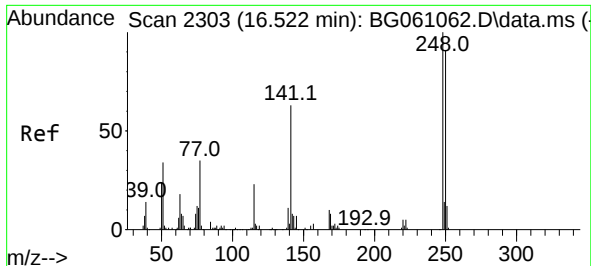

#67
4-Bromophenyl-phenylether
Concen: 5.276 ng
RT: 16.070 min Scan# 21
Delta R.T. -0.452 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:248 Resp: 10844
Ion Ratio Lower Upper
248 100
250 199.3 73.0 109.4#
141 410.5 50.8 76.2#

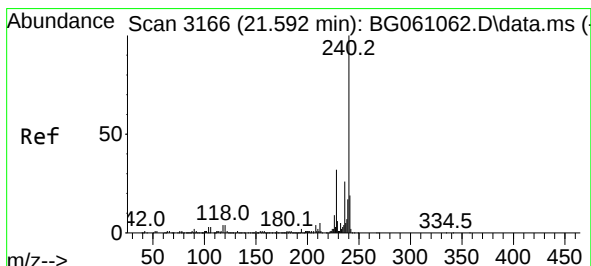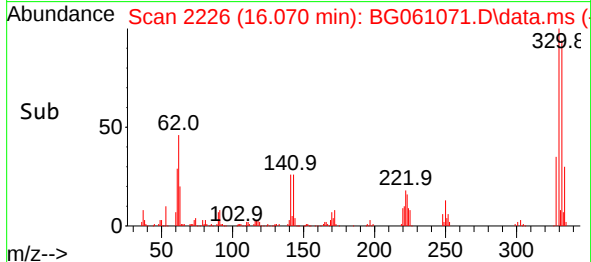

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.581 min Scan# 3164
Delta R.T. -0.011 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06

Tgt Ion:240 Resp: 213390
Ion Ratio Lower Upper
240 100
120 4.8 3.2 4.8
236 25.1 21.0 31.6


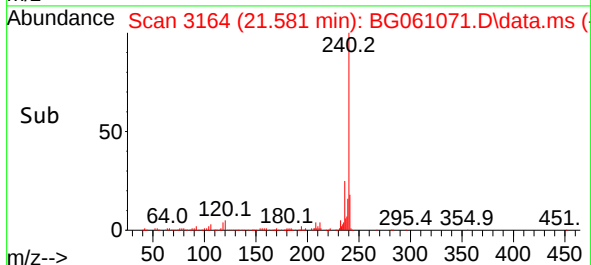
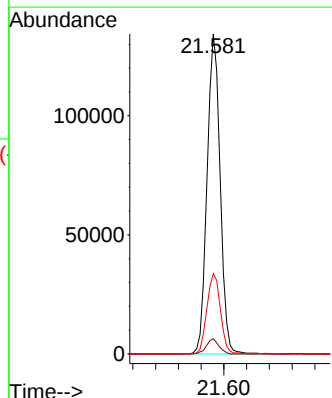
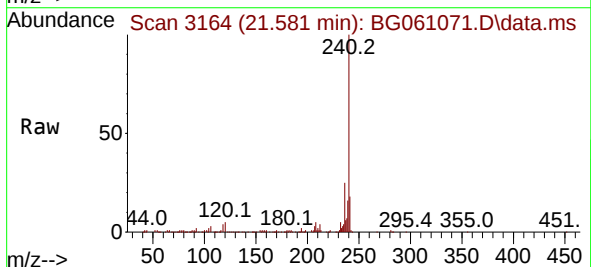




#77
Benzidine
Concen: 7.153 ng
RT: 19.948 min Scan# 21
Delta R.T. 0.383 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06




Instrument :
BNA_G
ClientSampleId :


Tgt Ion:184 Resp: 18789
Ion Ratio Lower Upper
184 100
185 19.0 12.0 18.0#
183 8.0 10.9 16.3#

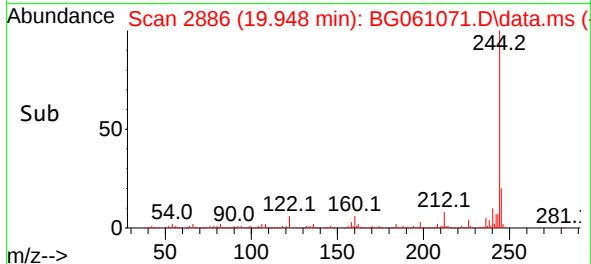

#79
Terphenyl-d14
Concen: 95.081 ng
RT: 19.948 min Scan# 2886
Delta R.T. -0.005 min
Lab File: BG061071.D
Acq: 1 May 2024 11:06


Tgt Ion:244 Resp: 1219937
Ion Ratio Lower Upper
244 100
212 7.6 5.7 8.5
122 5.5 4.2 6.2

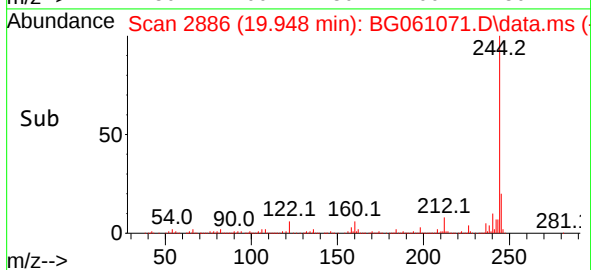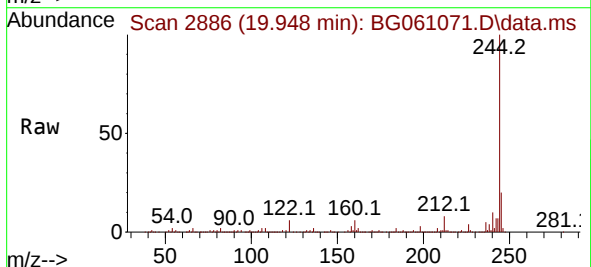



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.713 min Scan# 30
 Delta R.T. -0.017 min
 Lab File: BG061071.D
 Acq: 1 May 2024 11:06

Instrument :
 BNA_G
 ClientSampleId :



Tgt Ion:264 Resp: 238983
 Ion Ratio Lower Upper
 264 100
 260 23.4 17.7 26.5
 265 21.7 16.4 24.6

