


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050124\
Data File : BG061068.D
Acq On : 1 May 2024 9:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

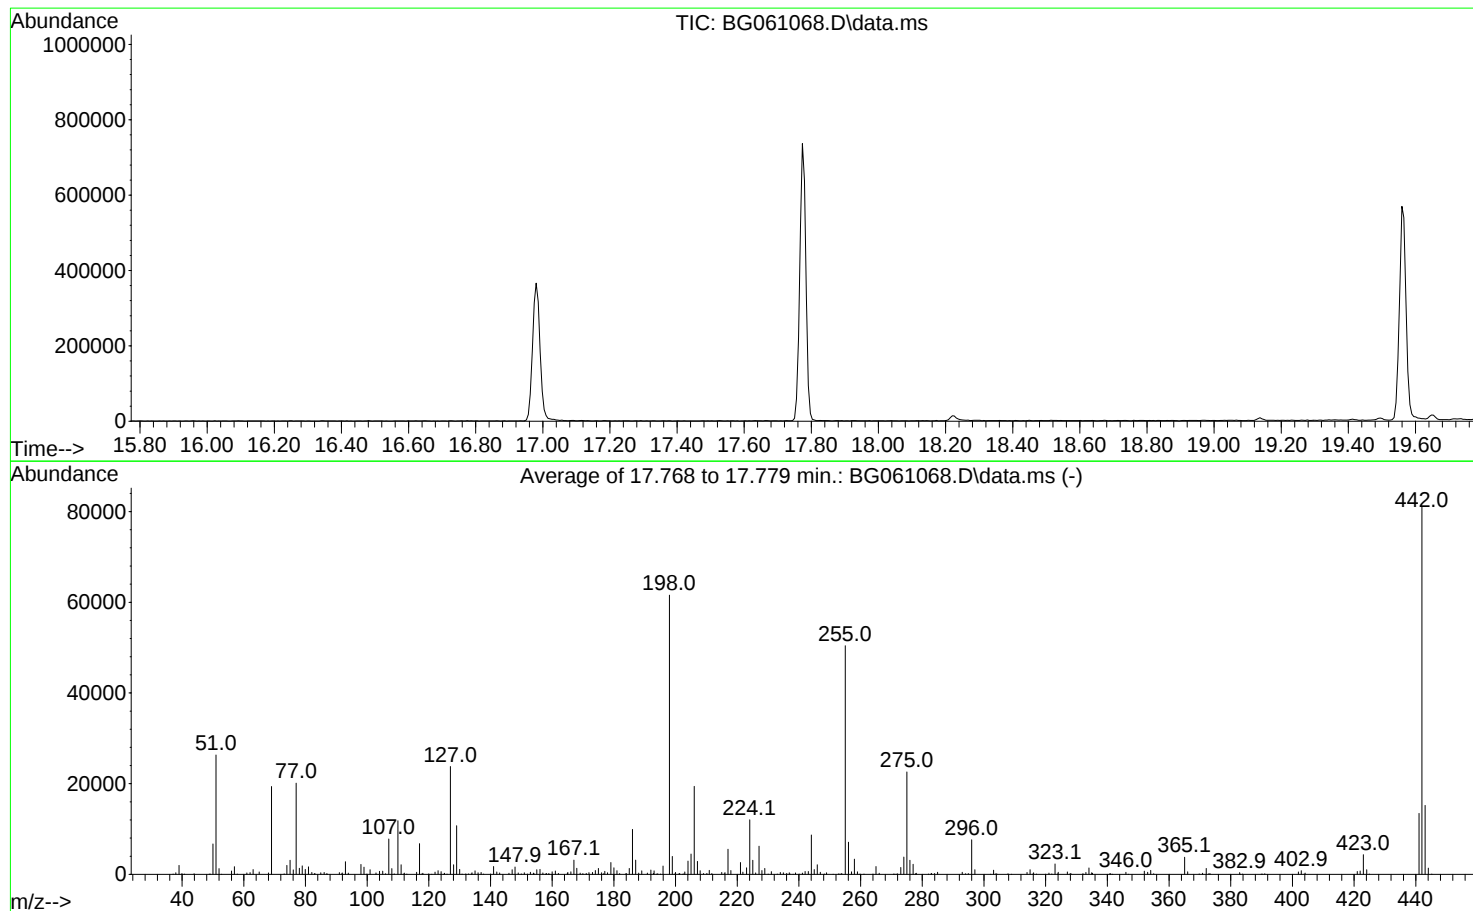

AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2509

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	42.7	26313	PASS
68	69	0.00	2	1.6	306	PASS
69	198	0.00	100	31.5	19387	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.7	23803	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61579	PASS
199	198	5	9	6.4	3957	PASS
275	198	10	60	36.7	22592	PASS
365	198	1	100	6.1	3780	PASS
441	198	0.01	100	21.8	13441	PASS
442	442	50	100	100.0	81123	PASS
443	442	15	24	18.7	15192	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/1/2024	BNA_G	<u>BG061068.D</u>
Compound Name	Response	Retention Time
DDT	256188	20.799
DDD	5386	20.359
DDE	122	19.842
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5508	261696	2.10

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050124\
Data File : BG061068.D
Acq On : 1 May 2024 9:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 01 11:22:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

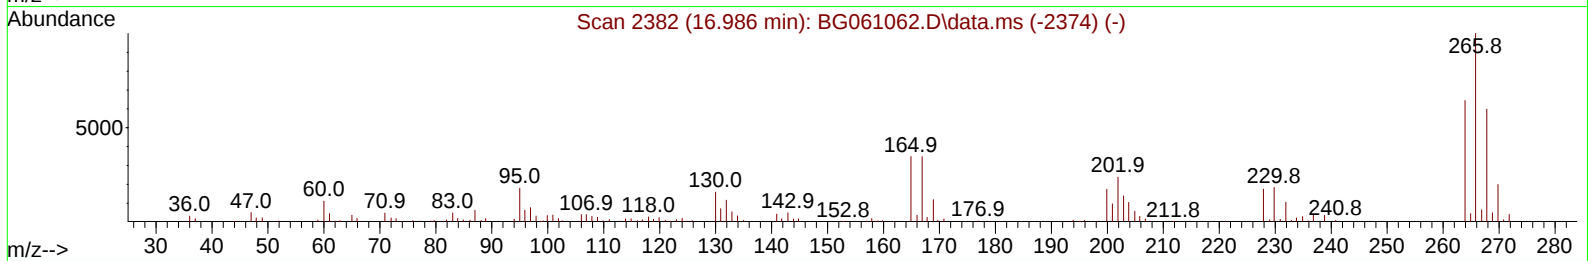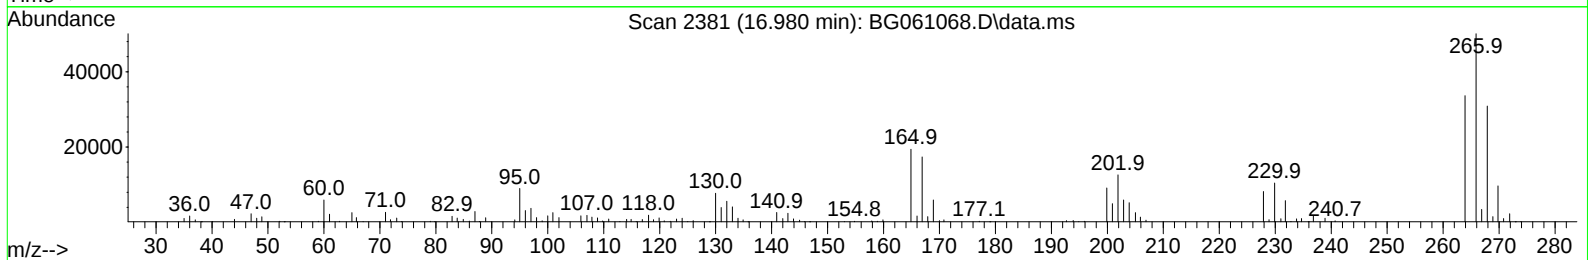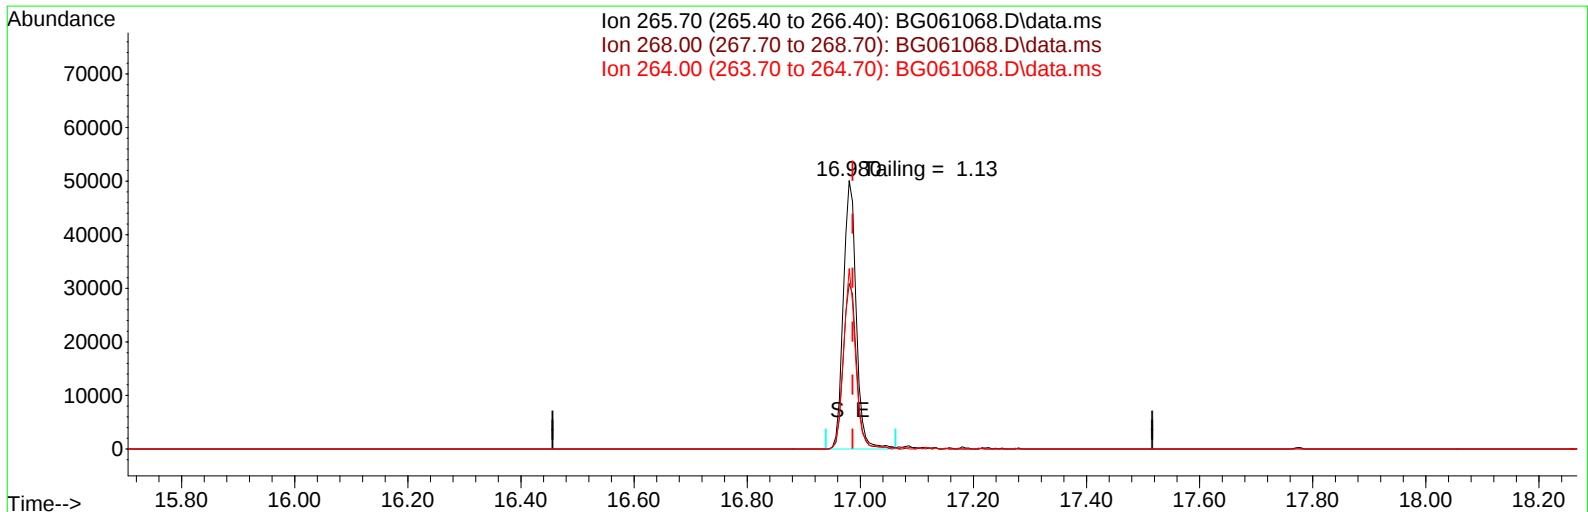

TIC: BG061068.D\data.ms

(70) Pentachlorophenol (C)

16.980min (-0.006) 163172.82 ng




response 79370

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	61.66
264.00	64.40	67.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050124\
Data File : BG061068.D
Acq On : 1 May 2024 9:03
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 01 11:22:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

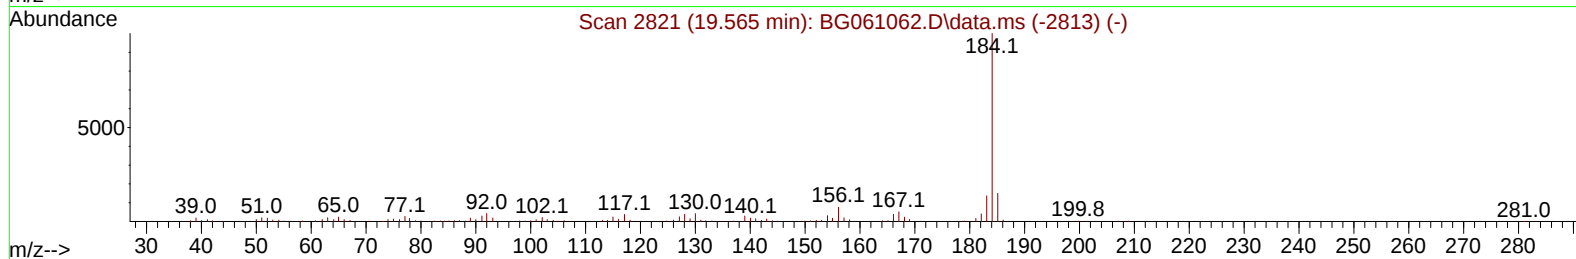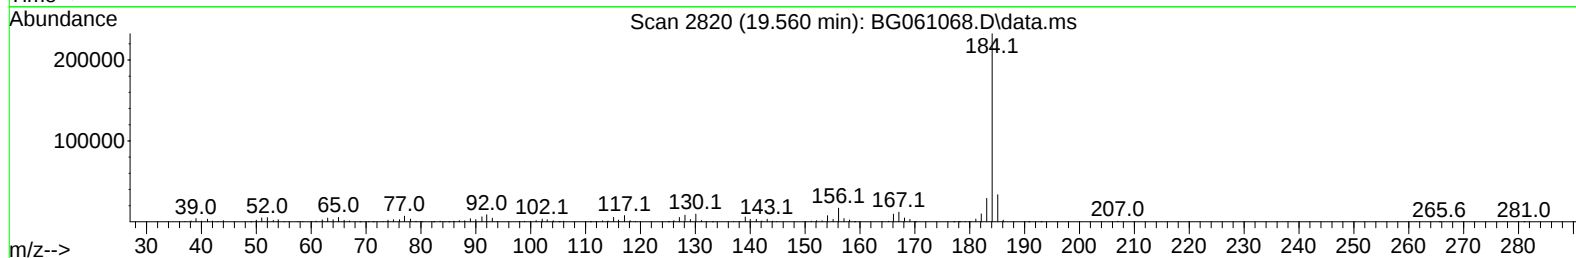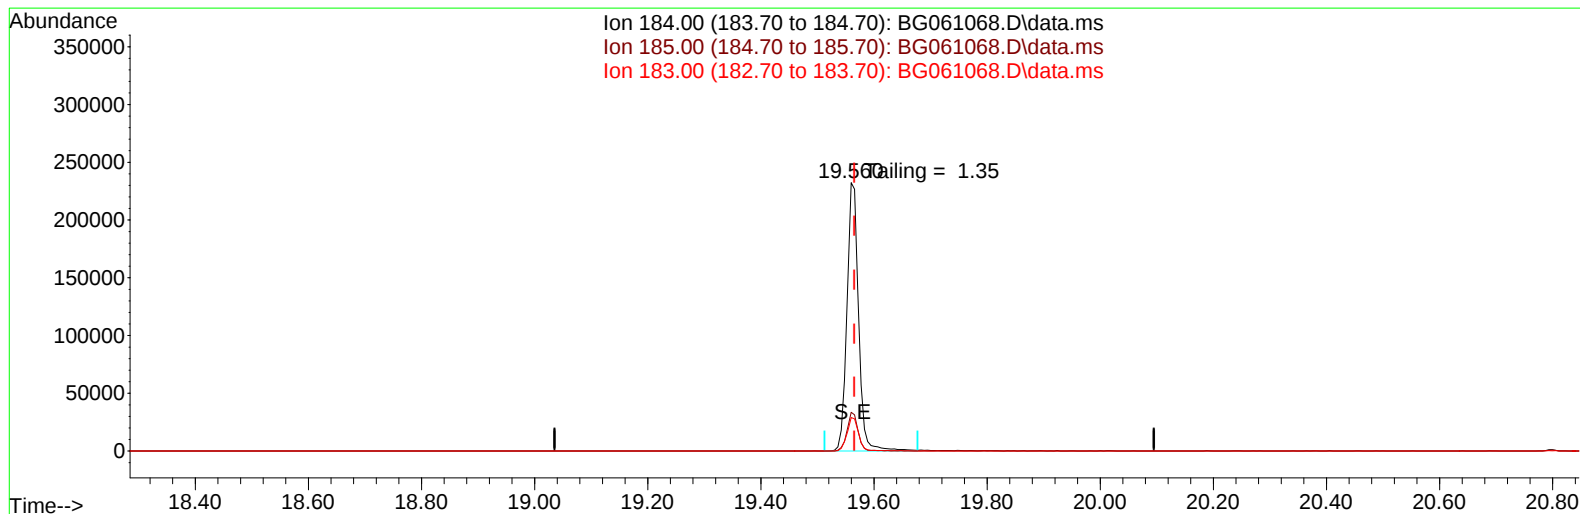

TIC: BG061068.D\data.ms

(77) Benzidine**19.560min (-0.005) 12997.39 ng****response 332148**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.43
183.00	13.60	12.49
0.00	0.00	0.00