
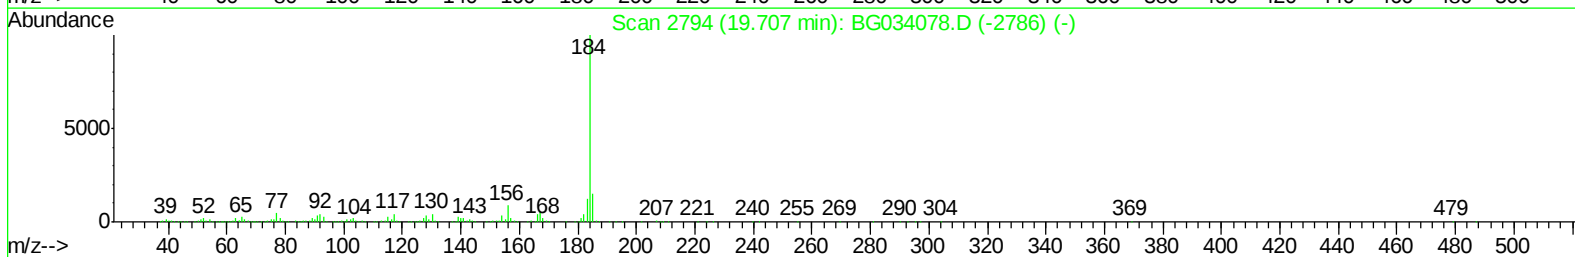
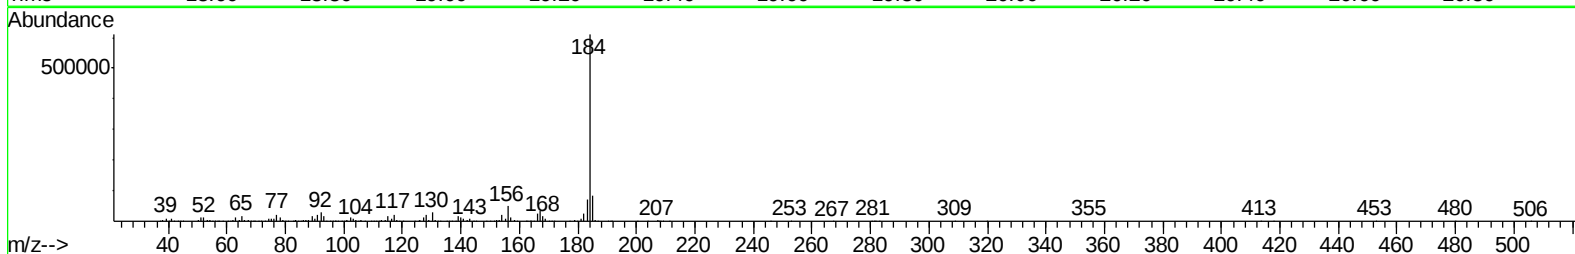


Data Path : Z:\HPCHEM1\BNA G\DATA\BG050218\
Data File : BG034118.D
Acq On : 2 May 2018 16:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 08:26:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

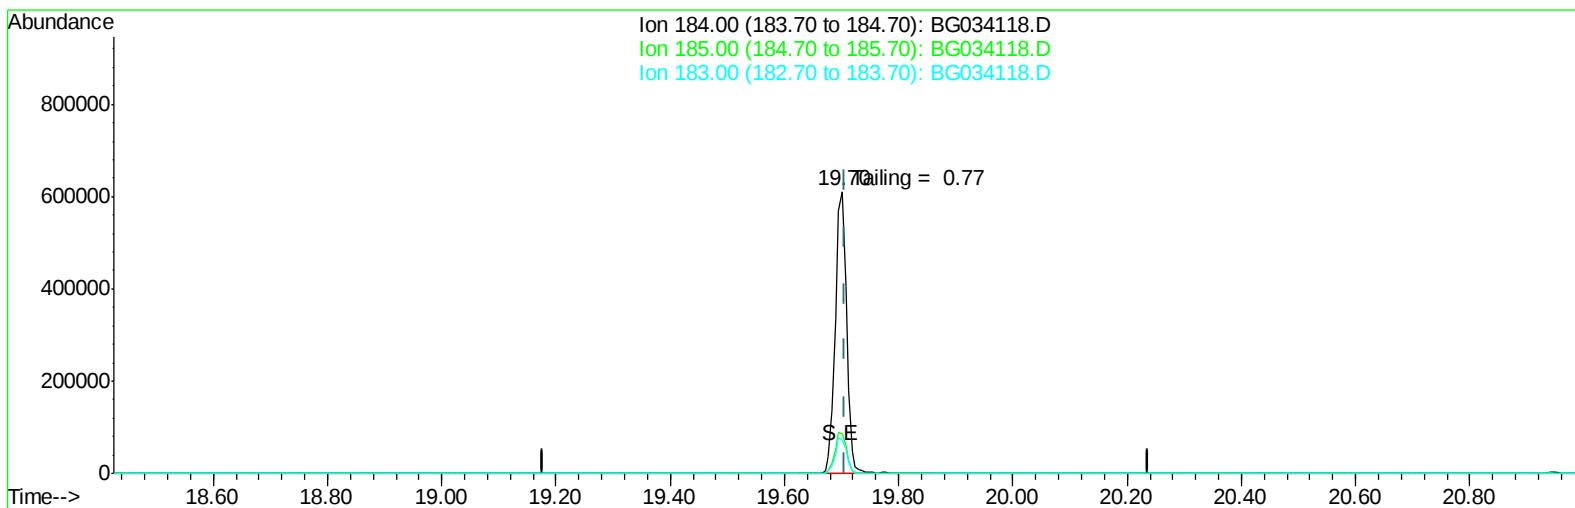

TIC: BG034118.D

(76) Benzidine

19.701min (-0.007) 496724.28ng

response 831685

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.95
183.00	13.30	11.97
0.00	0.00	0.00