
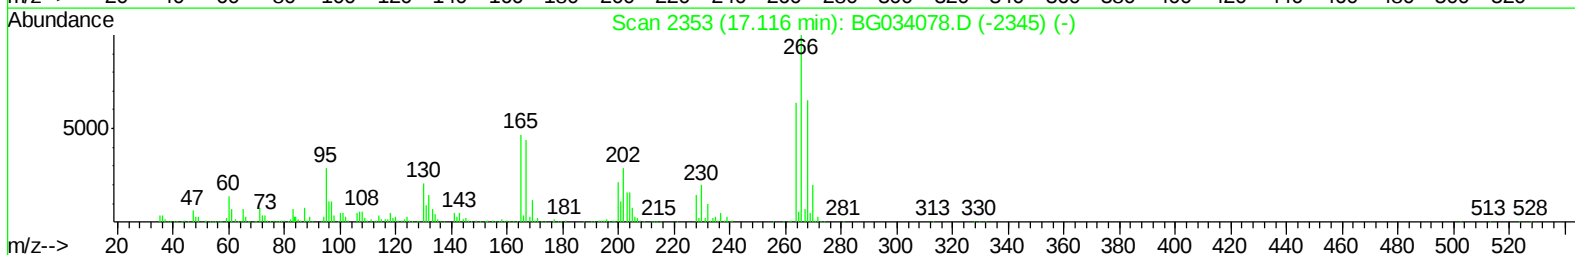
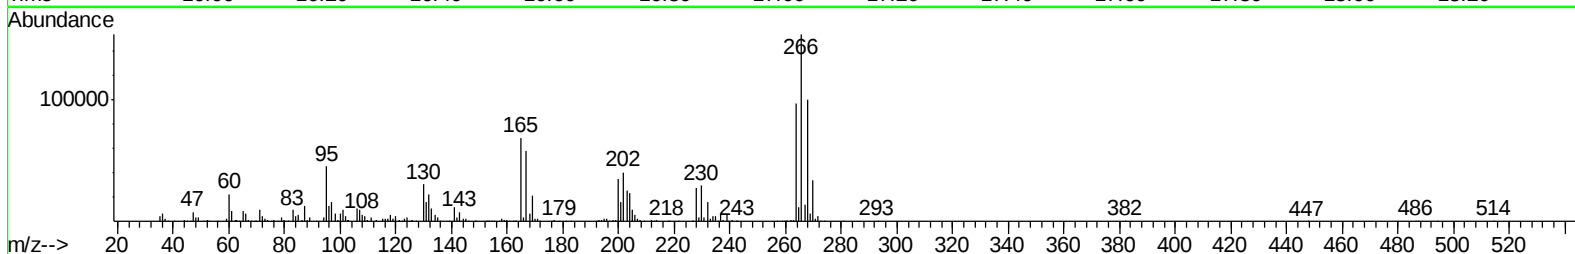


Data Path : Z:\HPCHEM1\BNA G\DATA\BG050218\
Data File : BG034137.D
Acq On : 3 May 2018 5:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 08:26:59 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 01 19:08:03 2018
Response via : Initial Calibration

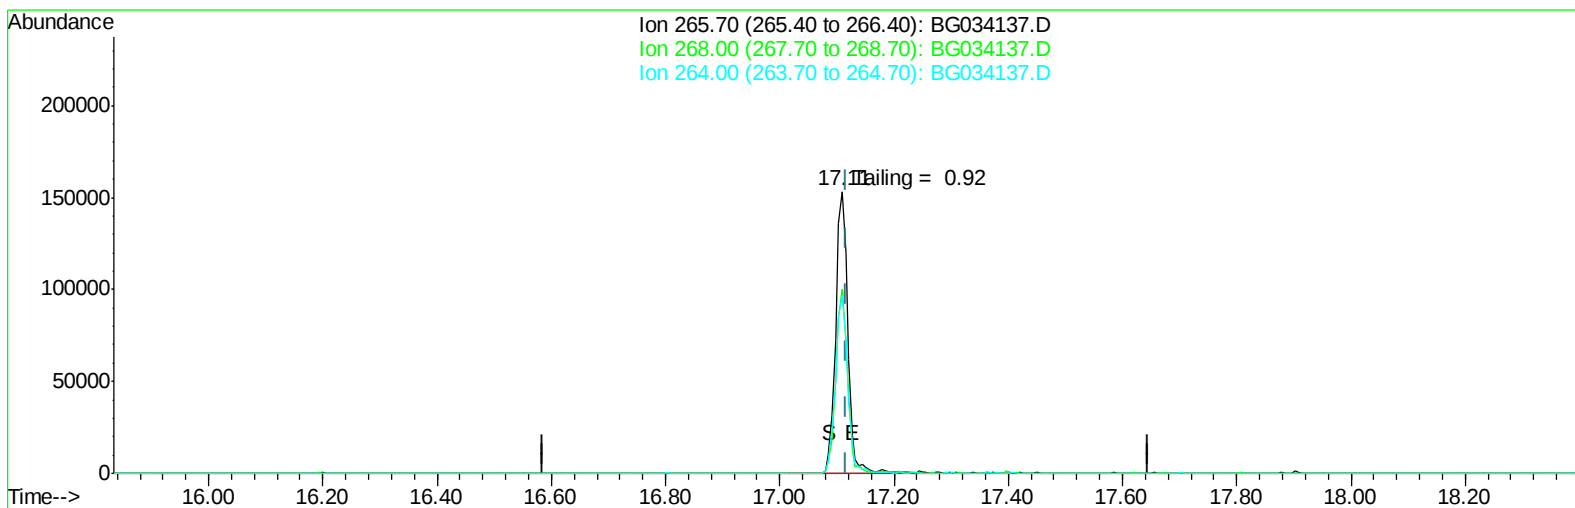

TIC: BG034137.D

(69) Pentachlorophenol (C)

17.109min (-0.007) 244356.40ng

response 223234

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.24
264.00	62.00	62.99
0.00	0.00	0.00