


Data Path : Z:\HPCHEM1\BNA G\Data\BG050218\
 Data File : BG034118.D
 Acq On : 2 May 2018 16:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 19:08:03 2018

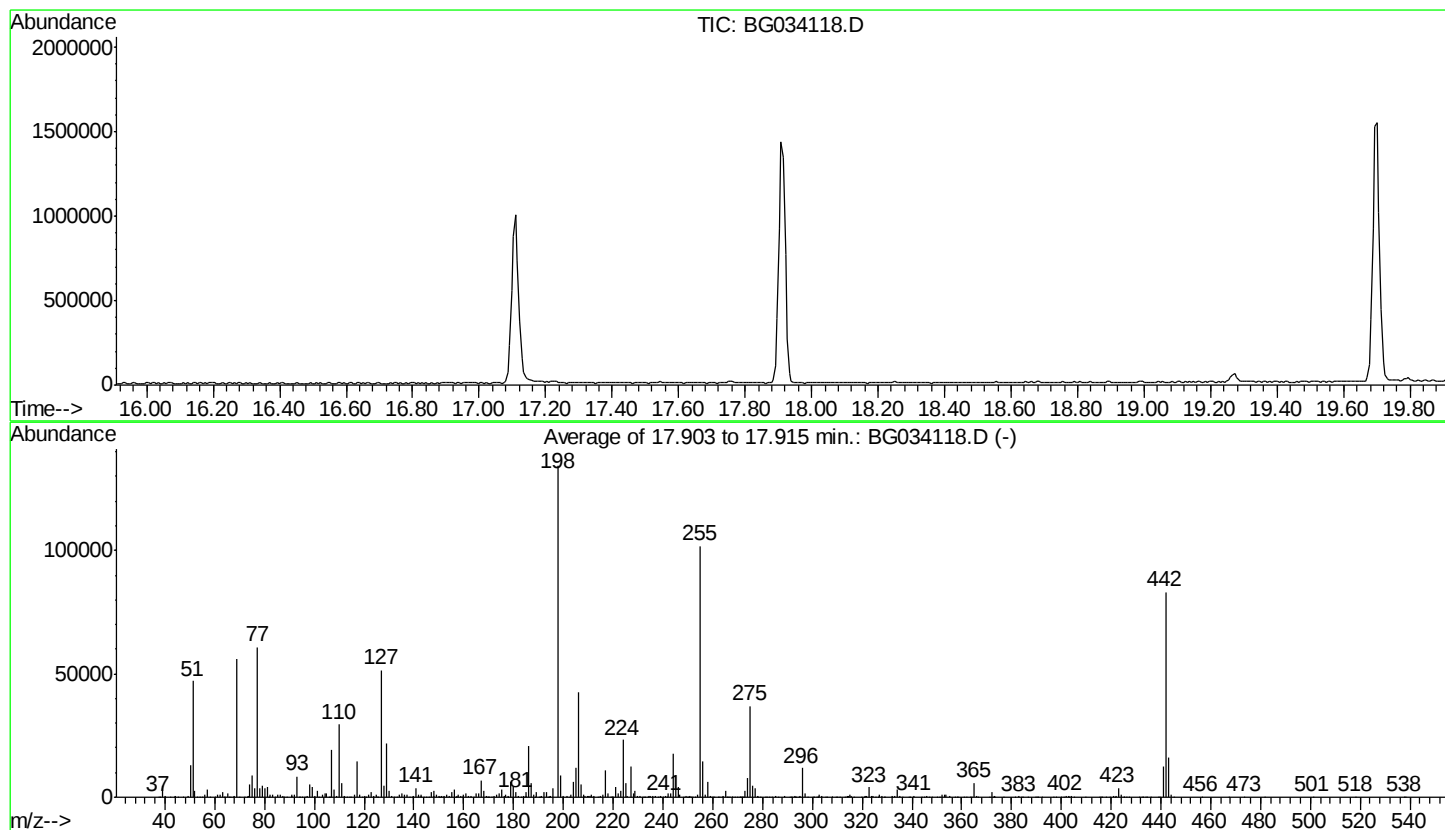

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	47108	PASS
68	69	0.00	2	1.0	540	PASS
69	198	0.00	100	41.9	56304	PASS
70	69	0.00	2	0.4	206	PASS
127	198	10	80	38.3	51493	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	134397	PASS
199	198	5	9	6.5	8741	PASS
275	198	10	60	27.5	36906	PASS
365	198	1	100	4.3	5804	PASS
441	443	0.01	100	78.3	12538	PASS
442	198	50	100	61.9	83197	PASS
443	442	15	24	19.3	16020	PASS