


Data Path : Z:\HPCHEM1\BNA G\Data\BG050218\
 Data File : BG034137.D
 Acq On : 3 May 2018 5:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 01 19:08:03 2018

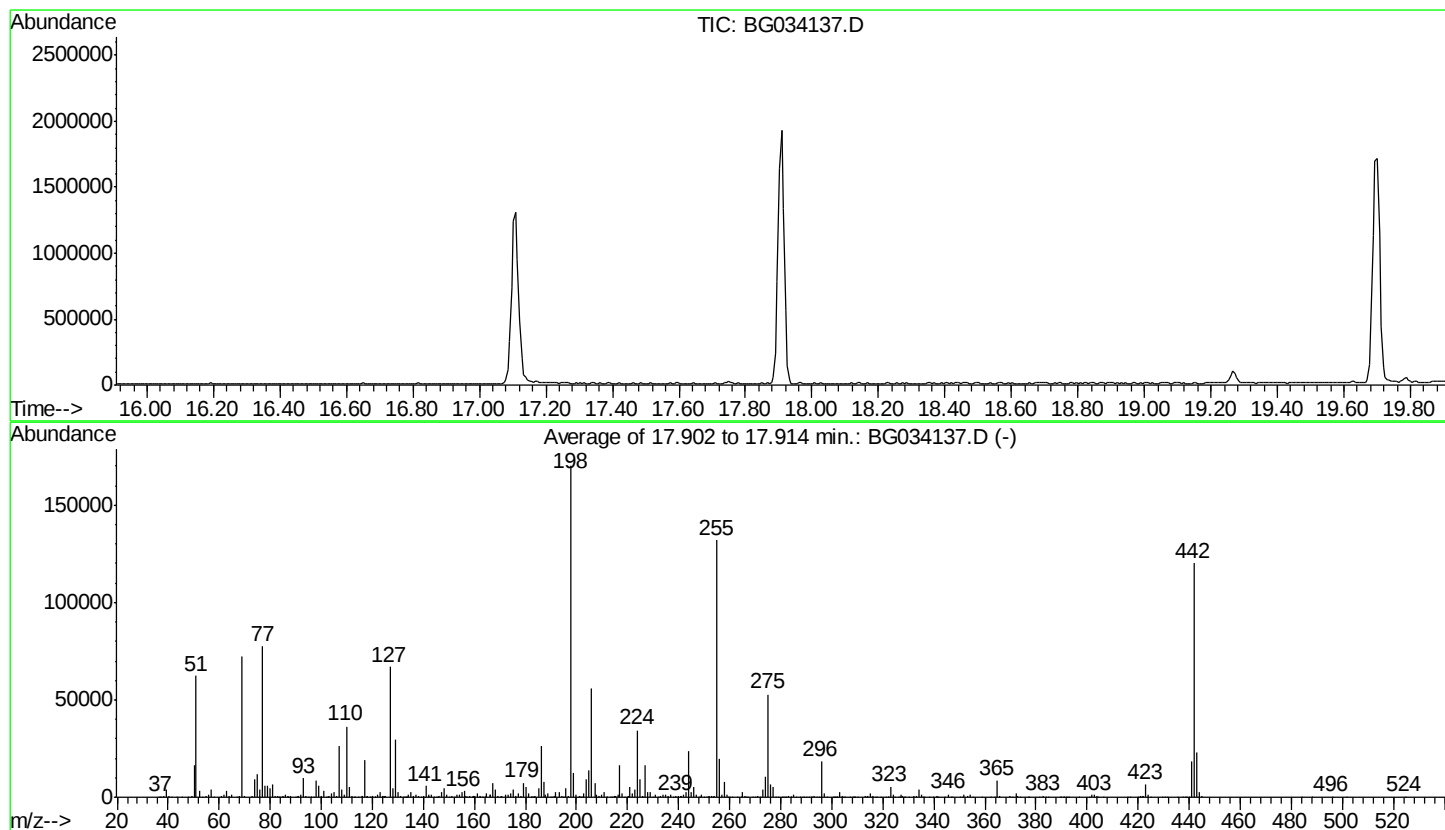

AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	62224	PASS
68	69	0.00	2	0.8	572	PASS
69	198	0.00	100	42.4	72133	PASS
70	69	0.00	2	0.9	642	PASS
127	198	10	80	39.2	66770	PASS
197	198	0.00	2	0.5	771	PASS
198	198	100	100	100.0	170240	PASS
199	198	5	9	7.3	12502	PASS
275	198	10	60	30.9	52680	PASS
365	198	1	100	4.9	8261	PASS
441	443	0.01	100	82.0	18713	PASS
442	198	50	100	70.6	120144	PASS
443	442	15	24	19.0	22813	PASS