
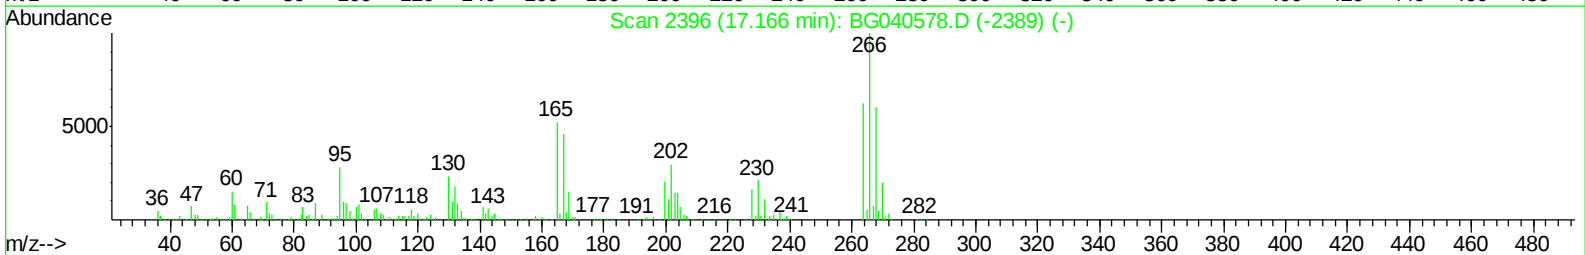
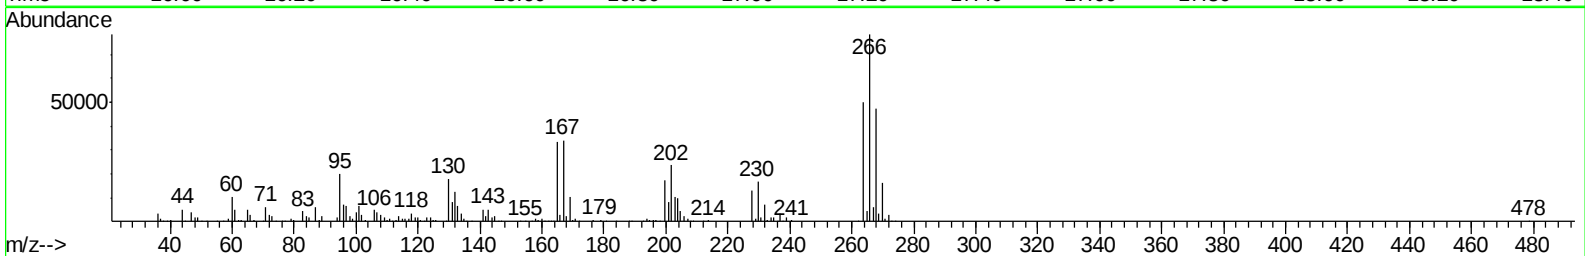


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG050219\
Data File : BG040706.D
Acq On : 2 May 2019 14:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:24:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

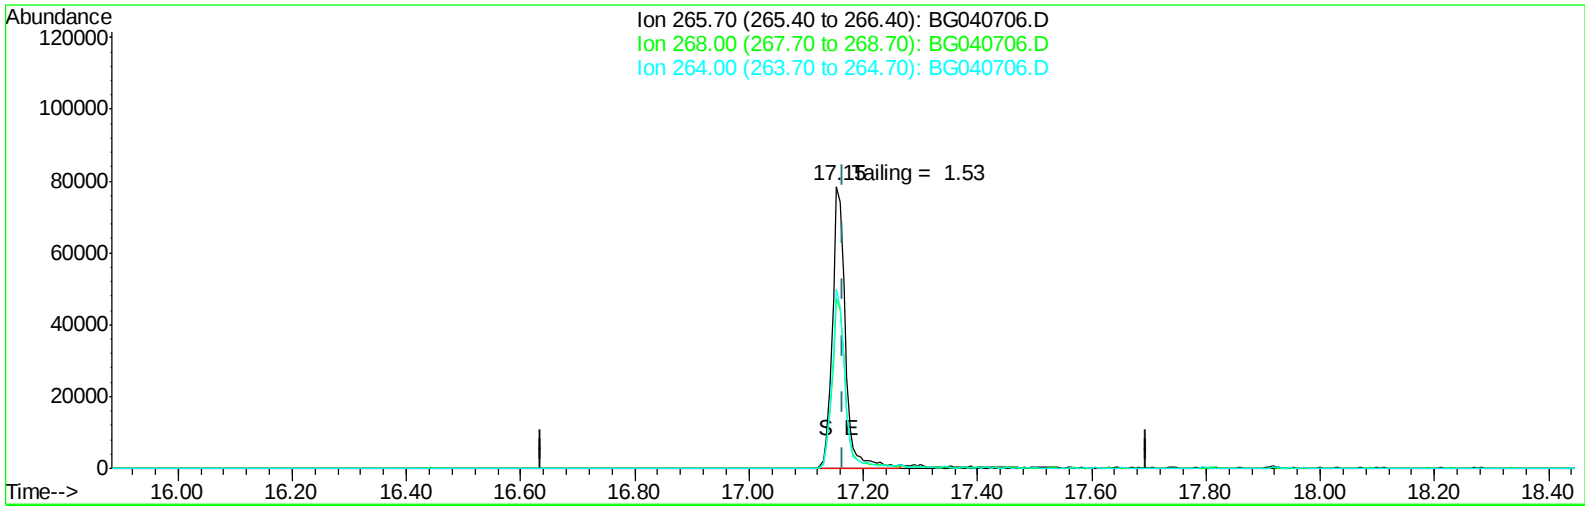

TIC: BG040706.D

(70) Pentachlorophenol (C)




17.153min (-0.012) 247212.88ng

response 122995

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	60.53
264.00	62.50	63.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG050219\
Data File : BG040706.D
Acq On : 2 May 2019 14:35
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 03 09:24:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

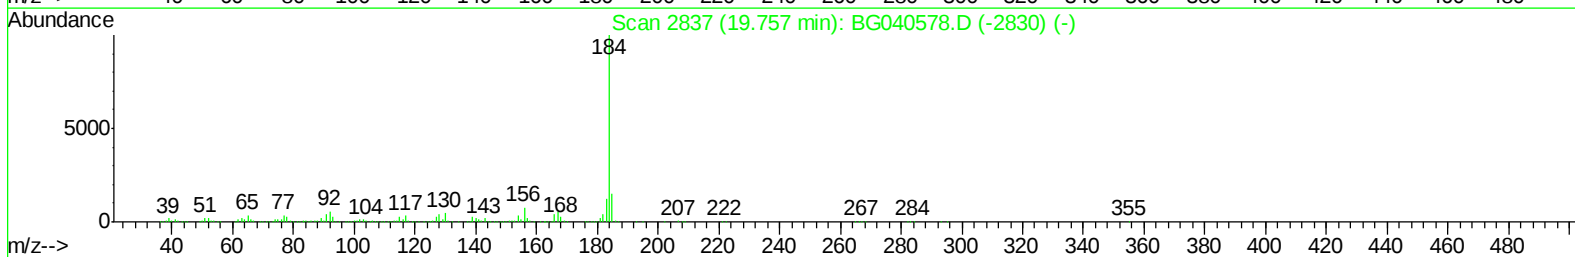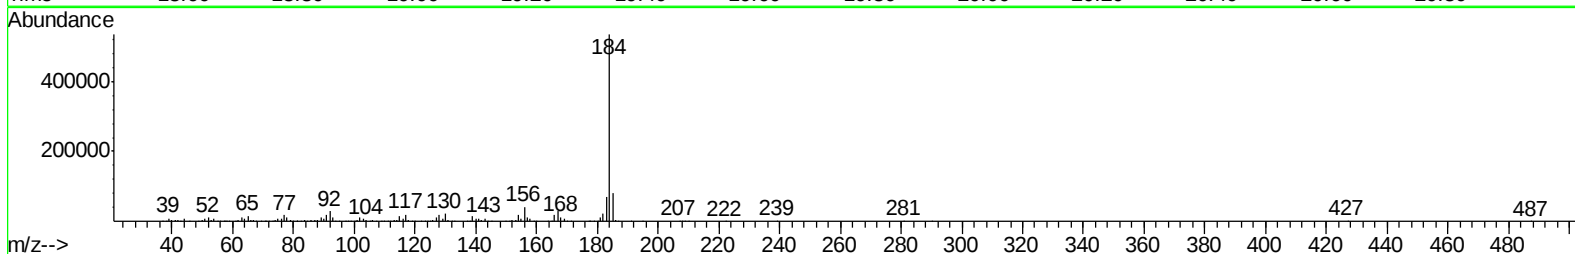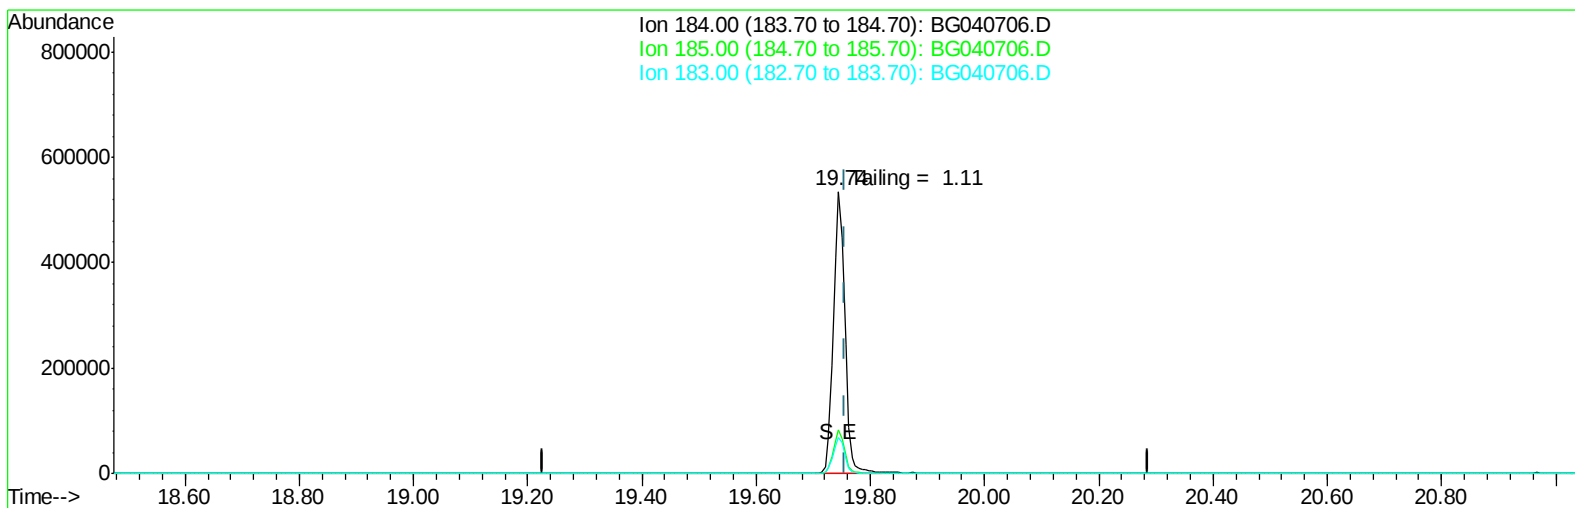

TIC: BG040706.D

(77) Benzidine

19.744min (-0.012) 381742.00ng

response 742112

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.26
183.00	12.70	12.93
0.00	0.00	0.00