
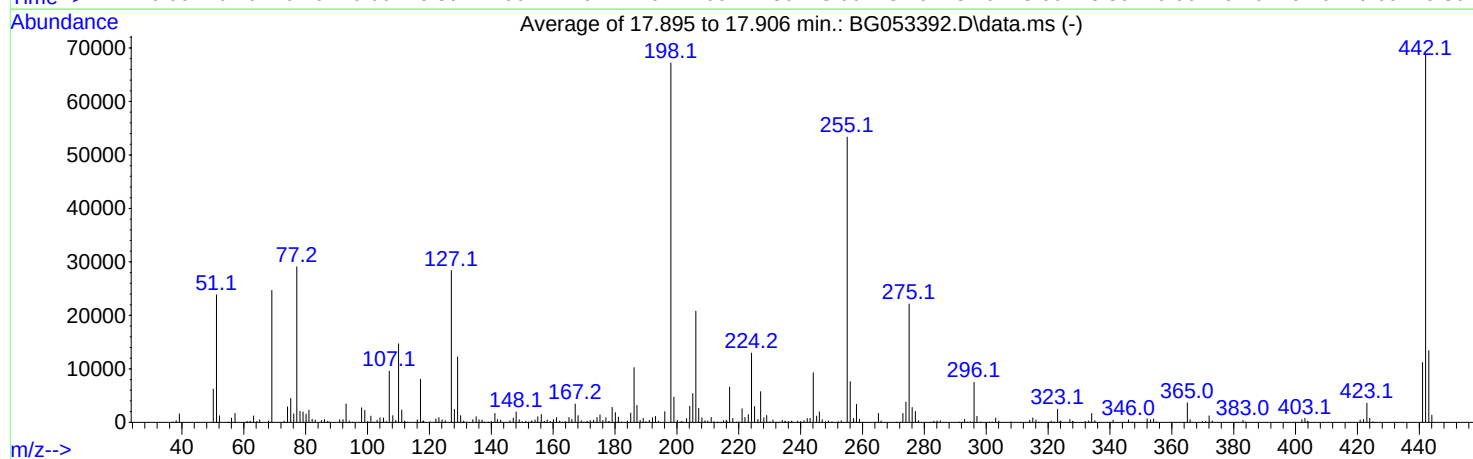


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050222\
 Data File : BG053392.D
 Acq On : 2 May 2022 10:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 06:03:03 2022

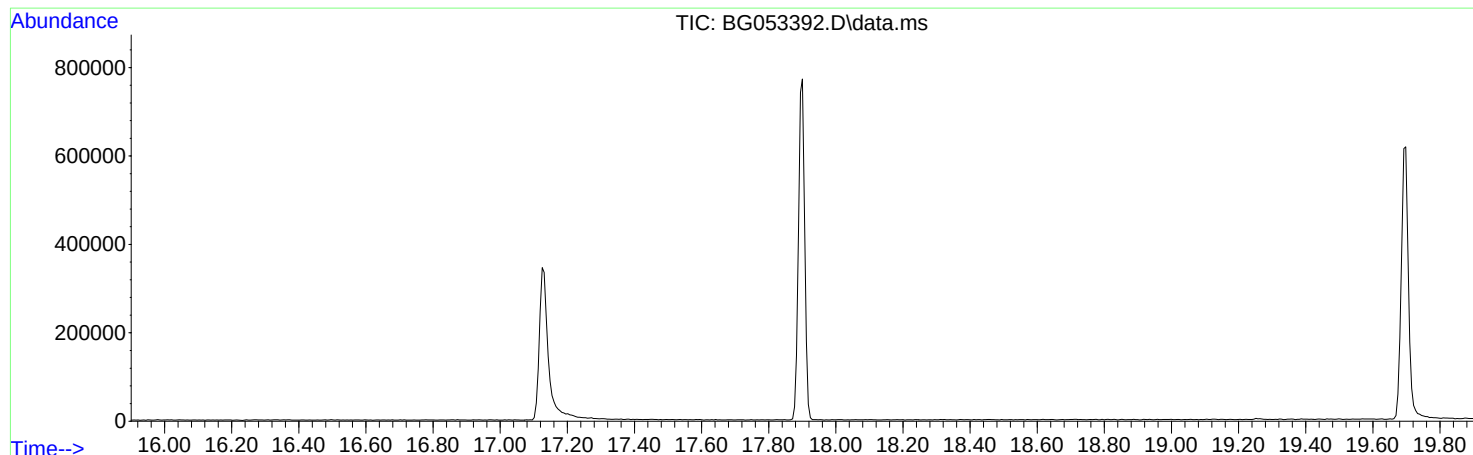




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	23834	PASS
68	69	0.00	2	1.2	284	PASS
69	198	0.00	100	36.7	24669	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	28403	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	67205	PASS
199	198	5	9	7.1	4739	PASS
275	198	10	60	32.9	22137	PASS
365	198	1	100	5.4	3651	PASS
441	198	0.01	100	16.7	11197	PASS
442	442	50	100	100.0	68779	PASS
443	442	15	24	19.5	13419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050222\
Data File : BG053392.D
Acq On : 2 May 2022 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 02 16:52:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

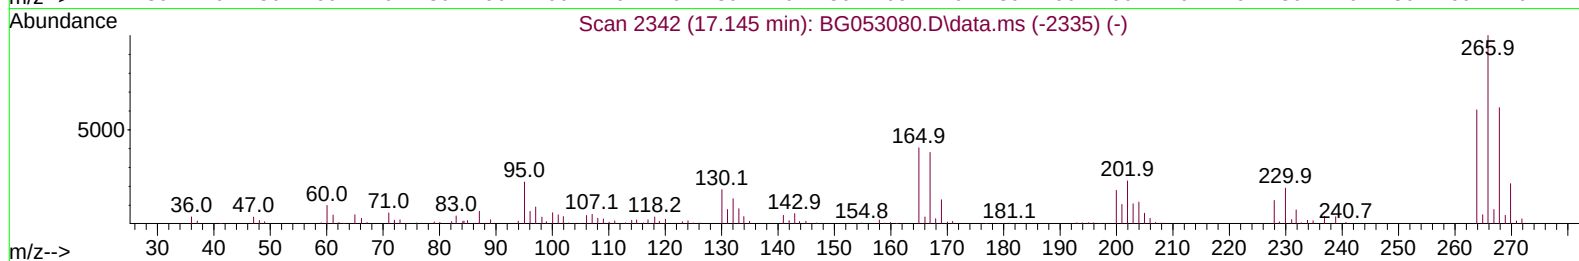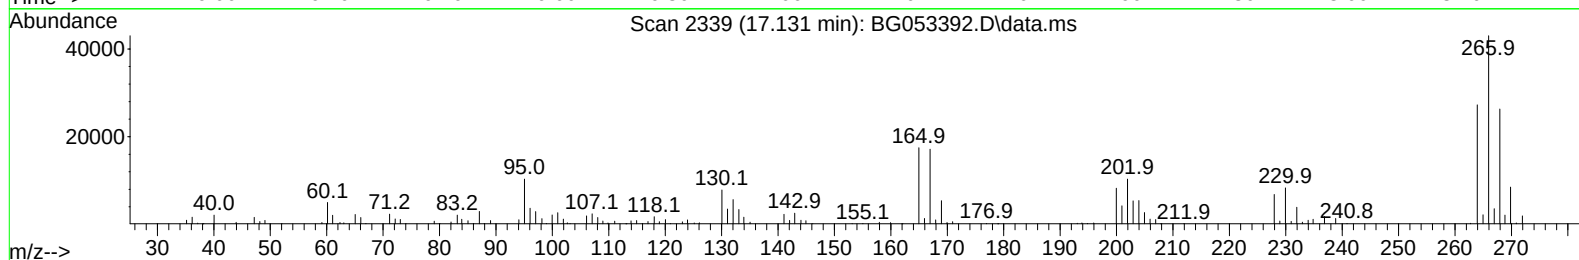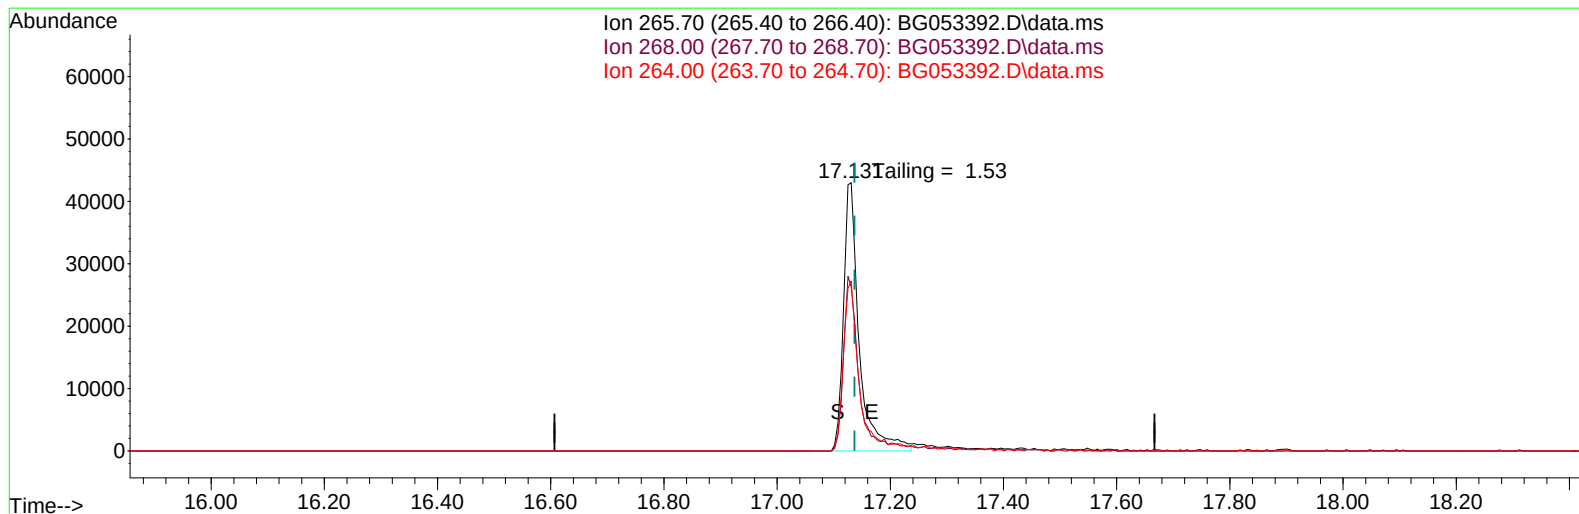

TIC: BG053392.D\data.ms

(70) Pentachlorophenol (C)

17.131min (-0.006) 21922.04 ng




response 86119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.13
264.00	56.60	63.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050222\
Data File : BG053392.D
Acq On : 2 May 2022 10:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 02 16:52:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

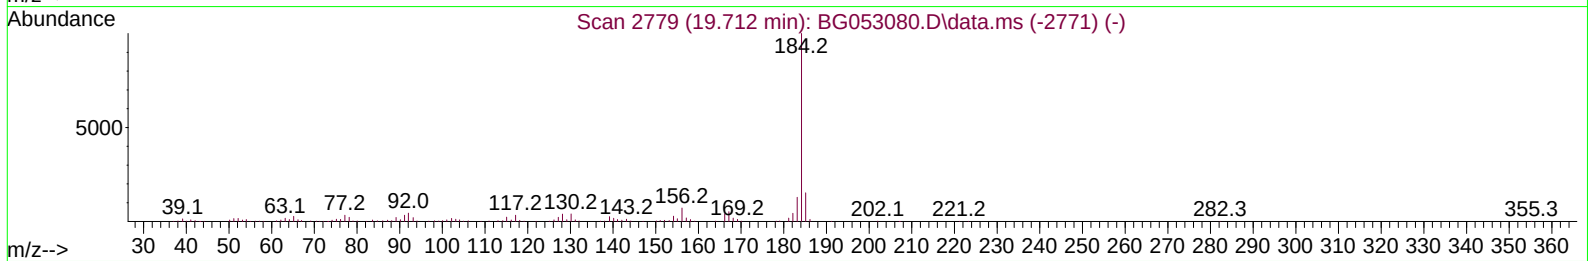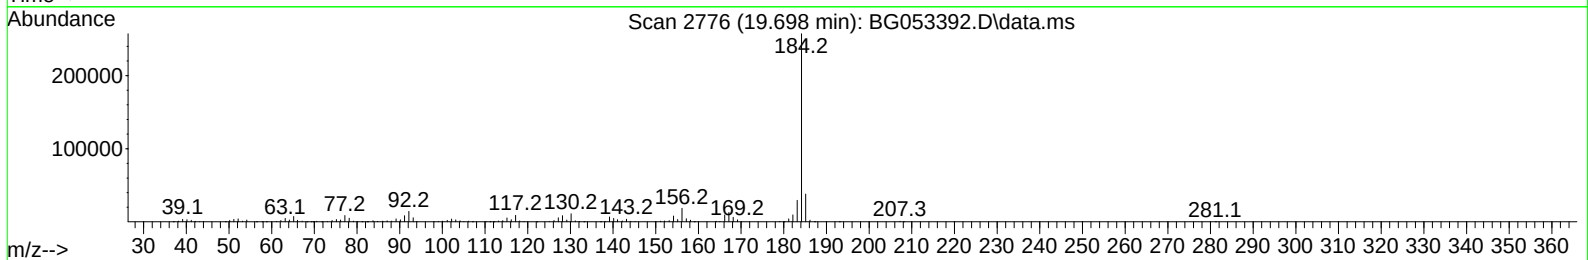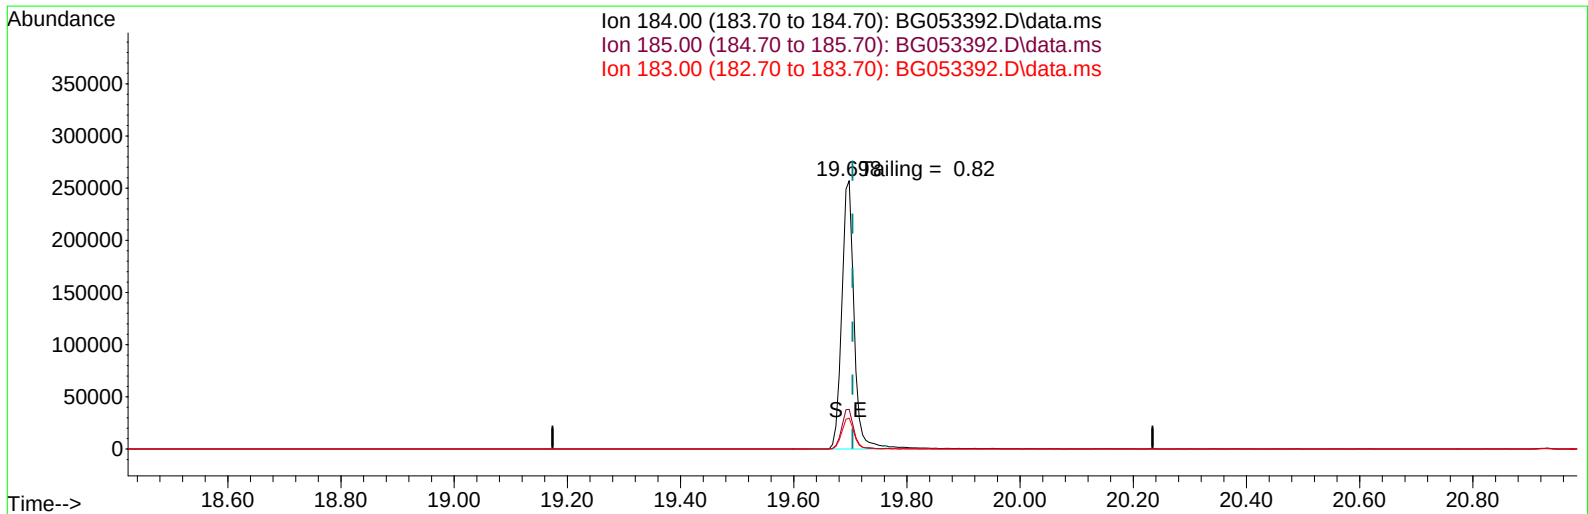

TIC: BG053392.D\data.ms

(77) Benzidine

19.698min (-0.006) 0.00 ng

response 391332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.78
183.00	11.80	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/2/2022	BNA_G	<u>BG053392.D</u>
Compound Name	Response	Retention Time
DDT	232690	20.93
DDD	1013	20.48
DDE	75	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1088	233778	0.47

Instrument :
BNA_G
ClientSampleId :
DFTPP