
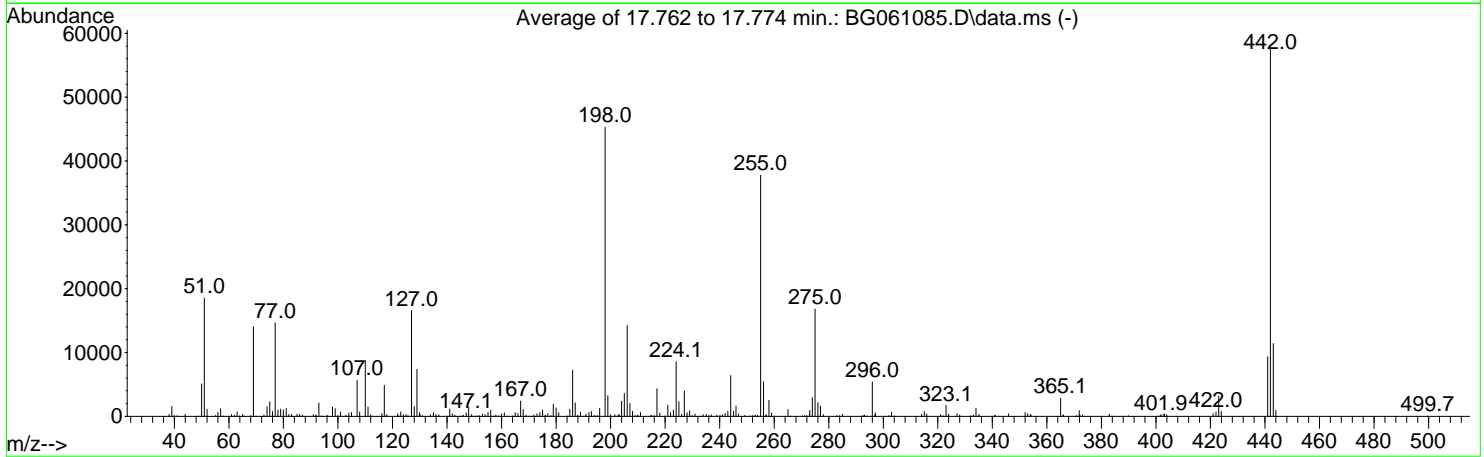


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050224\
 Data File : BG061085.D
 Acq On : 2 May 2024 9:10
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 01 05:11:25 2024

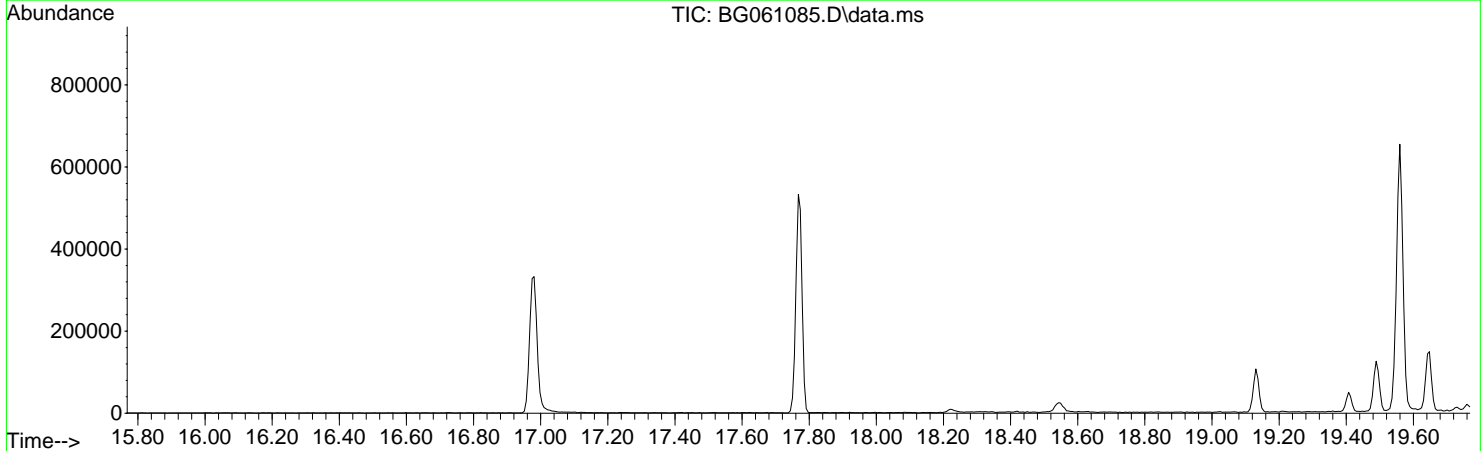

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	18547	PASS
68	69	0.00	2	0.8	116	PASS
69	198	0.00	100	31.0	14035	PASS
70	69	0.00	2	0.4	63	PASS
127	198	10	80	36.6	16557	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	45285	PASS
199	198	5	9	7.2	3239	PASS
275	198	10	60	37.1	16814	PASS
365	198	1	100	6.3	2839	PASS
441	198	0.01	100	20.6	9340	PASS
442	442	50	100	100.0	57613	PASS
443	442	15	24	19.8	11404	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/2/2024	BNA_G	<u>BG061085.D</u>
Compound Name	Response	Retention Time
DDT	240748	20.794
DDD	5321	20.406
DDE	243	19.495
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5564	246312	2.26

Instrument :
 BNA_G
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050224\
 Data File : BG061085.D
 Acq On : 2 May 2024 9:10
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 02 12:18:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 05:11:25 2024
 Response via : Initial Calibration

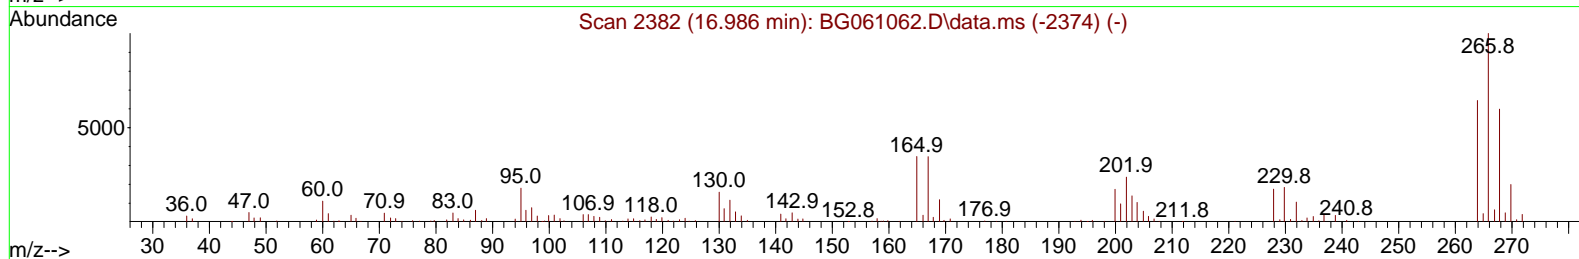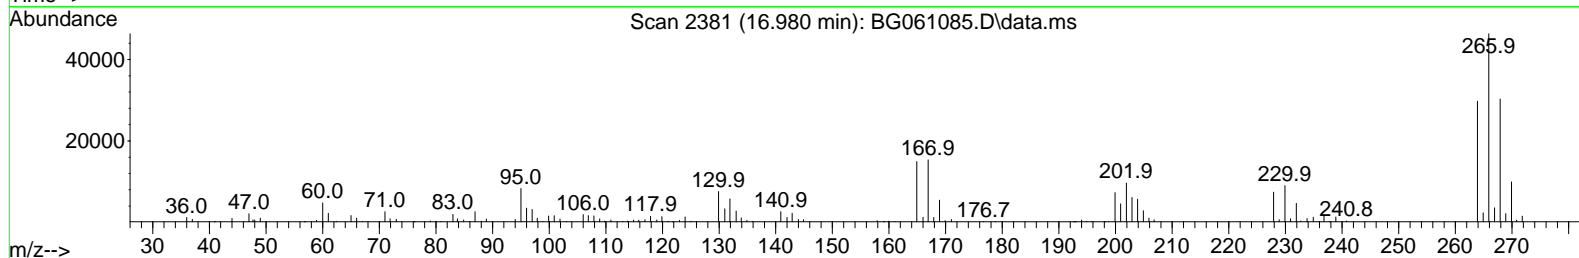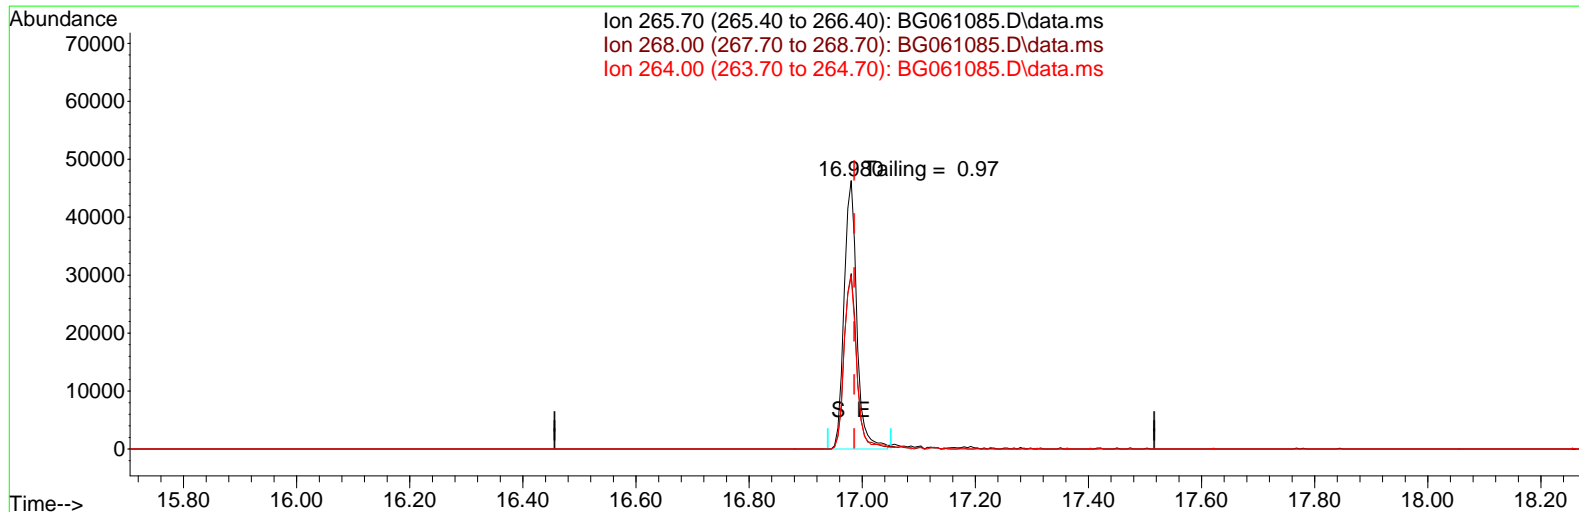

TIC: BG061085.D\data.ms

(70) Pentachlorophenol (C)

16.980min (-0.006) 152357.80 ng




response 72737

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	65.37
264.00	64.40	64.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050224\
 Data File : BG061085.D
 Acq On : 2 May 2024 9:10
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 02 12:18:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 05:11:25 2024
 Response via : Initial Calibration

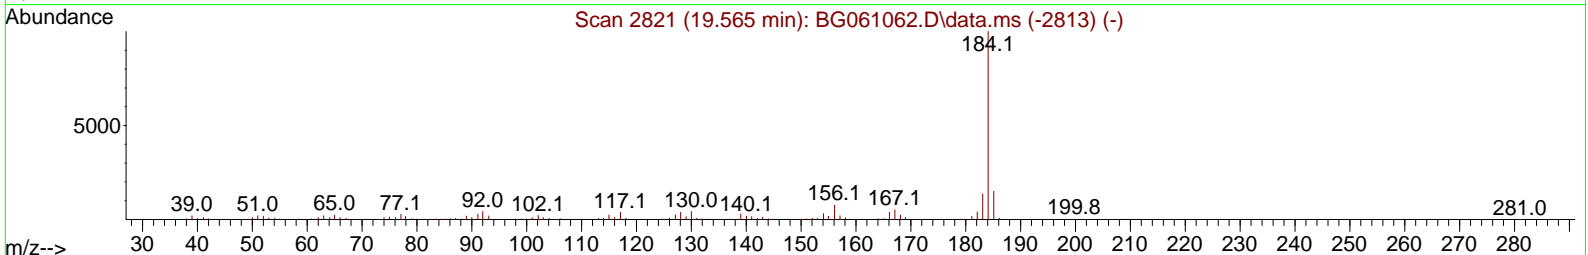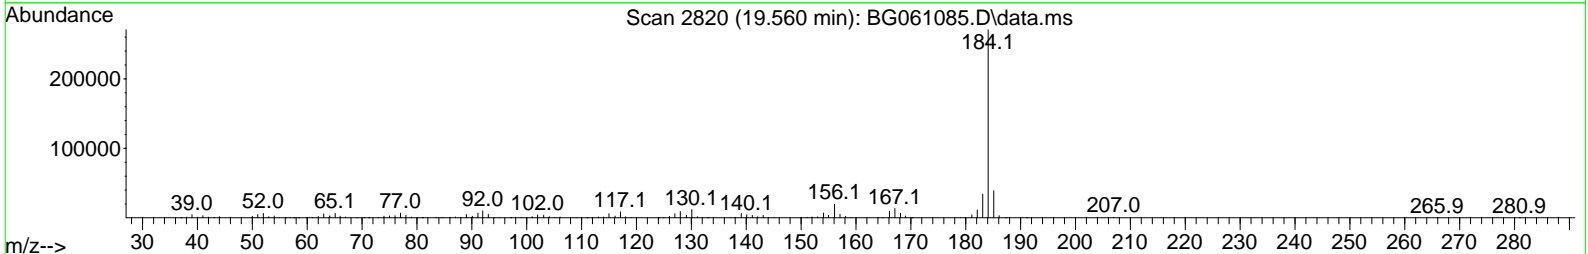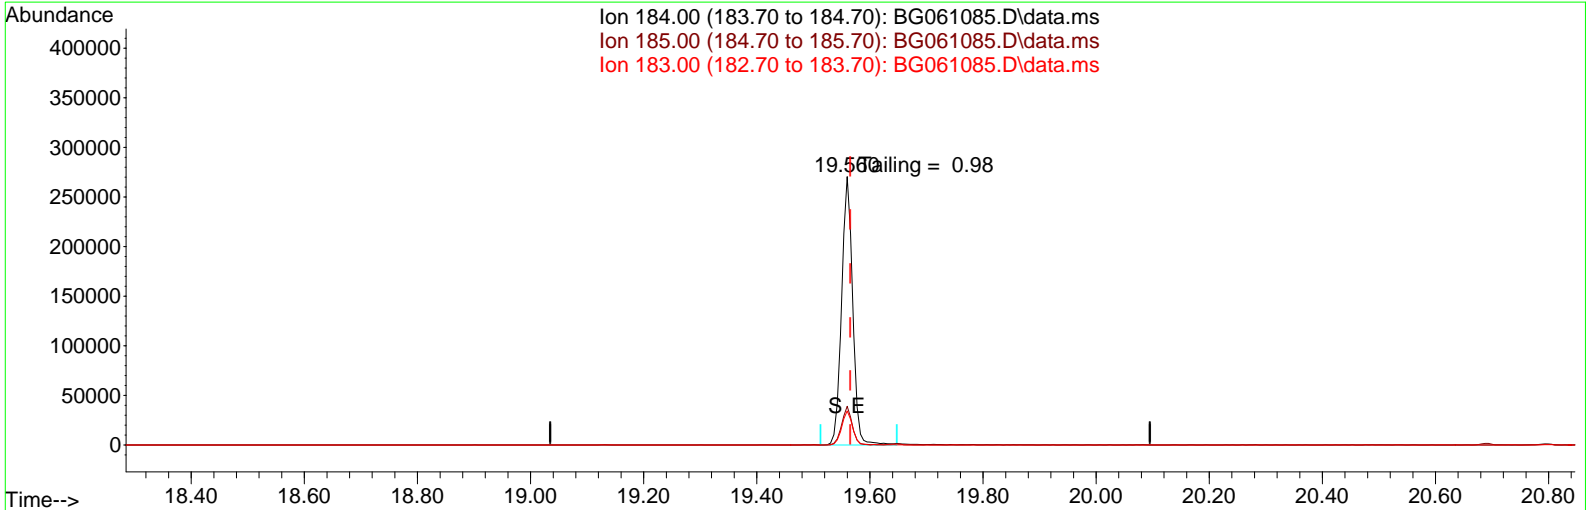

TIC: BG061085.D\data.ms

(77) Benzidine

19.560min (-0.005) 268689.53 ng

response 369176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.44
183.00	13.60	12.70
0.00	0.00	0.00