

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050317\
 Data File : BG026854.D
 Acq On : 3 May 2017 16:46
 Operator : SJ/MA
 Sample : I2871-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAB19

Quant Time: May 04 00:51:04 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 04 00:50:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	164275	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	825032	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	469010	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	906683	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	809544	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	843547	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	23935	6.56	ng/uL	0.00
5) Phenol-d5	7.18	99	535810	36.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	319778	37.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	424068	34.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	445021	36.57	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	225772	32.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	251176	33.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	397296	33.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	600441	37.64	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1249622	33.10	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1625604	34.28	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	197157	28.98	ng/ul	0.00
57) Fluorene-d10	15.61	176	1054461	32.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	146225	26.56	ng/ul	0.00
70) Anthracene-d10	17.45	188	1481758	33.67	ng/ul	0.00
76) Pyrene-d10	19.73	212	1427258	33.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1349000	33.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.07	163	371727	10.06	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050317\
Data File : BG026854.D
Acq On : 3 May 2017 16:46
Operator : SJ/MA
Sample : I2871-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAB19

Quant Time: May 04 00:51:04 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 04 00:50:13 2017
Response via : Initial Calibration

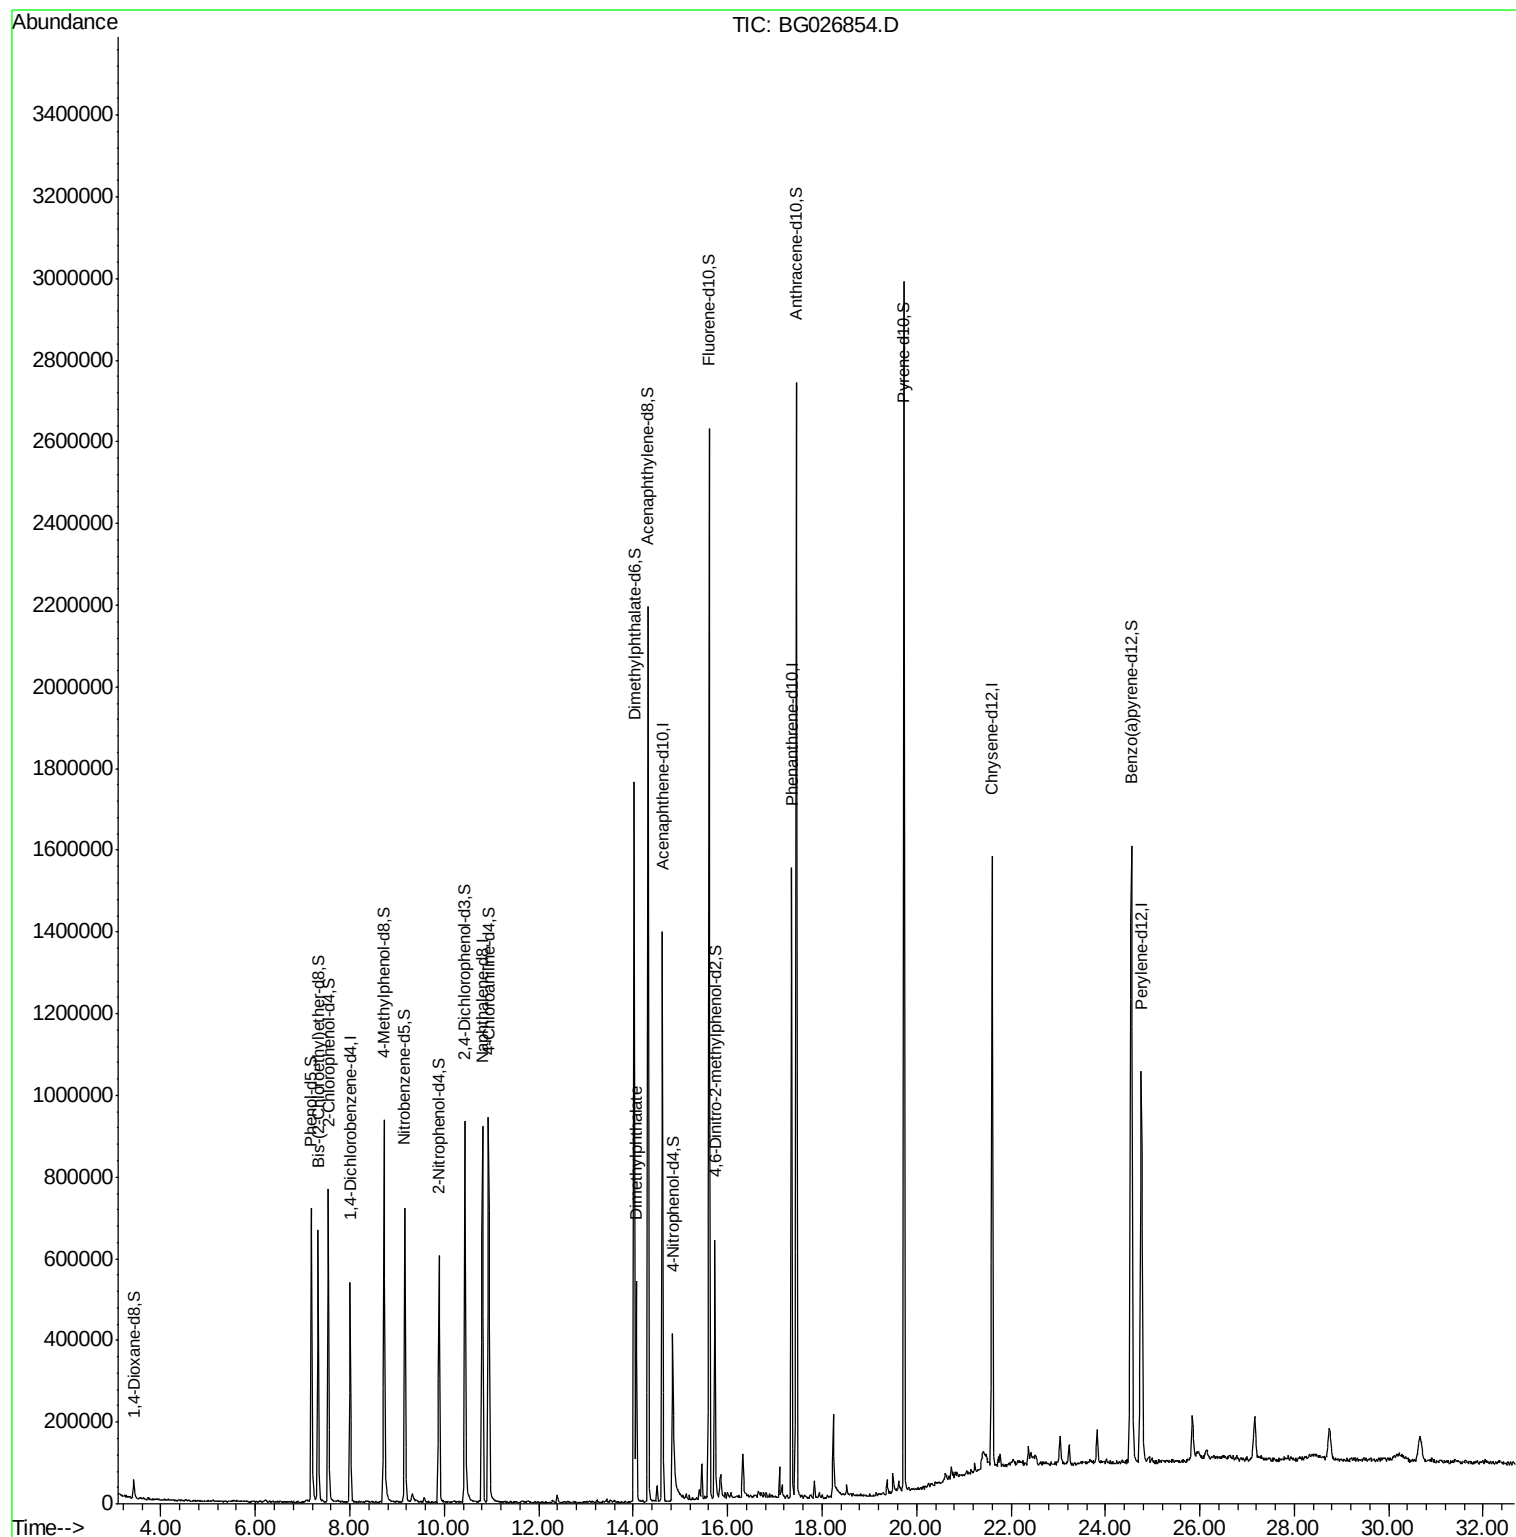

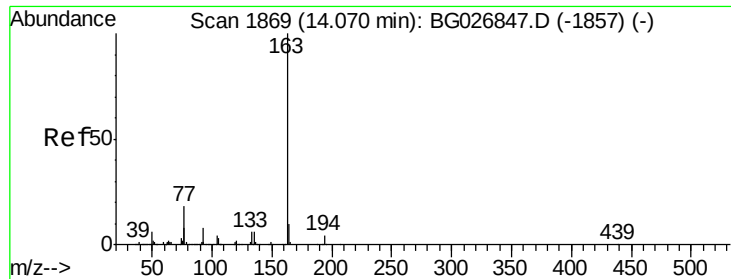

#44

Dimethylphthalate

Concen: 10.06 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG026854.D

Acq: 3 May 2017 16:46

Instrument :

BNA_G

ClientSampleId :

YAB19


Tgt Ion:163 Resp: 371727

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.2 9.0 13.4

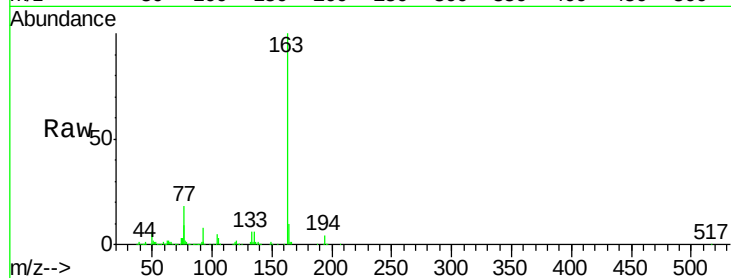

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

