

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050317\
 Data File : BG026855.D
 Acq On : 3 May 2017 17:25
 Operator : SJ/MA
 Sample : I2871-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAB20

Quant Time: May 04 00:51:11 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 04 00:50:13 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	158423	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	794012	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	445020	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	862297	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	788143	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	818629	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.42	96	21446	6.10	ng/uL	0.00
5) Phenol-d5	7.18	99	509511	36.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	305880	36.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	411287	34.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	433107	36.91	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	214502	32.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	242961	33.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	387821	33.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	571643	37.23	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	1195437	33.37	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1566174	34.81	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	192983	29.89	ng/ul	0.00
57) Fluorene-d10	15.61	176	1018679	32.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	139048	26.56	ng/ul	0.00
70) Anthracene-d10	17.45	188	1429961	34.17	ng/ul	0.00
76) Pyrene-d10	19.73	212	1395933	33.56	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	1323053	34.18	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	14.07	163	314058	8.96 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050317\
Data File : BG026855.D
Acq On : 3 May 2017 17:25
Operator : SJ/MA
Sample : I2871-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAB20

Quant Time: May 04 00:51:11 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 04 00:50:13 2017
Response via : Initial Calibration

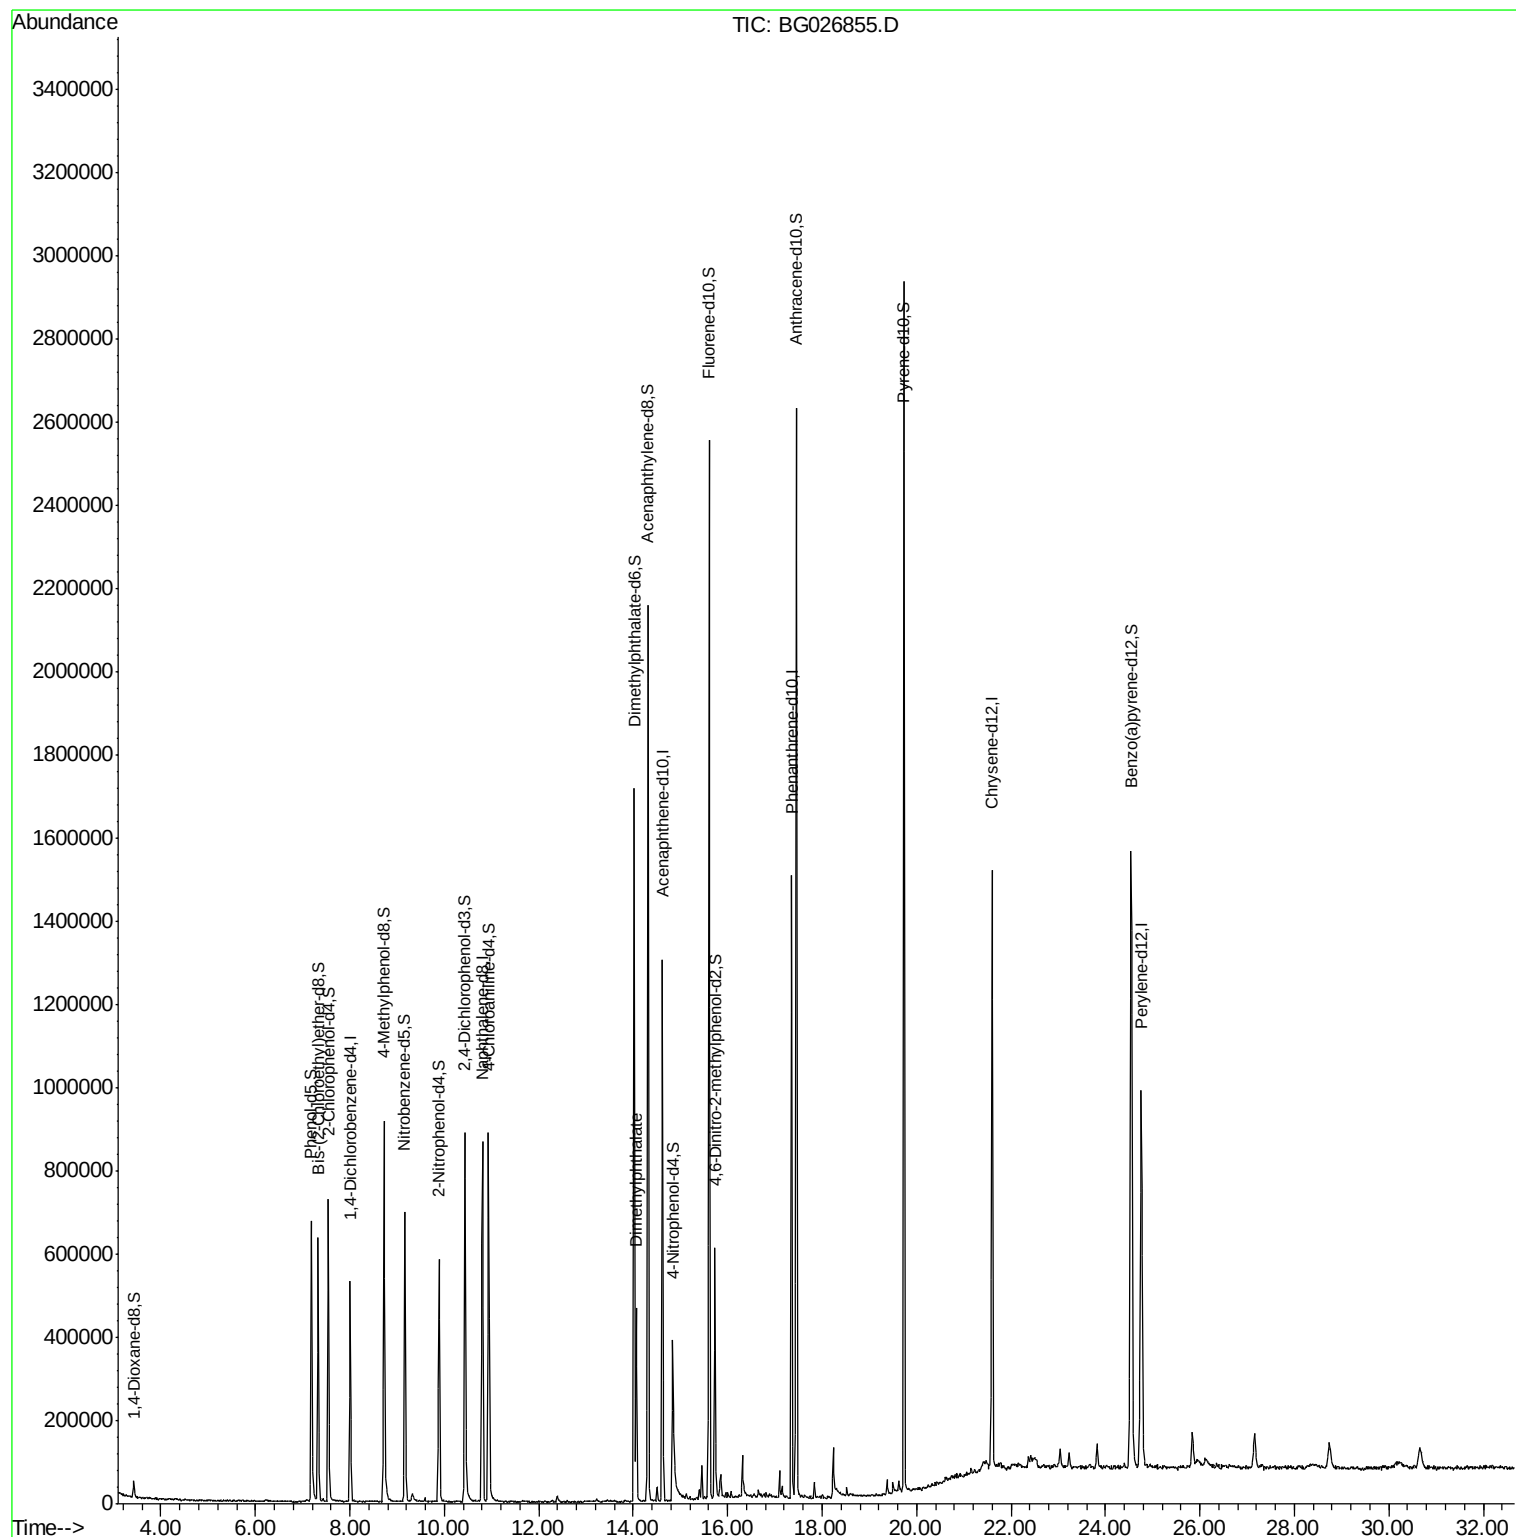

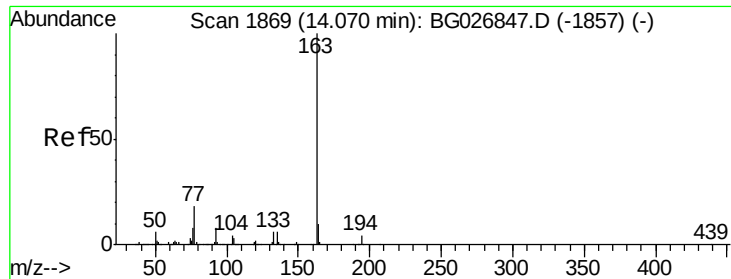

#44

Dimethylphthalate

Concen: 8.96 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG026855.D

Acq: 3 May 2017 17:25

Instrument :

BNA_G

ClientSampleId :

YAB20

Tgt Ion:163 Resp: 314058

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.3 9.0 13.4

