
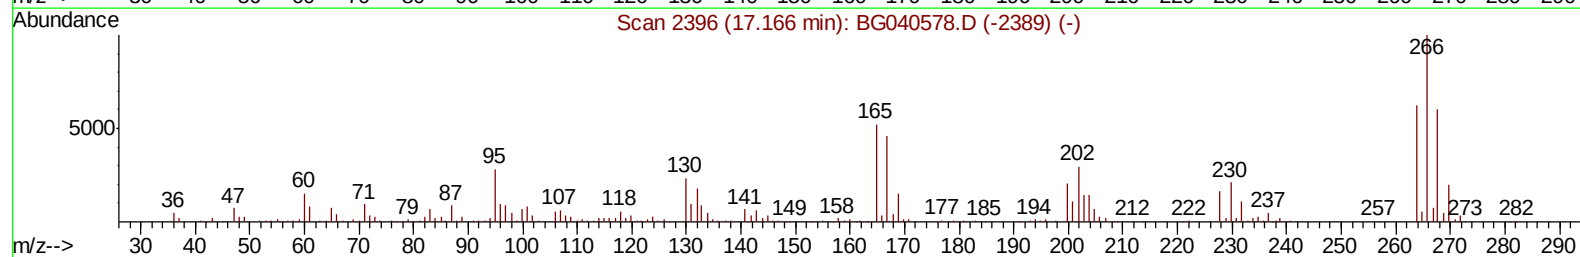
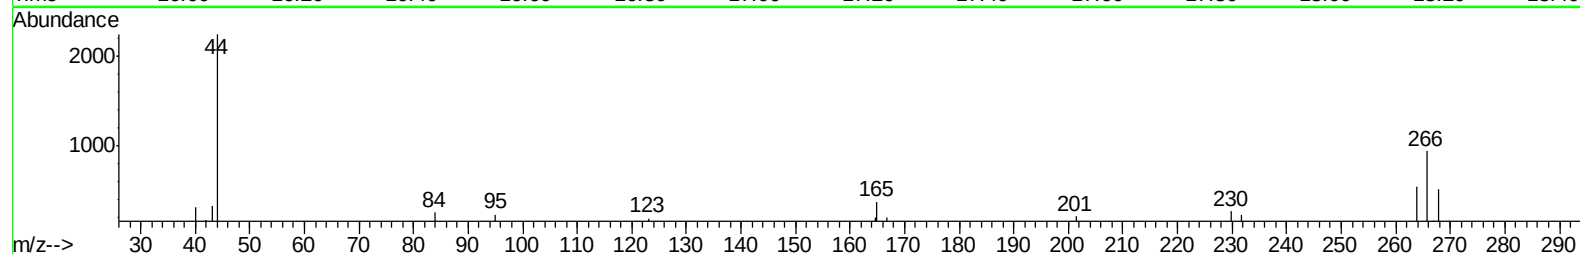


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG050319\
 Data File : BG040743.D
 Acq On : 4 May 2019 3:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 02:08:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

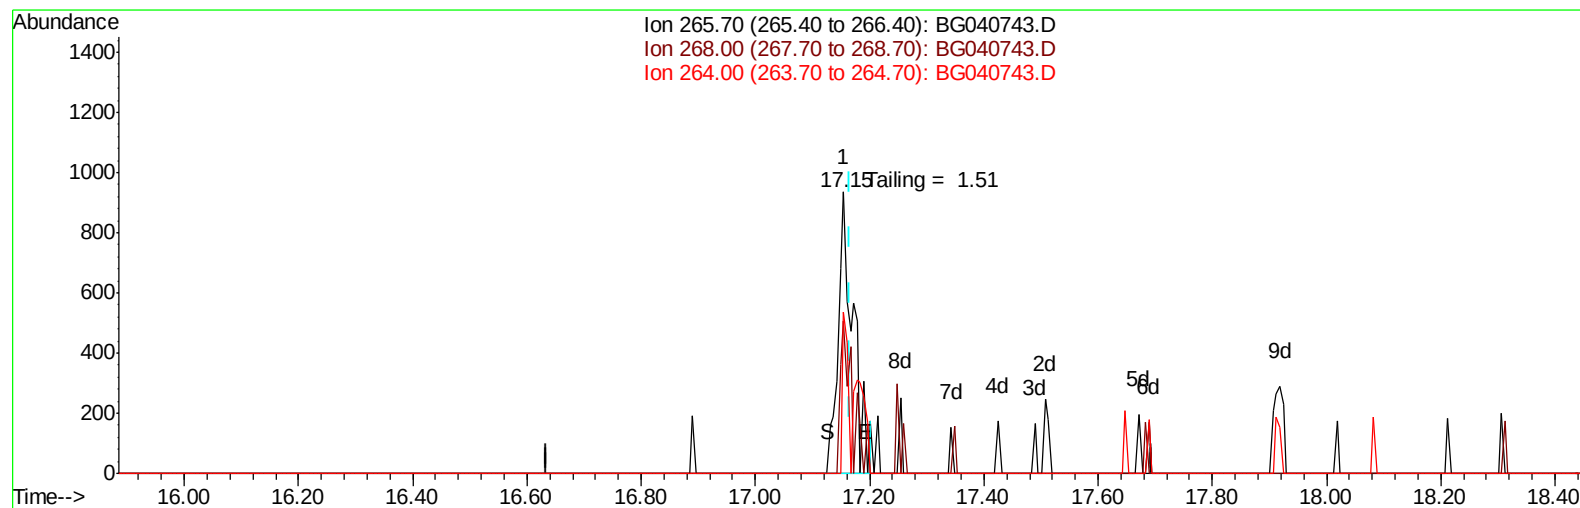

TIC: BG040743.D

(70) Pentachlorophenol (C)




17.155min (-0.011) 392.47ng

response 1784

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	54.27
264.00	62.50	57.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG050319\
 Data File : BG040743.D
 Acq On : 4 May 2019 3:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 02:08:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

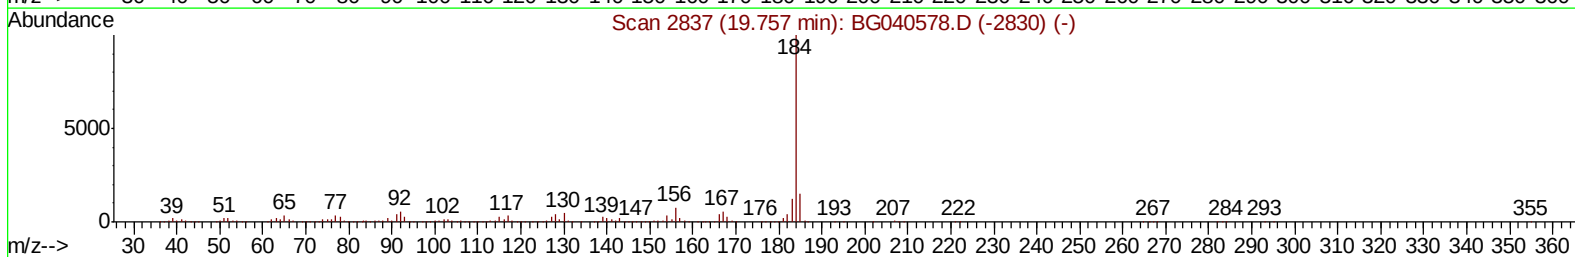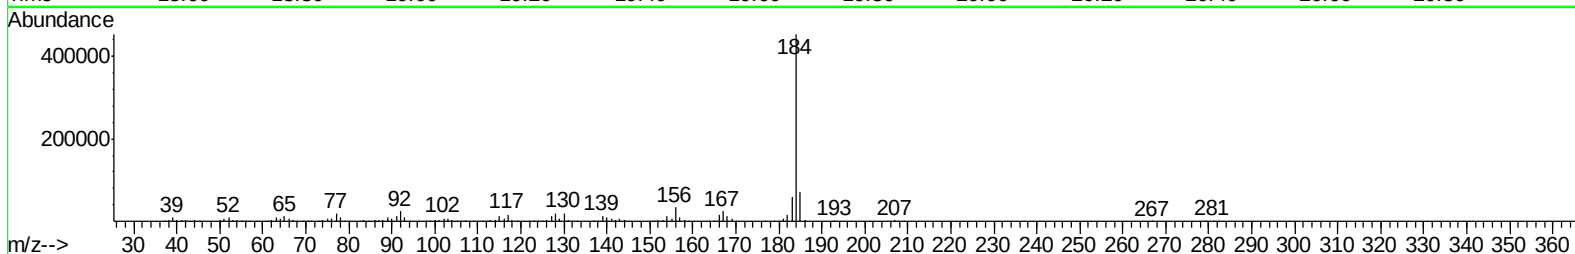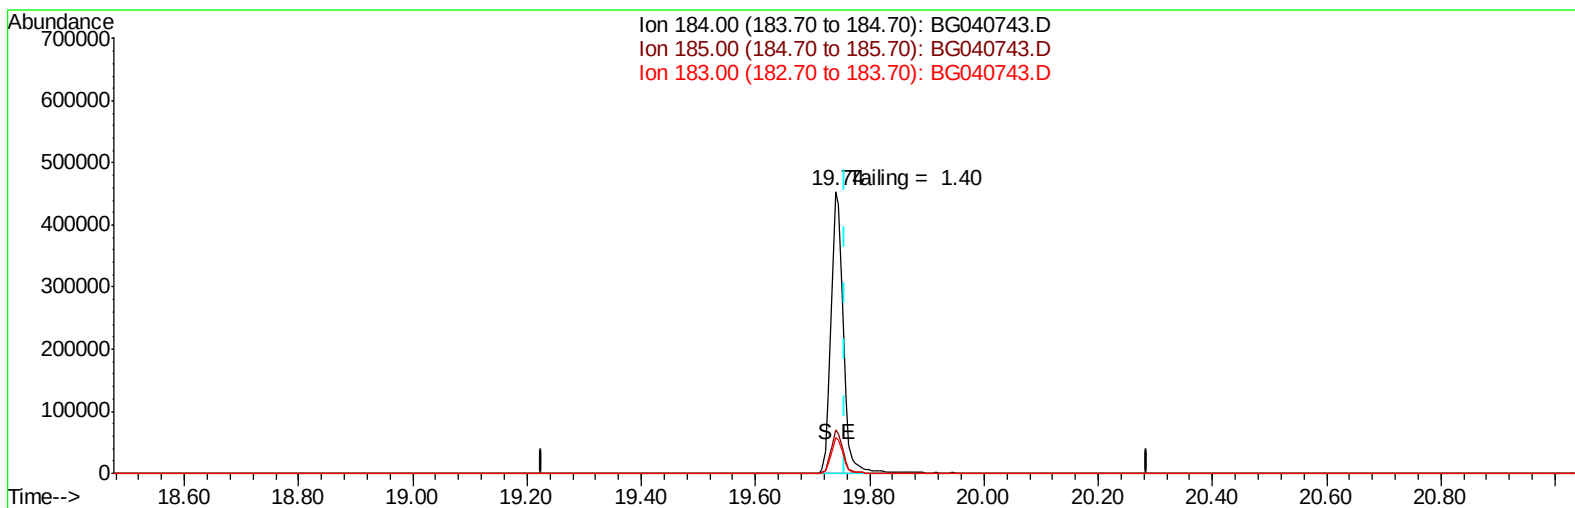

TIC: BG040743.D

(77) Benzidine

19.740min (-0.017) 0.00ng

response 668998

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.51
183.00	12.70	12.90
0.00	0.00	0.00