


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG050319\
 Data File : BG040724.D
 Acq On : 3 May 2019 14:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

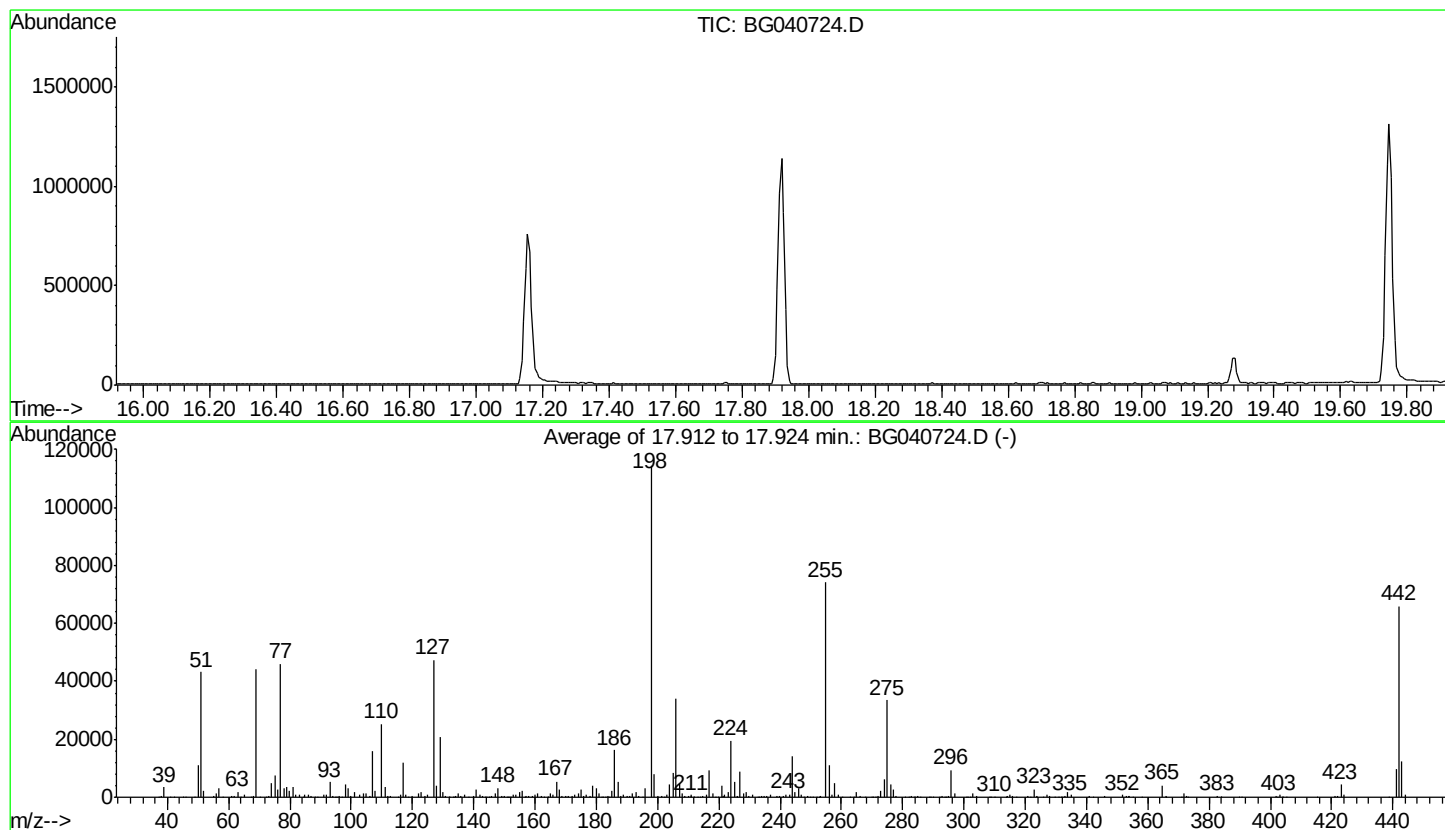

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	43218	PASS
68	69	0.00	2	0.6	255	PASS
69	198	0.00	100	38.5	44021	PASS
70	69	0.00	2	0.4	185	PASS
127	198	10	80	41.4	47349	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	114448	PASS
199	198	5	9	6.8	7782	PASS
275	198	10	60	29.2	33474	PASS
365	198	1	100	3.7	4185	PASS
441	198	0.01	100	8.6	9880	PASS
442	198	50	100	57.6	65976	PASS
443	442	15	24	18.5	12235	PASS