


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG050319\
 Data File : BG040743.D
 Acq On : 4 May 2019 3:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

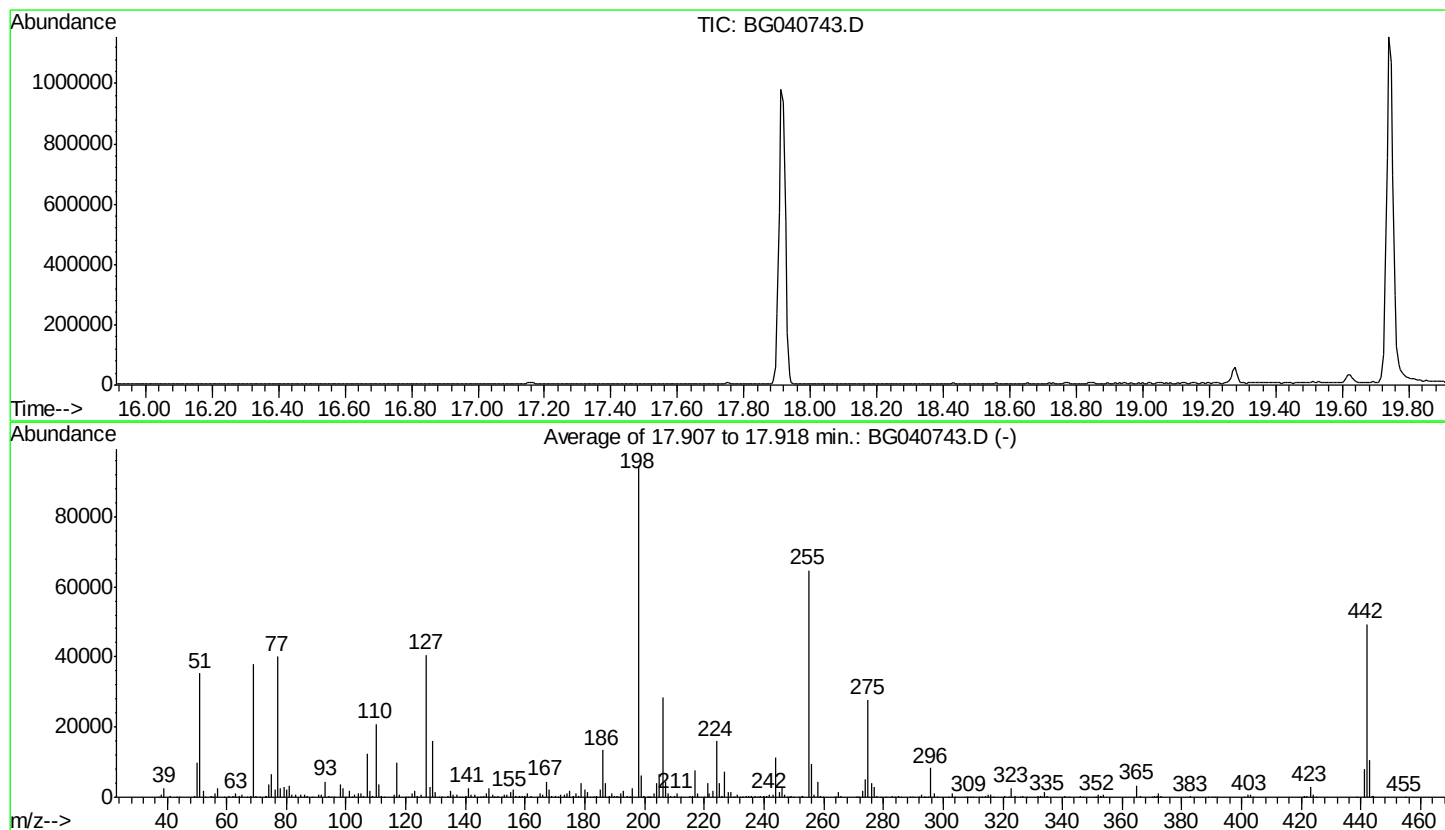

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	35354	PASS
68	69	0.00	2	0.7	268	PASS
69	198	0.00	100	40.1	37901	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	42.9	40554	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94528	PASS
199	198	5	9	6.6	6242	PASS
275	198	10	60	29.5	27896	PASS
365	198	1	100	3.6	3383	PASS
441	198	0.01	100	8.4	7919	PASS
442	198	50	100	52.2	49314	PASS
443	442	15	24	21.7	10686	PASS