
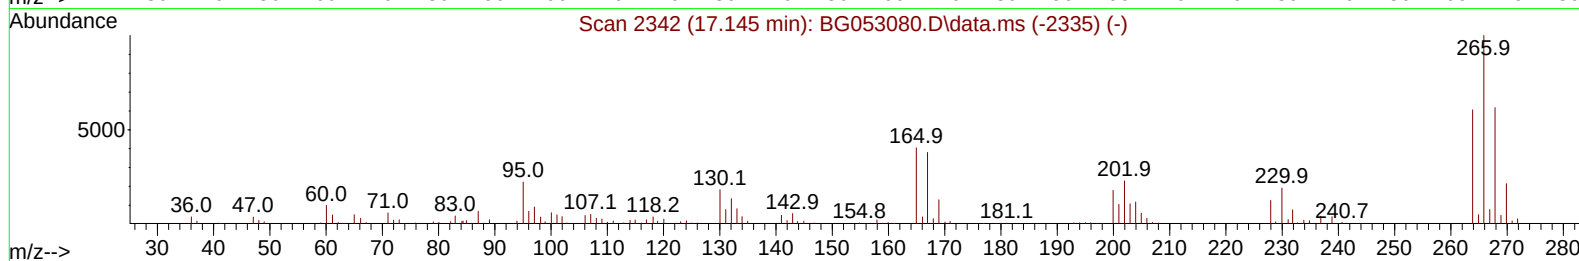
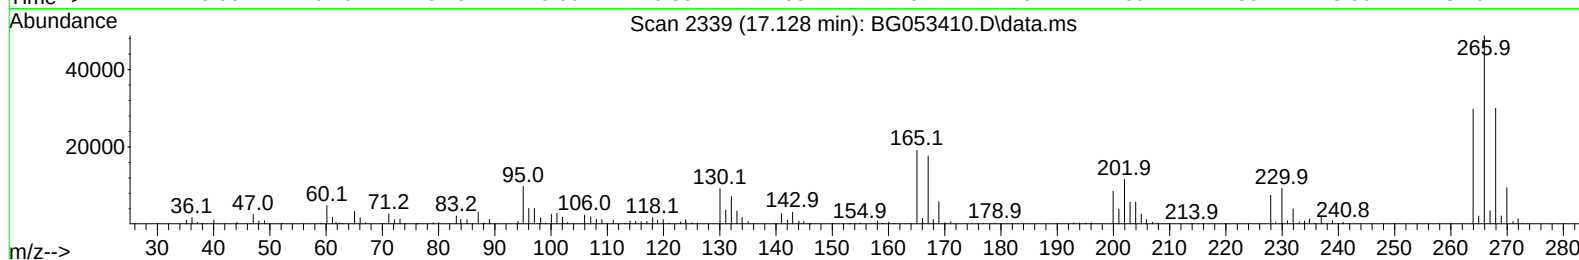


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050322\
Data File : BG053410.D
Acq On : 3 May 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:09:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 06:03:03 2022
Response via : Initial Calibration

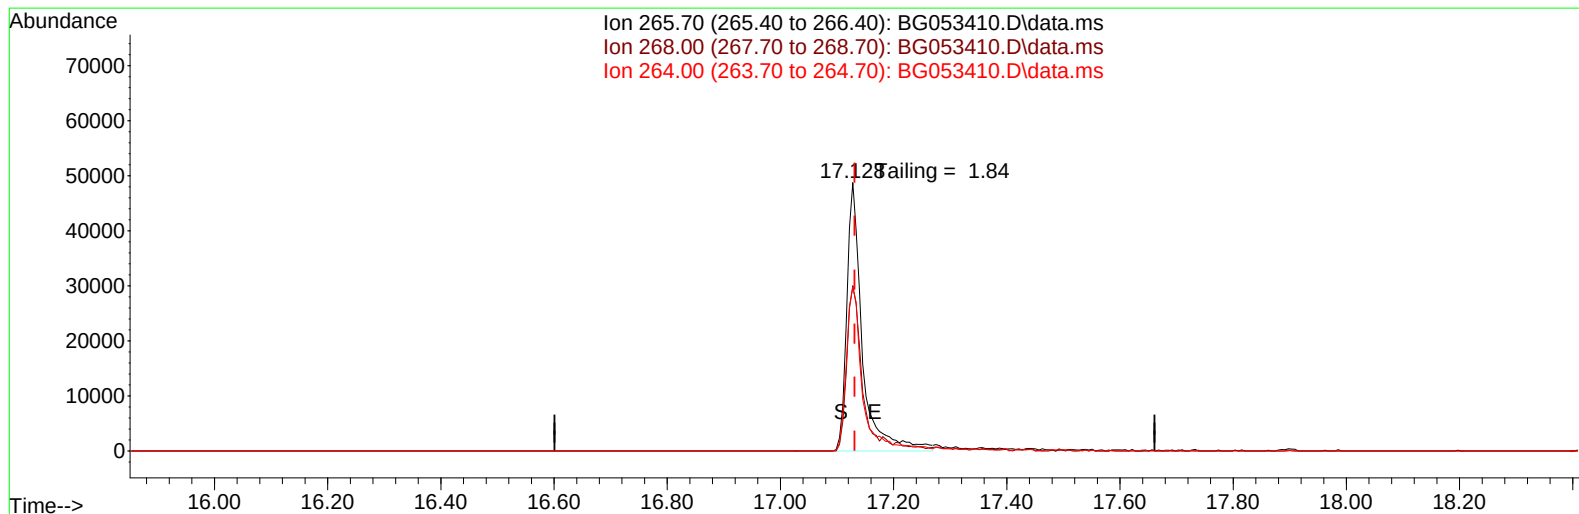

TIC: BG053410.D\data.ms

(70) Pentachlorophenol (C)




17.128min (-0.003) 32991.20 ng

response 89071

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.59
264.00	56.60	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050322\
Data File : BG053410.D
Acq On : 3 May 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 09:09:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 06:03:03 2022
Response via : Initial Calibration

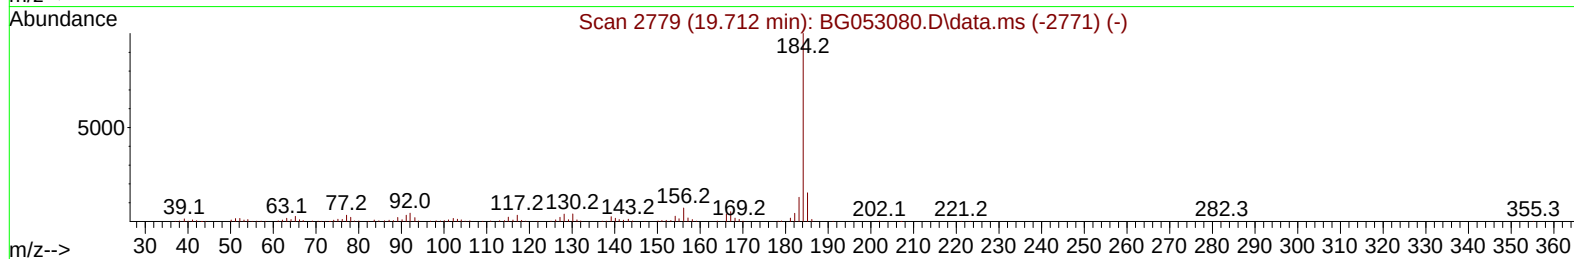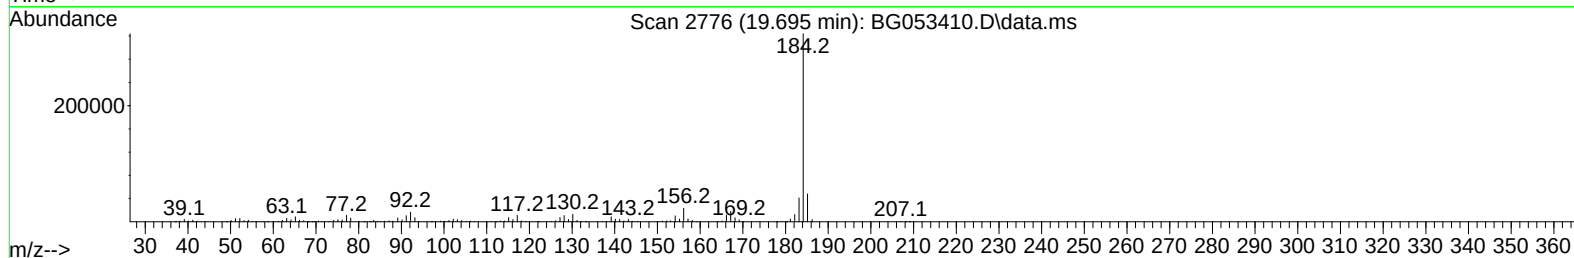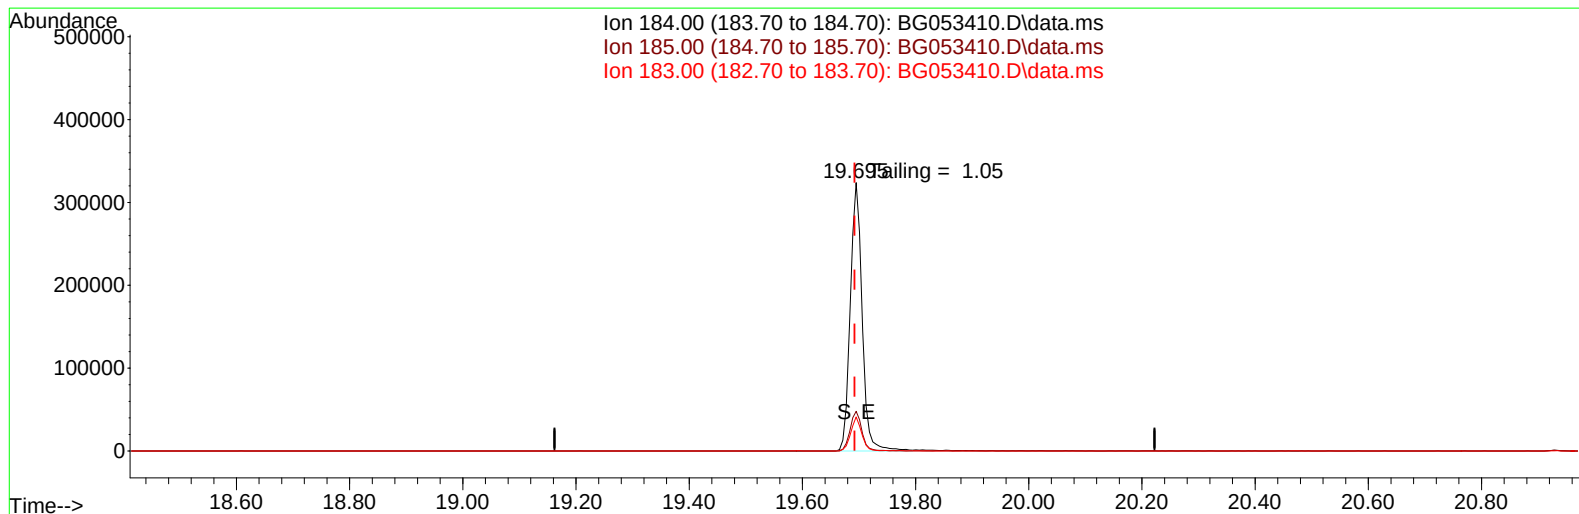

TIC: BG053410.D\data.ms

(77) Benzidine

19.695min (+ 0.003) 0.00 ng

response 472459

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.83
183.00	11.80	12.69
0.00	0.00	0.00