
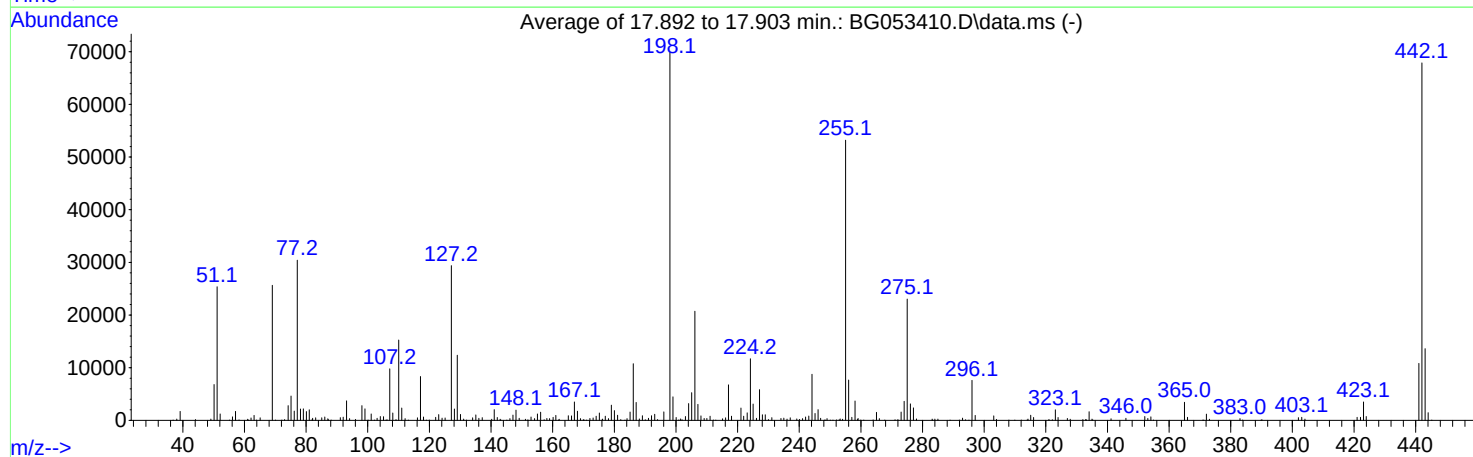


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050322\
 Data File : BG053410.D
 Acq On : 3 May 2022 9:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 06:03:03 2022

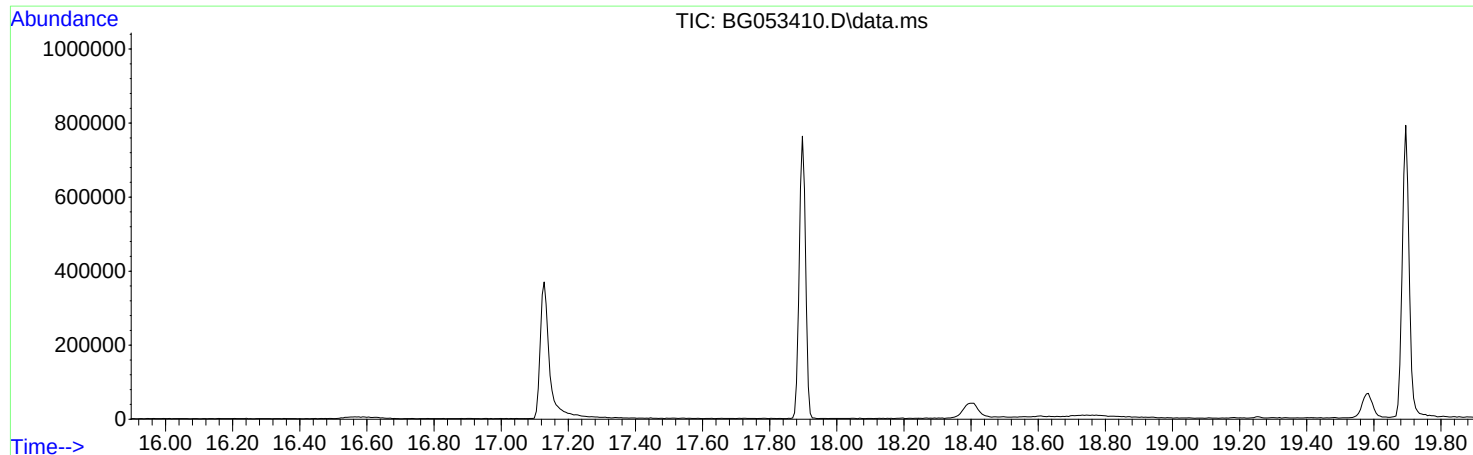




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	25371	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.7	25645	PASS
70	69	0.00	2	0.3	71	PASS
127	198	10	80	42.1	29397	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69853	PASS
199	198	5	9	6.4	4477	PASS
275	198	10	60	33.0	23035	PASS
365	198	1	100	4.9	3428	PASS
441	198	0.01	100	15.5	10806	PASS
442	442	50	100	100.0	67888	PASS
443	442	15	24	20.1	13617	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050322\
Data File : BG053410.D
Acq On : 3 May 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 04 09:09:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 06:03:03 2022
Response via : Initial Calibration

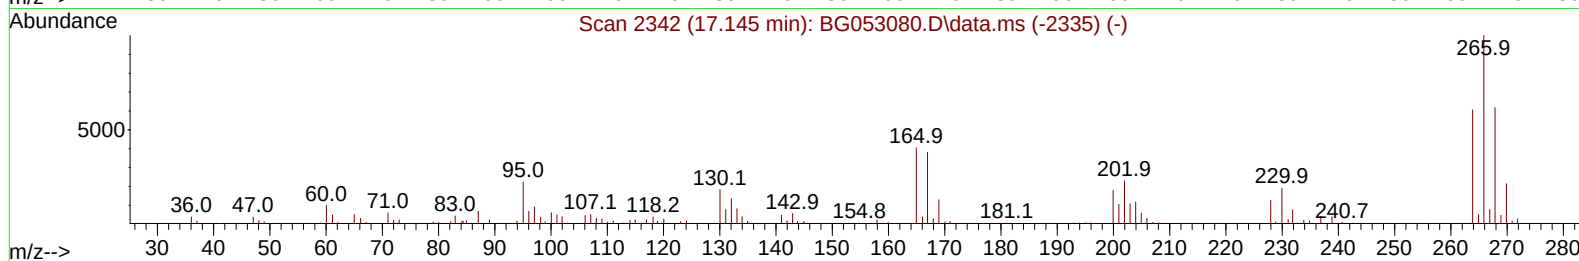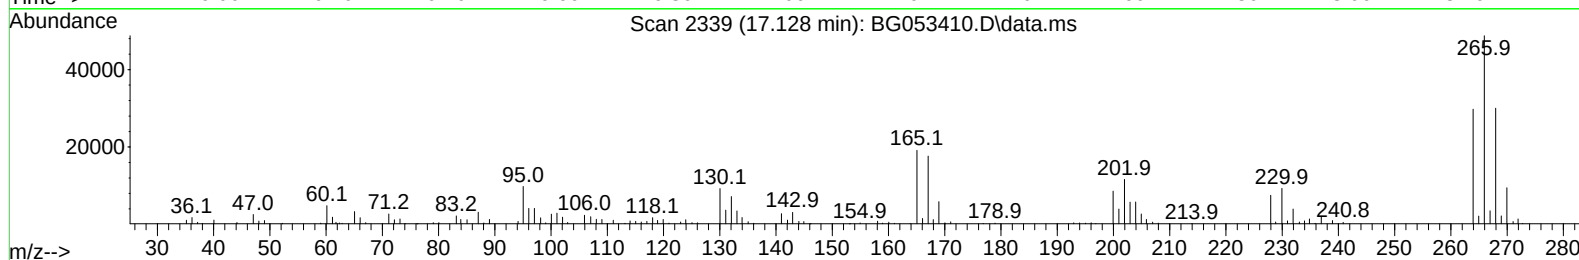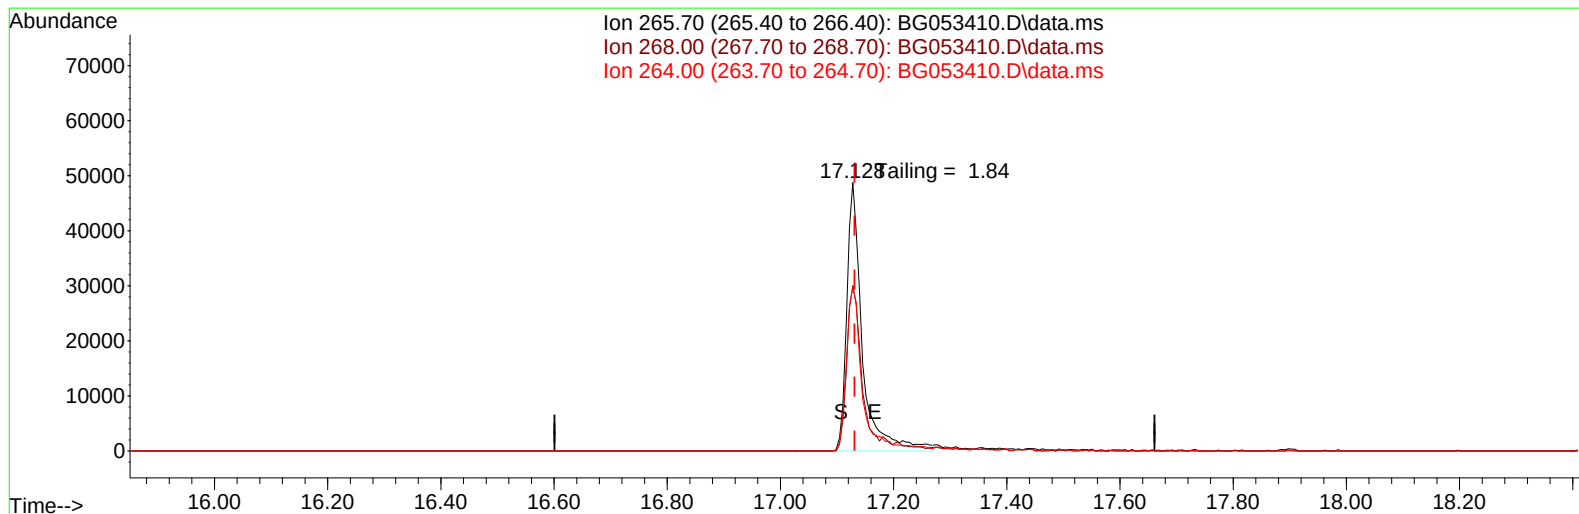

TIC: BG053410.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.003) 32991.20 ng




response 89071

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.59
264.00	56.60	61.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050322\
Data File : BG053410.D
Acq On : 3 May 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 04 09:09:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 06:03:03 2022
Response via : Initial Calibration

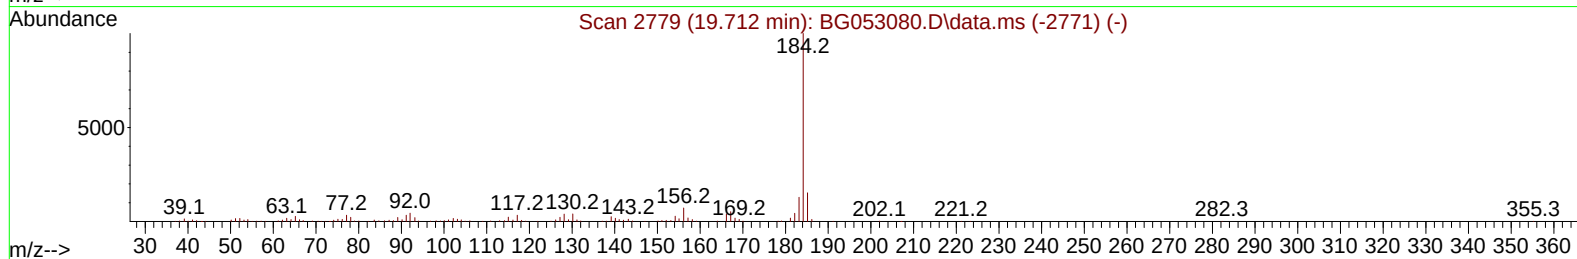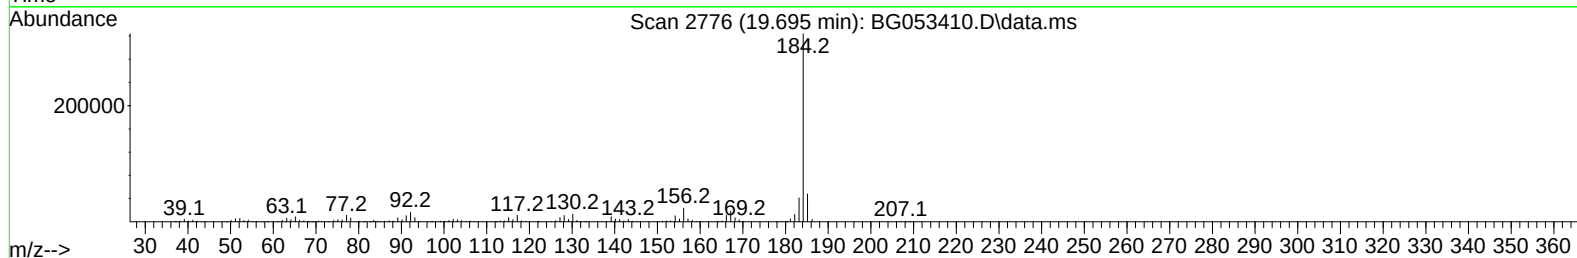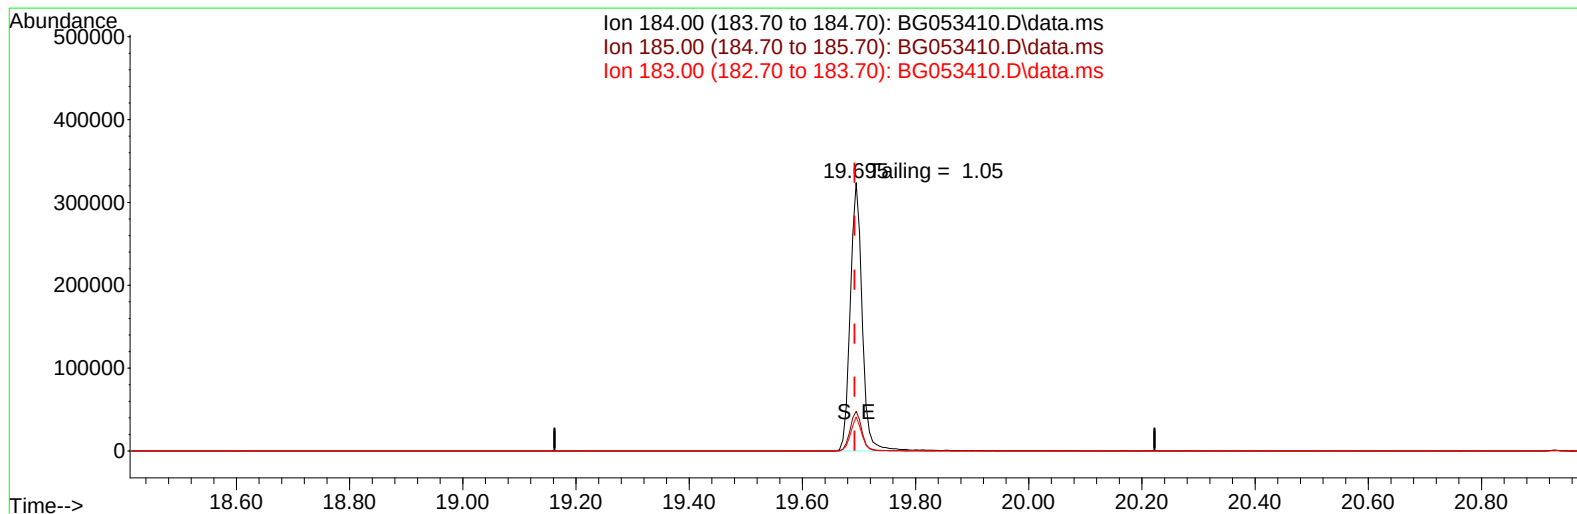

TIC: BG053410.D\data.ms

(77) Benzidine

19.695min (+ 0.003) 0.00 ng

response 472459

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.83
183.00	11.80	12.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/3/2022	BNA_G	<u>BG053410.D</u>
Compound Name	Response	Retention Time
DDT	264168	20.929
DDD	3019	20.488
DDE	162	19.989
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3181	267349	1.19

Instrument :
BNA_G
ClientSampleId :
DFTPP