

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050417\
 Data File : BG026869.D
 Acq On : 4 May 2017 12:49
 Operator : SJ/MA
 Sample : I2871-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 YAB22

Quant Time: May 04 17:52:21 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 04 17:40:44 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	165861	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	801101	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	424662	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	787351	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	710934	20.00	ng/ul	0.00
83) Perylene-d12	24.76	264	741148	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	11221	3.05	ng/uL	0.00
5) Phenol-d5	7.19	99	239786	16.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	160862	18.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.54	132	208231	16.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	220429	17.94	ng/ul	0.00
19) Nitrobenzene-d5	9.17	128	108285	16.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	123466	16.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.43	165	184155	15.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	270149	17.44	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	632435	18.50	ng/ul	0.00
46) Acenaphthylene-d8	14.31	160	724417	16.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	65063	10.56	ng/ul	0.00
57) Fluorene-d10	15.60	176	528765	17.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	57107	11.94	ng/ul	0.00
70) Anthracene-d10	17.45	188	690104	18.06	ng/ul	0.00
76) Pyrene-d10	19.73	212	530807	14.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.54	264	396095	11.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.07	163	214722	6.42	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050417\
Data File : BG026869.D
Acq On : 4 May 2017 12:49
Operator : SJ/MA
Sample : I2871-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAB22

Quant Time: May 04 17:52:21 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 04 17:40:44 2017
Response via : Initial Calibration

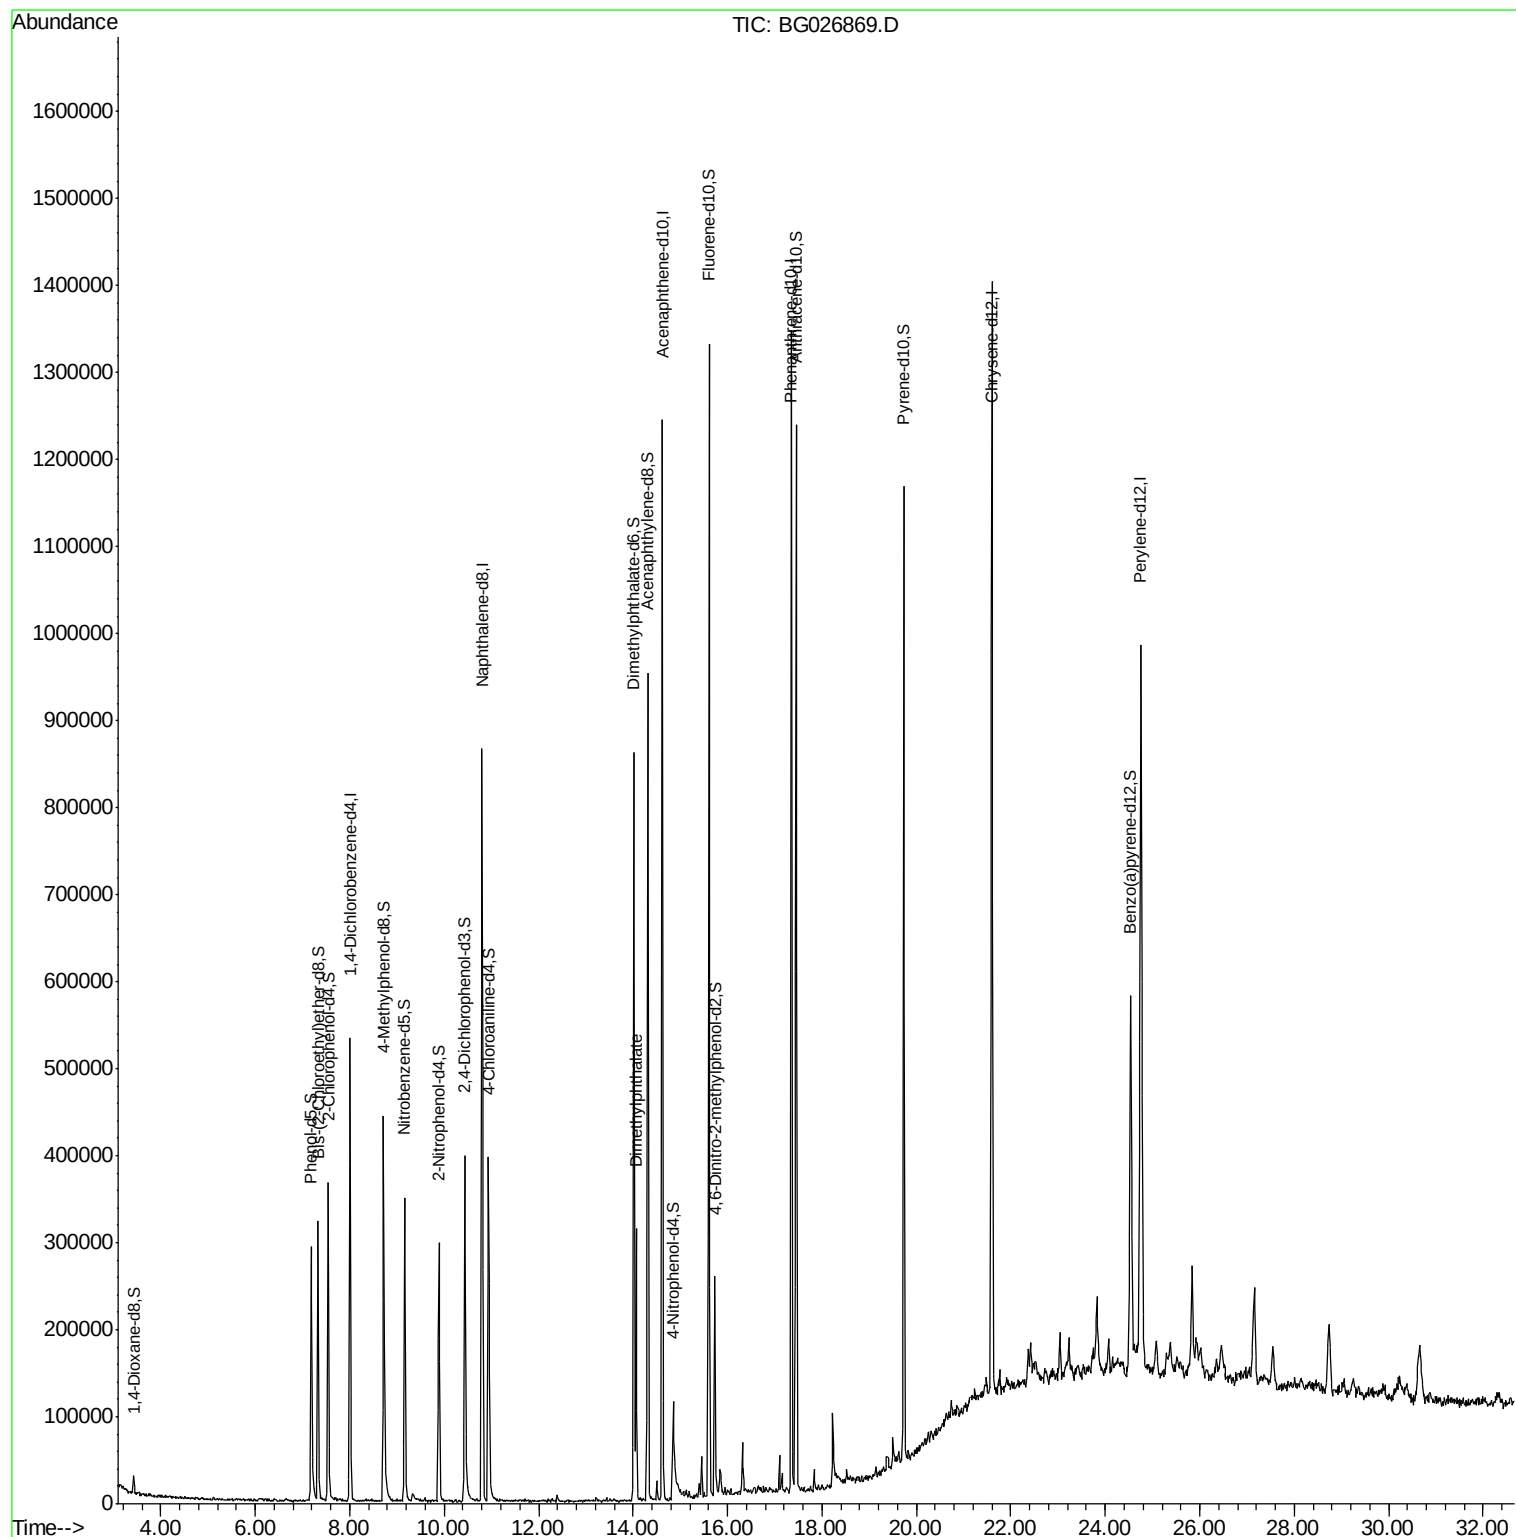

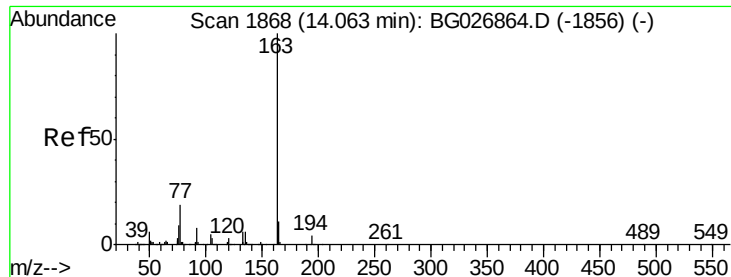

#44

Dimethylphthalate

Concen: 6.42 ng/ul

RT: 14.07 min Scan# 1868

Delta R.T. 0.00 min

Lab File: BG026869.D

Acq: 4 May 2017 12:49

Instrument :

BNA_G

ClientSampleId :

YAB22

Tgt Ion:163 Resp: 214722

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.0

164 10.3 9.0 13.4

