
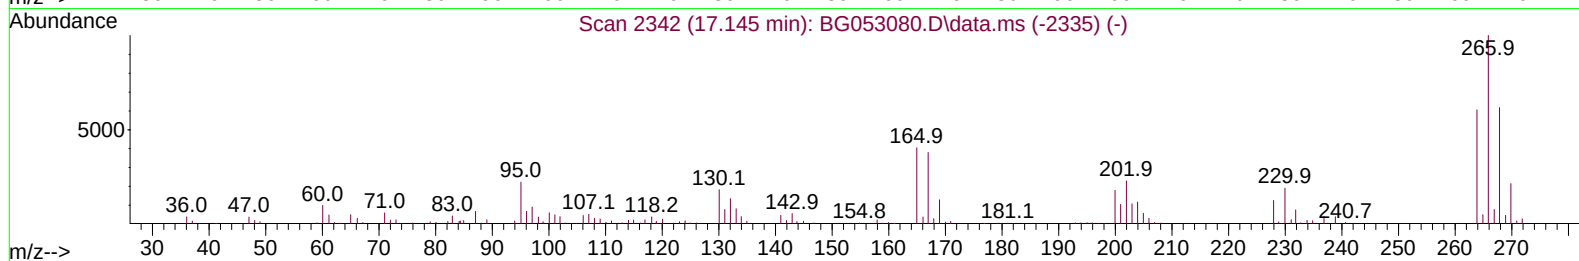
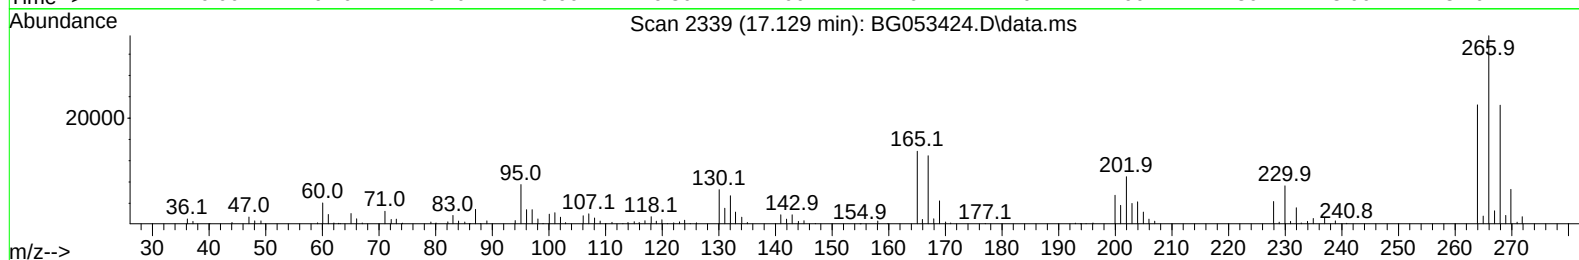


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050422\
Data File : BG053424.D
Acq On : 4 May 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 18:16:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 18:06:54 2022
Response via : Initial Calibration

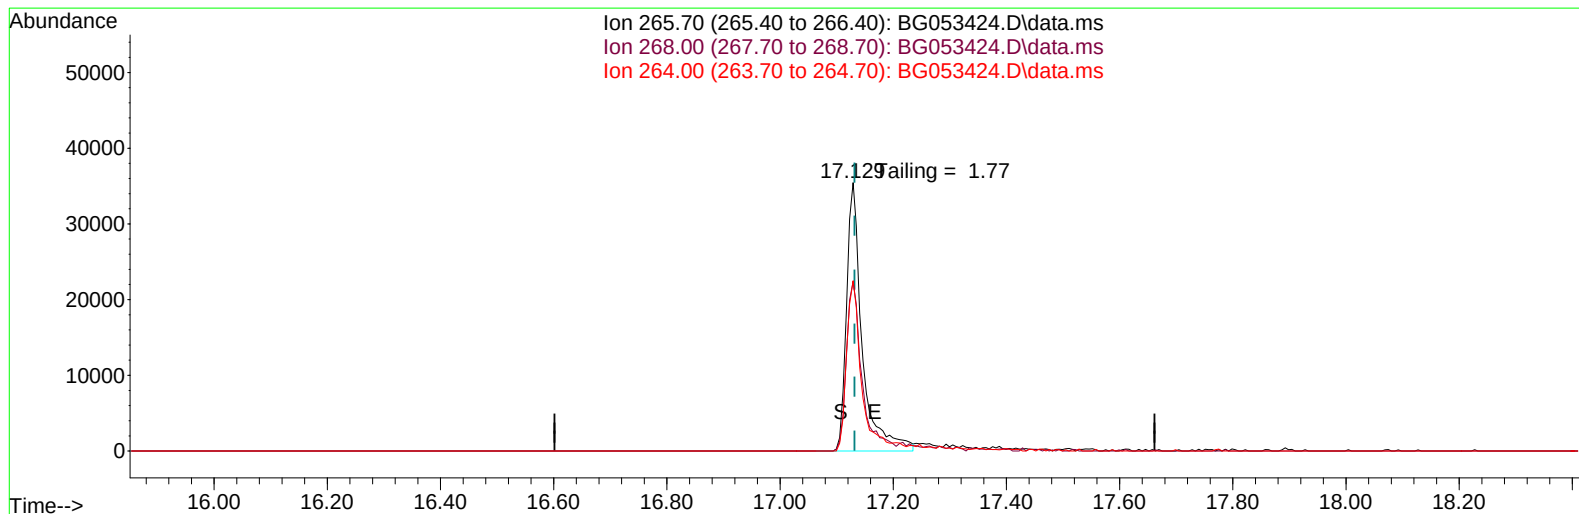

TIC: BG053424.D\data.ms

(70) Pentachlorophenol (C)




17.129min (-0.003) 21325.43 ng

response 70837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	63.22
264.00	56.60	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050422\
 Data File : BG053424.D
 Acq On : 4 May 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 04 18:16:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 18:06:54 2022
 Response via : Initial Calibration

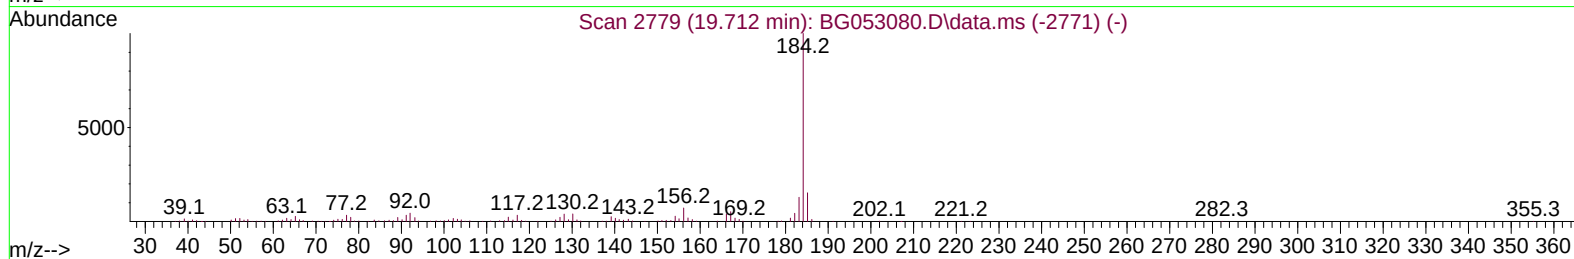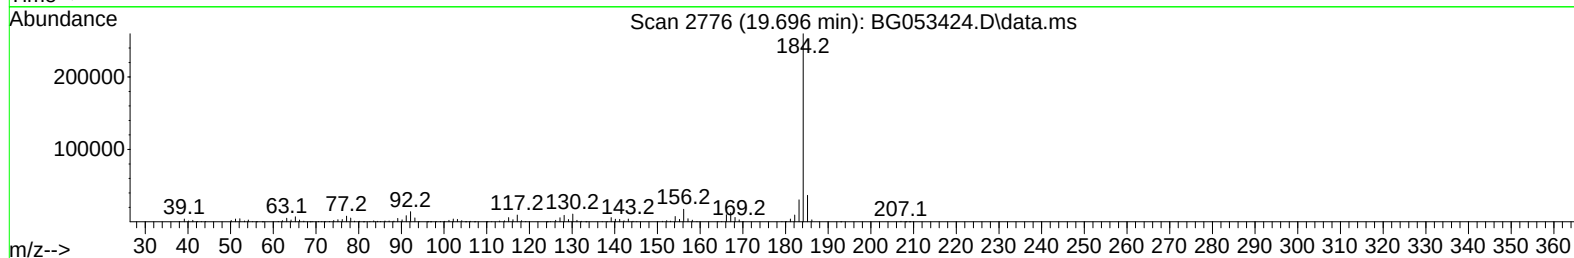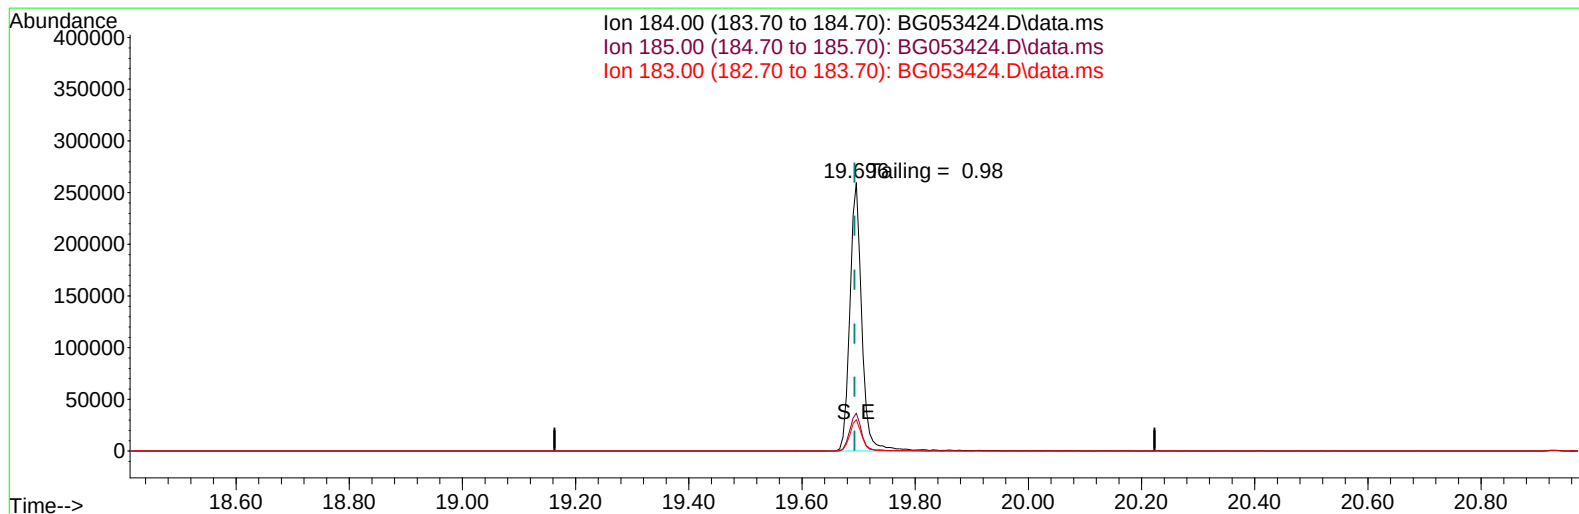

TIC: BG053424.D\data.ms

(77) Benzidine

19.696min (+ 0.003) 0.00 ng

response 376453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.80	11.73
0.00	0.00	0.00