


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050422\
 Data File : BG053424.D
 Acq On : 4 May 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 04 18:06:54 2022

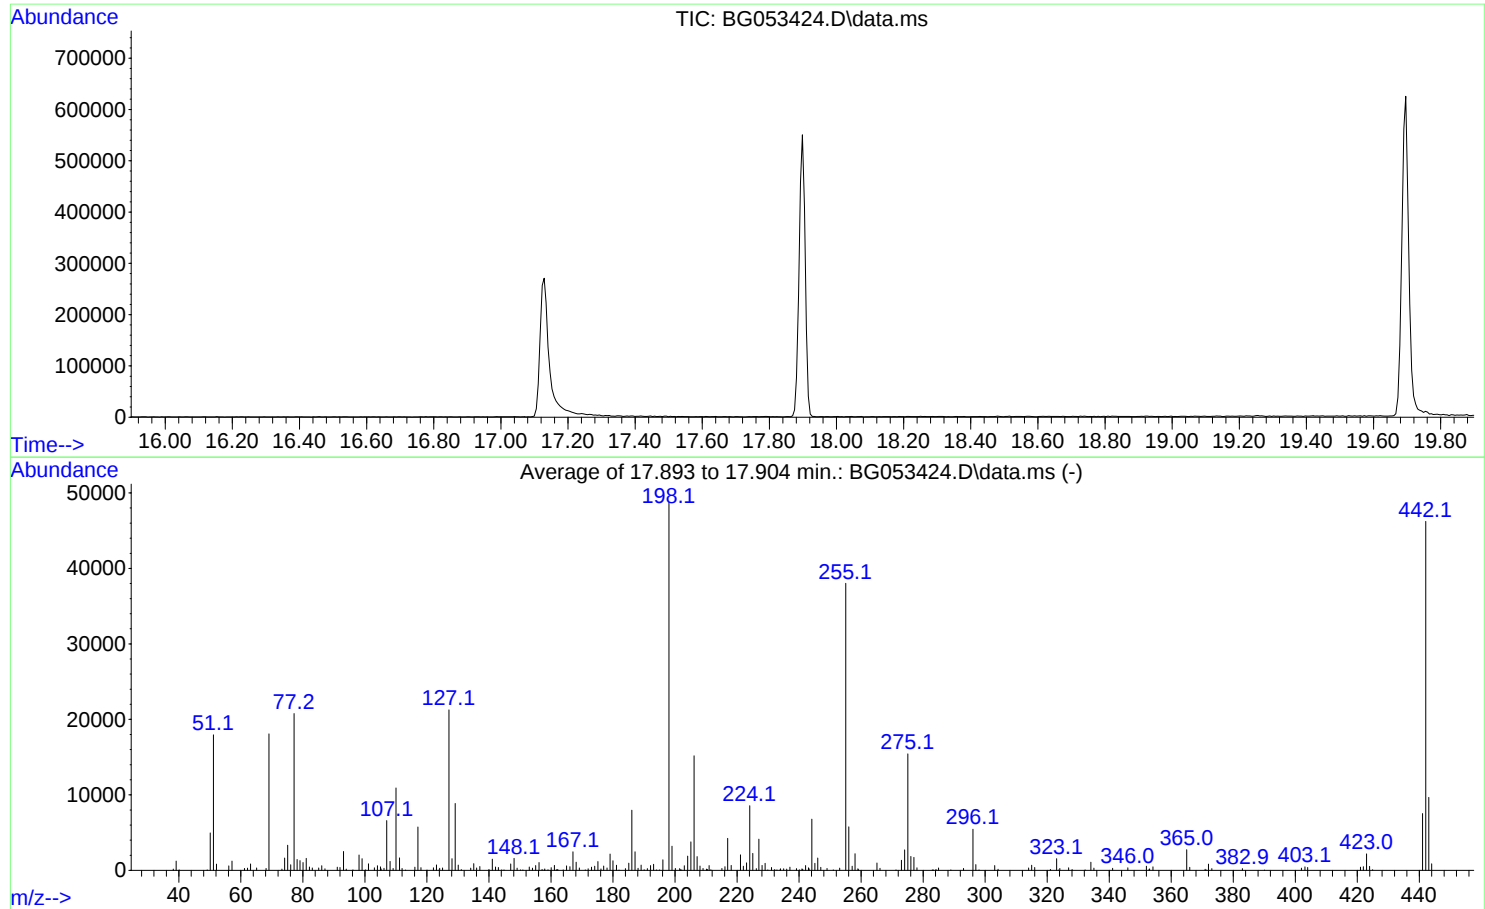




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	17956	PASS
68	69	0.00	2	1.4	254	PASS
69	198	0.00	100	37.1	18077	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	21257	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48731	PASS
199	198	5	9	6.6	3207	PASS
275	198	10	60	31.7	15430	PASS
365	198	1	100	5.6	2745	PASS
441	198	0.01	100	15.5	7529	PASS
442	442	50	100	100.0	46221	PASS
443	442	15	24	20.9	9656	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050422\
Data File : BG053424.D
Acq On : 4 May 2022 10:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 04 18:16:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 04 18:06:54 2022
Response via : Initial Calibration

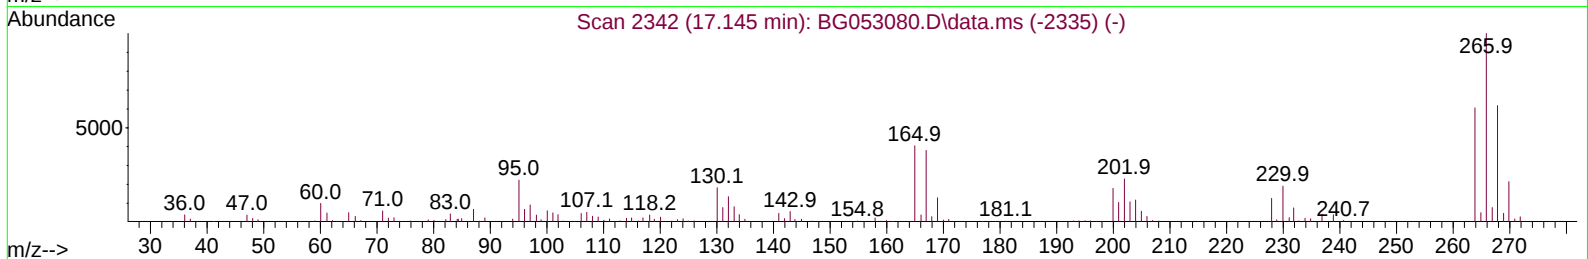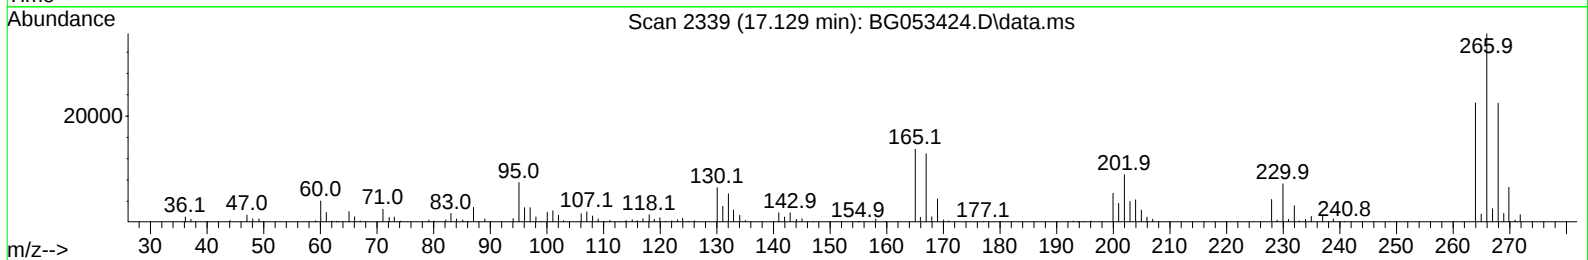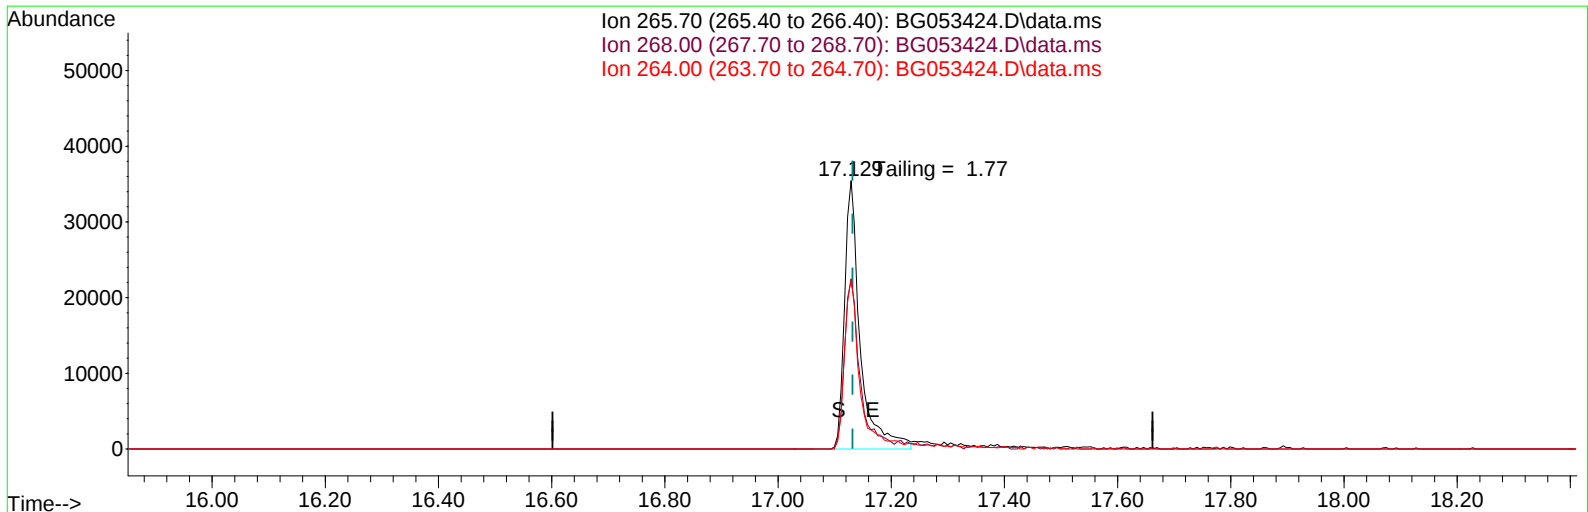

TIC: BG053424.D\data.ms

(70) Pentachlorophenol (C)

17.129min (-0.003) 21325.43 ng




response 70837

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	63.22
264.00	56.60	63.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050422\
 Data File : BG053424.D
 Acq On : 4 May 2022 10:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: May 04 18:16:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 04 18:06:54 2022
 Response via : Initial Calibration

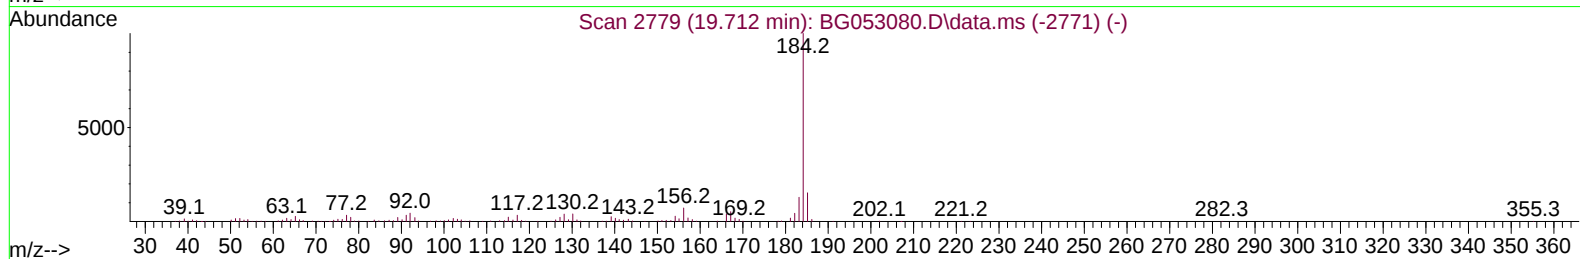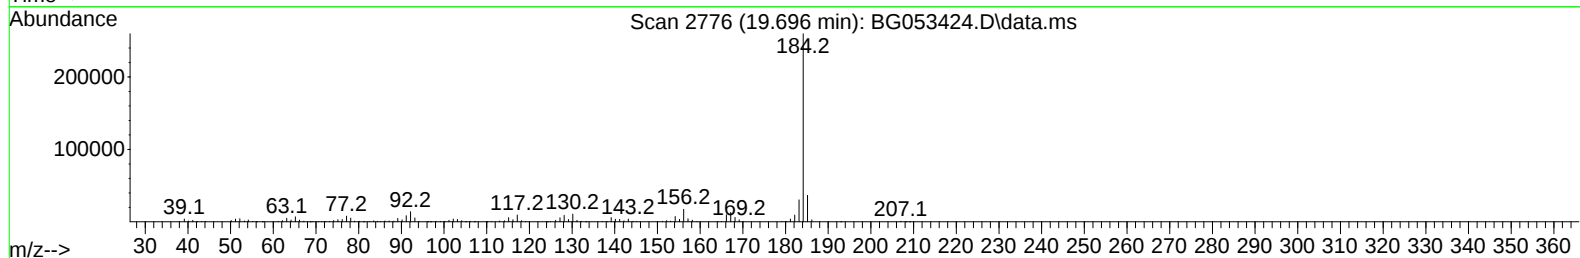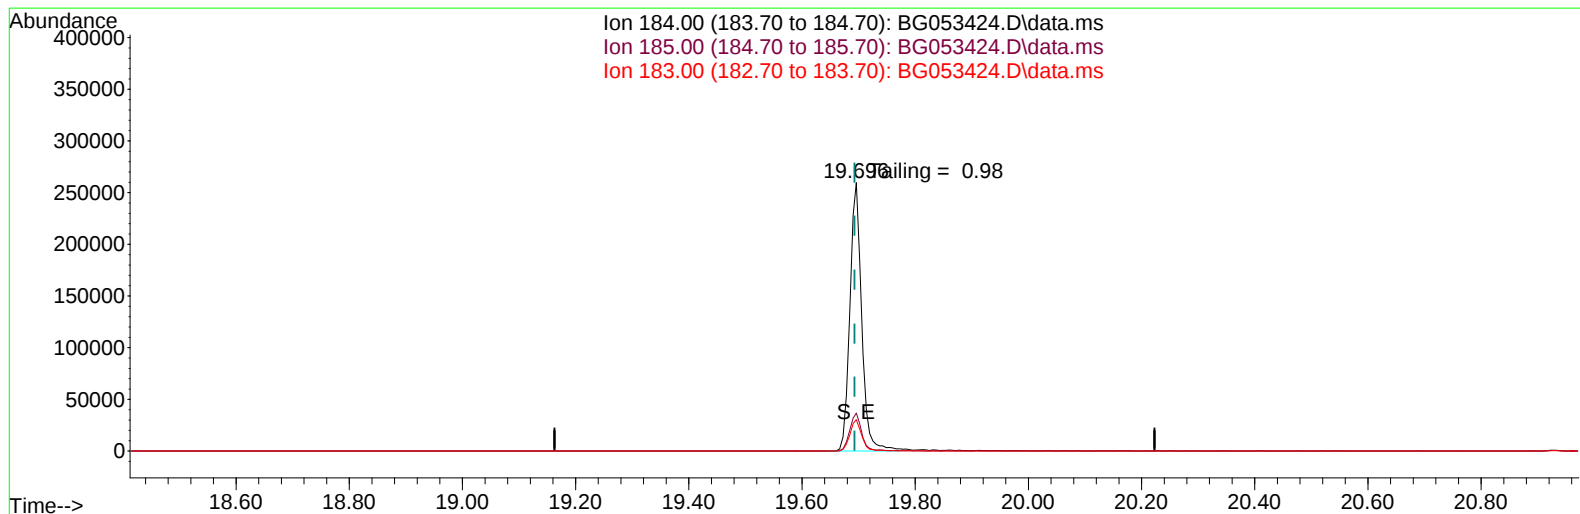

TIC: BG053424.D\data.ms

(77) Benzidine

19.696min (+ 0.003) 0.00 ng

response 376453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.80	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/4/2022	BNA_G	<u>BG053424.D</u>
Compound Name	Response	Retention Time
DDT	198333	20.93
DDD	1297	20.48
DDE	79	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1376	199709	0.69

Instrument :
BNA_G
ClientSampleId :
DFTPP