
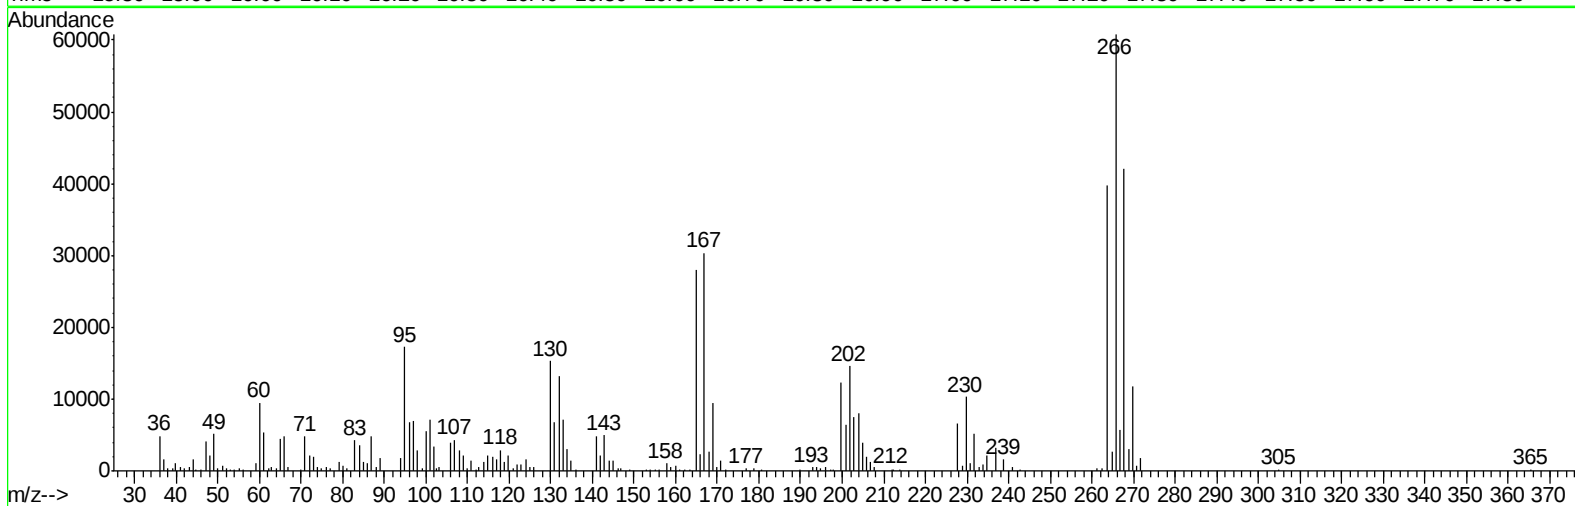


Data Path : Z:\HPCHEM1\BNA_G\Data\BG050515\
Data File : BG016877.D
Acq On : 5 May 2015 23:10
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 07:10:20 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 16:13:58 2015
Response via : Initial Calibration

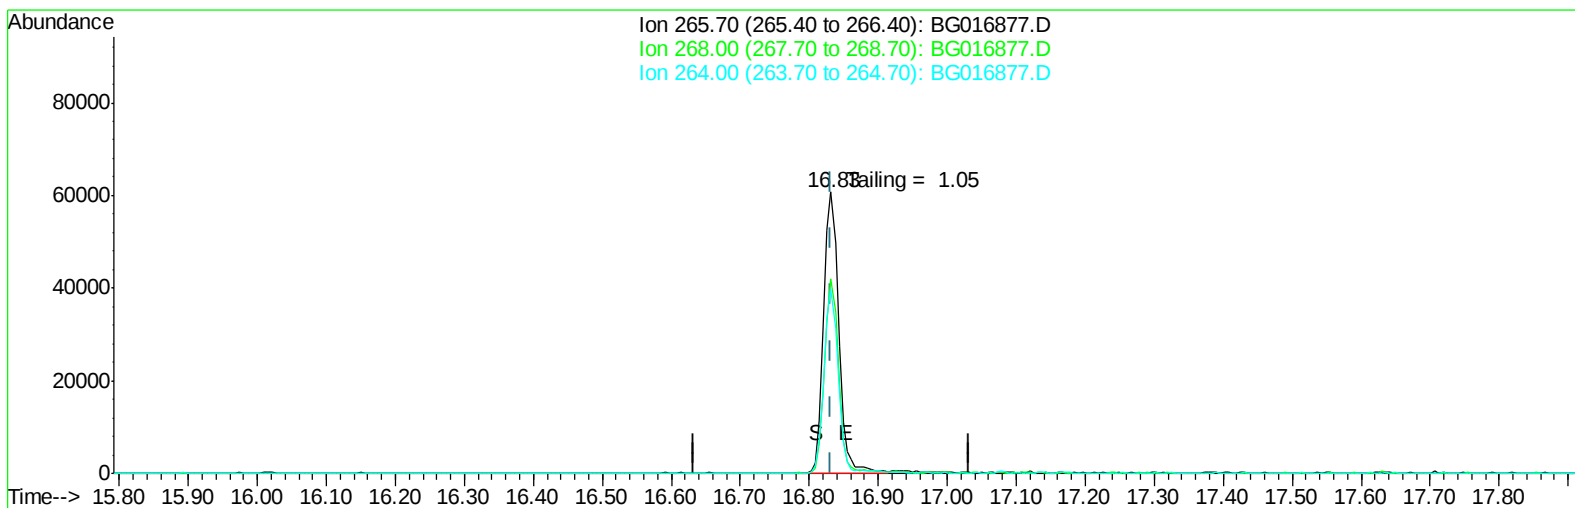

TIC: BG016877.D

(69) Pentachlorophenol (C)



16.832min (-0.001) 201022.16ng

response 92555

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	69.30
264.00	64.20	65.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG050515\
Data File : BG016877.D
Acq On : 5 May 2015 23:10
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 07:10:20 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 16:13:58 2015
Response via : Initial Calibration

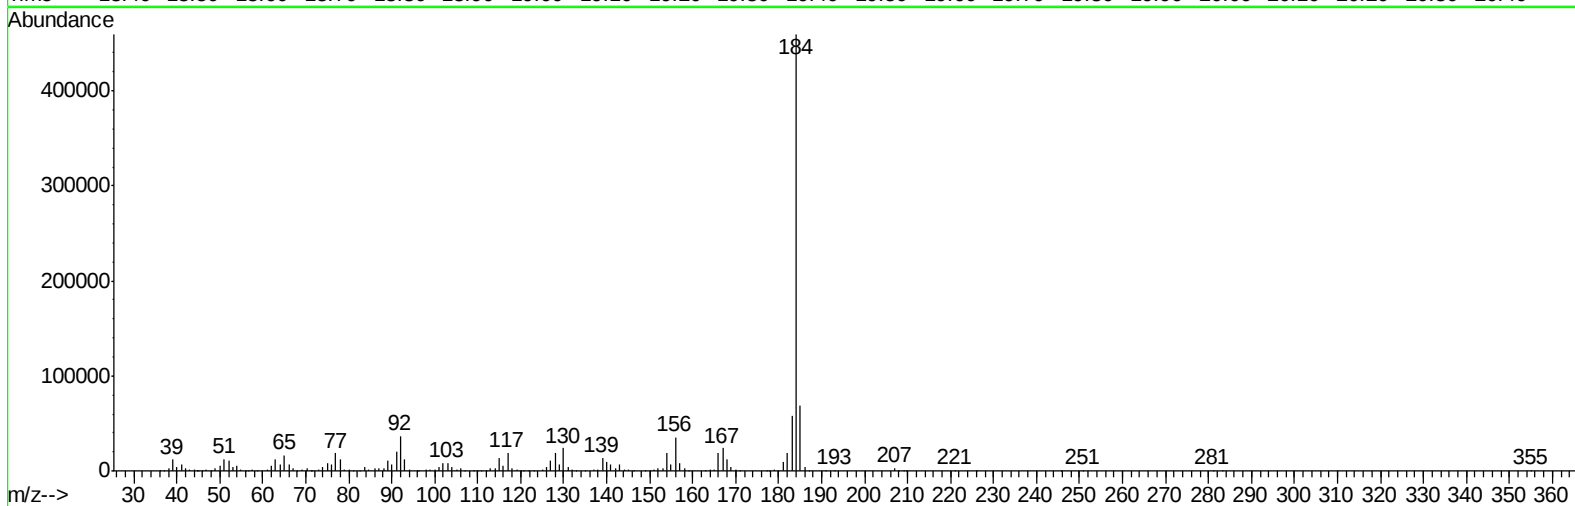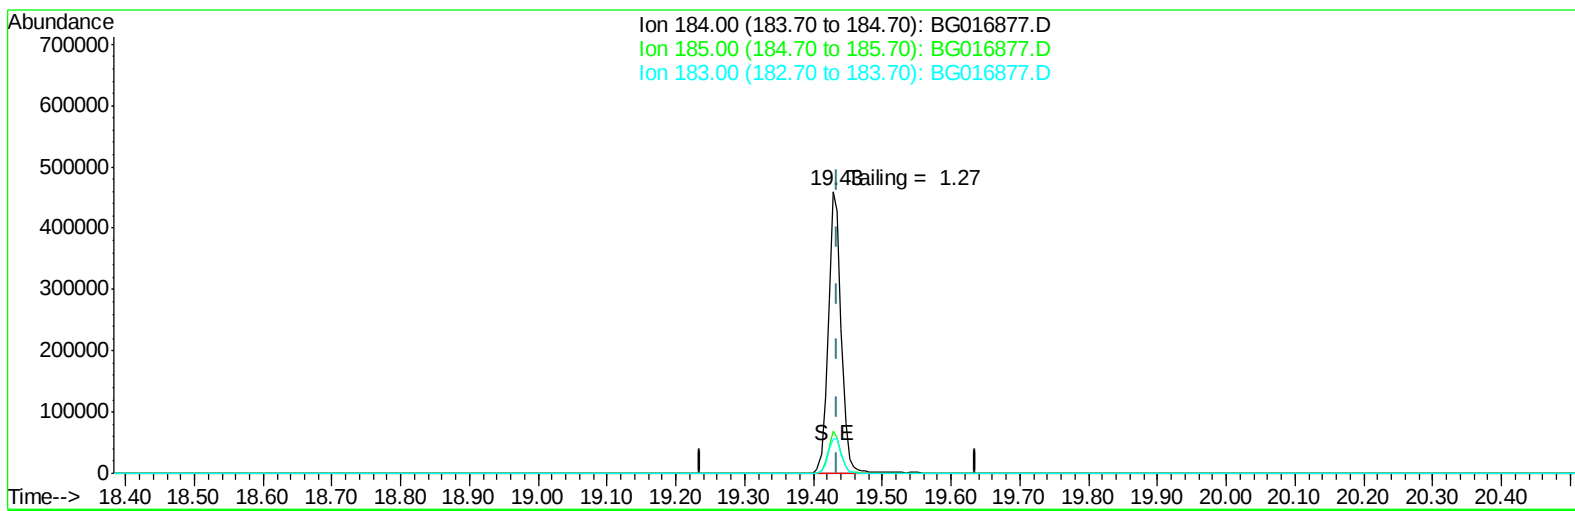

TIC: BG016877.D

(76) Benzidine

19.429min (-0.007) 7791.41ng

response 602551

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.89
183.00	13.20	12.47
0.00	0.00	0.00