

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050515\
 Data File : BG016886.D
 Acq On : 6 May 2015 4:57
 Operator : TP/IZ
 Sample : G2114-09
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GRID-3(12-23)

Quant Time: May 06 05:58:48 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 06 03:35:52 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	74828	20.00	ng	0.00
21) Naphthalene-d8	10.60	136	325231	20.00	ng	0.00
38) Acenaphthene-d10	14.44	164	210612	20.00	ng	0.00
63) Phenanthrene-d10	17.18	188	473119	20.00	ng	0.00
75) Chrysene-d12	21.36	240	484084	20.00	ng	0.00
86) Perylene-d12	23.67	264	469439	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	446151	103.82	ng	0.00
7) Phenol-d6	6.97	99	616208	100.37	ng	0.00
23) Nitrobenzene-d5	8.96	82	389693	58.54	ng	0.00
41) 2,4,6-Tribromophenol	15.93	330	203776	96.38	ng	0.00
44) 2-Fluorobiphenyl	13.06	172	740355	53.05	ng	0.00
78) Terphenyl-d14	19.82	244	1081729	52.38	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.90	163	43332	2.76	ng	Qvalue # 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050515\
Data File : BG016886.D
Acq On : 6 May 2015 4:57
Operator : TP/IZ
Sample : G2114-09
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GRID-3(12-23)

Quant Time: May 06 05:58:48 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 06 03:35:52 2015
Response via : Initial Calibration

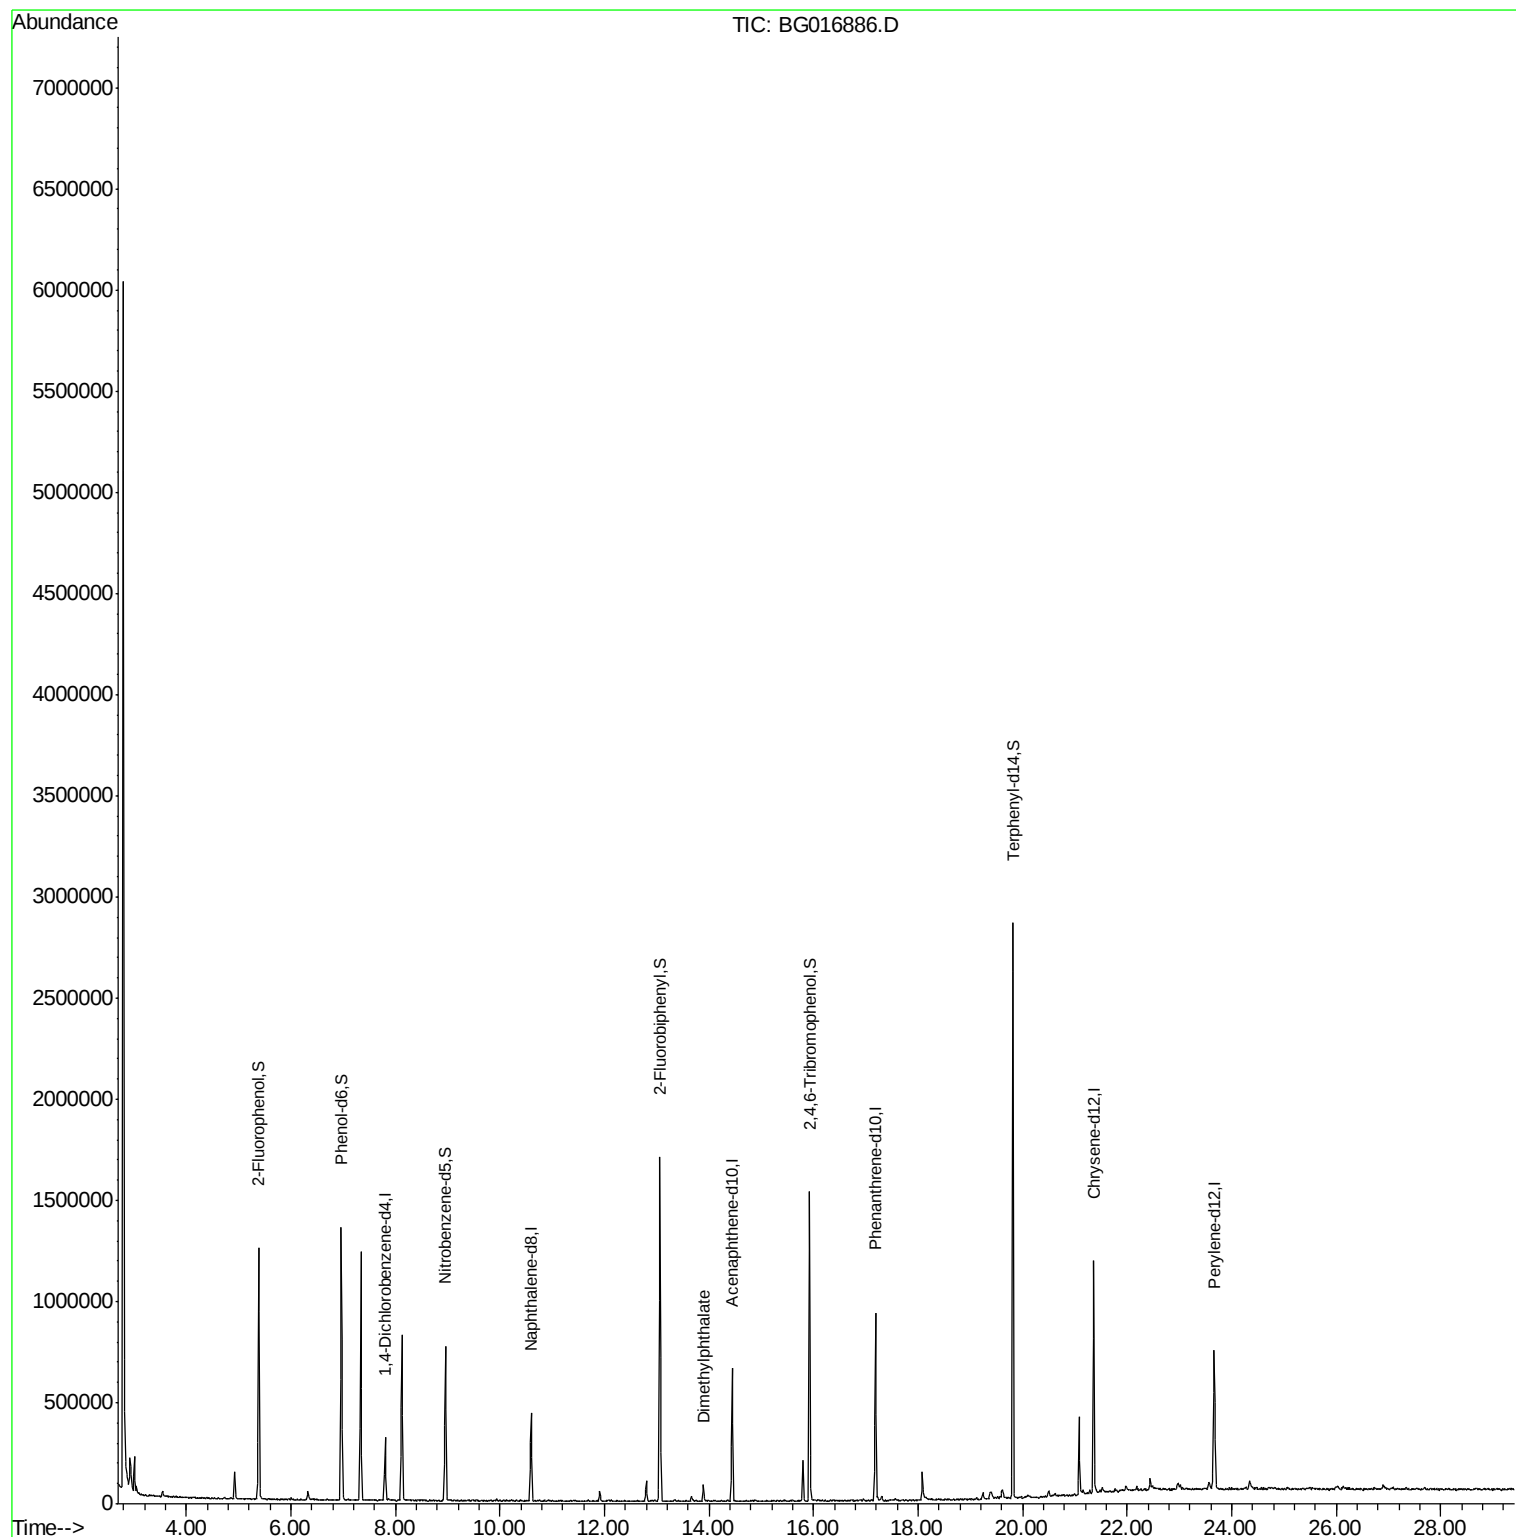




#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.81 min Scan# 871
Delta R.T. 0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Instrument :
BNA_G
ClientSampleId :
GRID-3(12-23)

Tot Ion	Ratio	Lower	Upper
152	100		
150	143.1	121.0	181.4
115	56.2	50.5	75.7

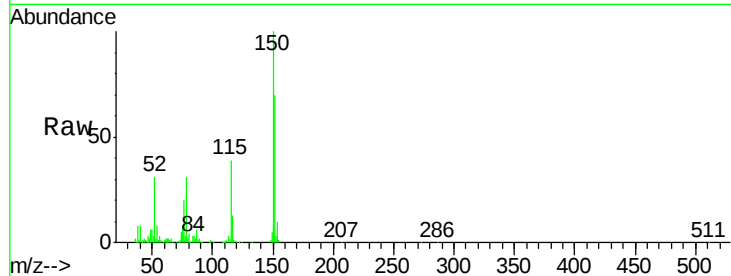


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

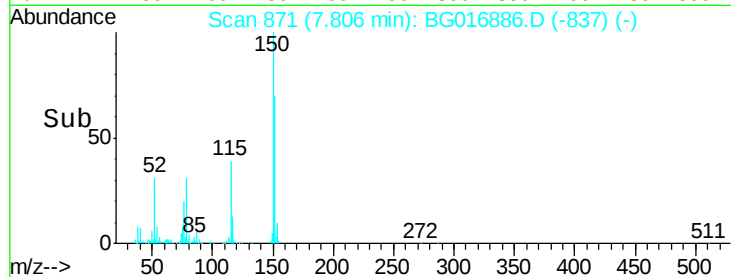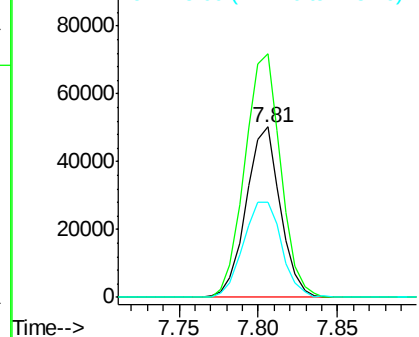



#5


2-Fluorophenol
Concen: 103.82 ng
RT: 5.39 min Scan# 459
Delta R.T. 0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Tgt Ion	Ratio	Lower	Upper
112	100		
64	69.4	51.4	77.2
63	39.0	28.1	42.1

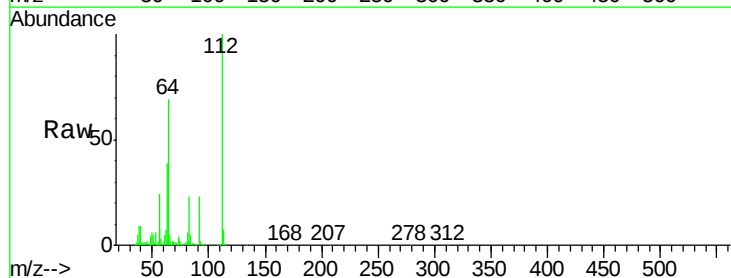

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

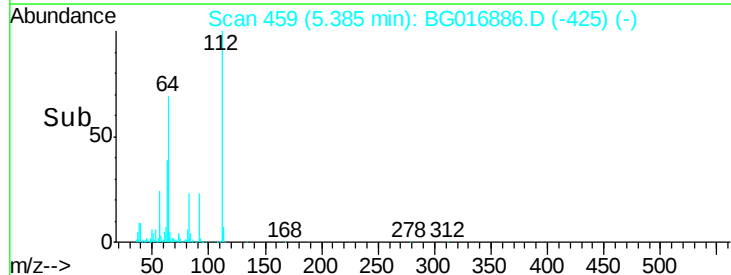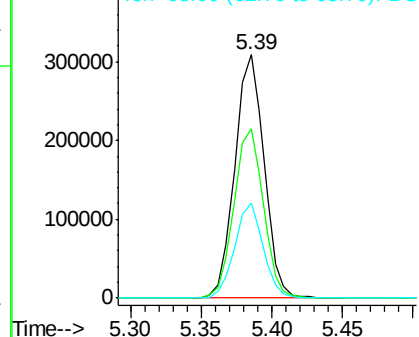

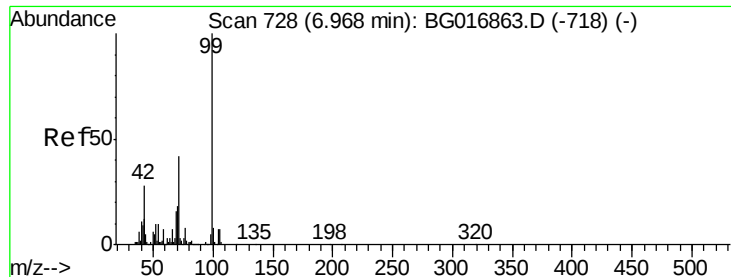

#7

Phenol-d6

Concen: 100.37 ng

RT: 6.97 min Scan# 728

Delta R.T. 0.00 min

Lab File: BG016886.D

Acq: 6 May 2015 4:57

Instrument :

BNA_G

ClientSampleId :

GRID-3(12-23)


Tot Ion: 99 Resp: 616208

Ion Ratio Lower Upper




99 100

42 27.7 22.1 33.1

71 43.8 33.4 50.0

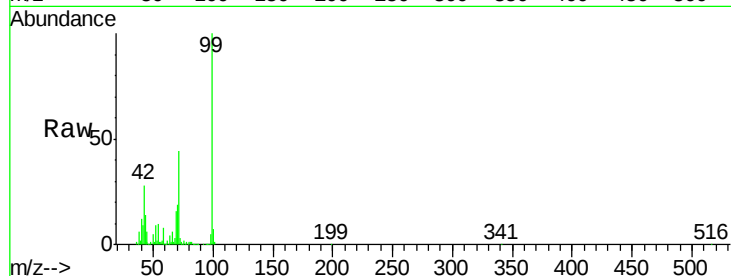

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

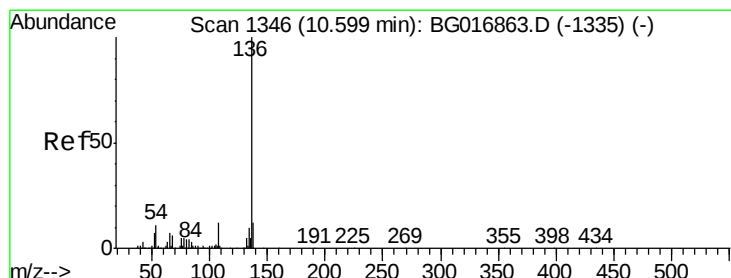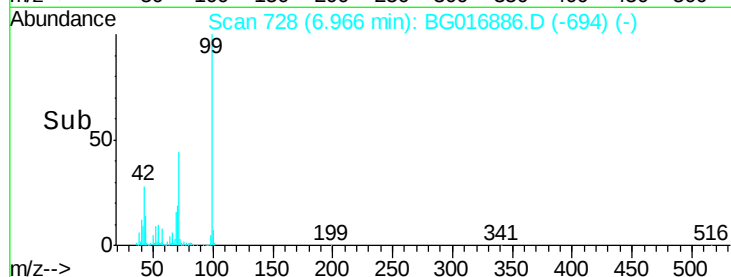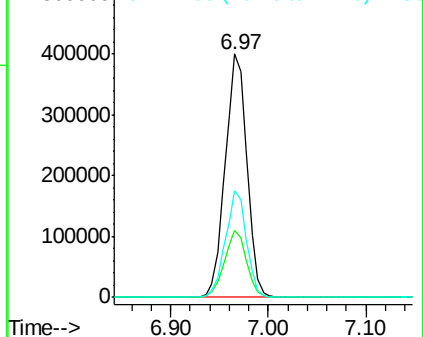

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.60 min Scan# 1346

Delta R.T. 0.00 min

Lab File: BG016886.D

Acq: 6 May 2015 4:57

Tgt Ion: 136 Resp: 325231


Ion Ratio Lower Upper

136 100



137 10.4 9.8 14.8


54 10.8 8.7 13.1

68 5.9 5.0 7.4

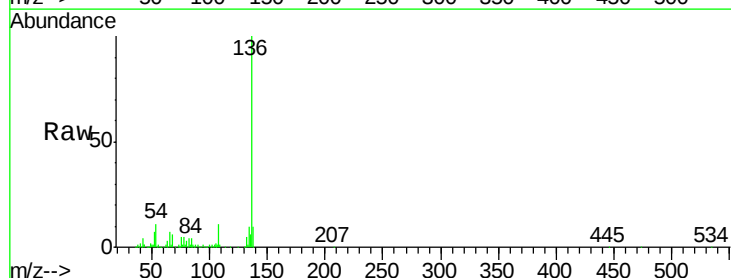

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



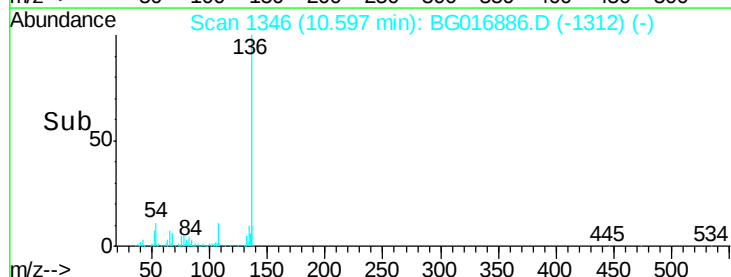
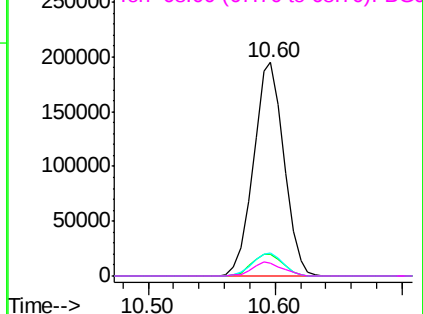


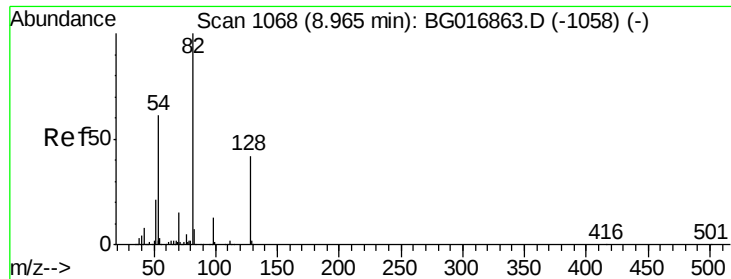

#23
Nitrobenzene-d5
Concen: 58.54 ng
RT: 8.96 min Scan# 1067
Delta R.T. -0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57




Instrument :
BNA_G
ClientSampleId :
GRID-3(12-23)


Tot Ion	82	Resp	389693
Ion Ratio	Lower	Upper	
82	100		
128	41.0	33.2	49.8
54	56.8	48.6	72.8

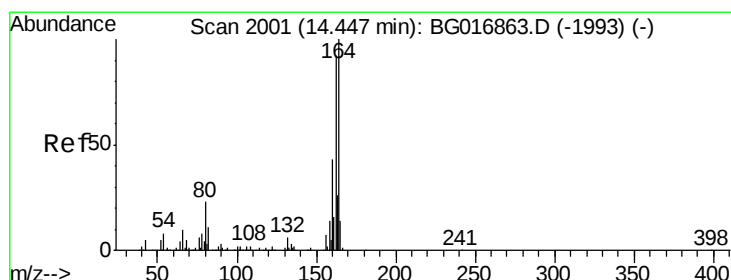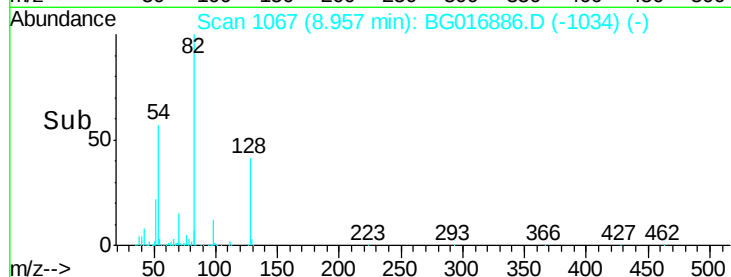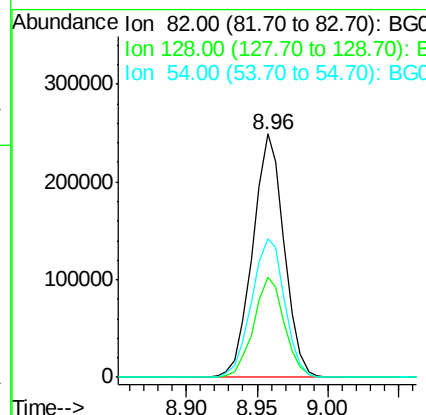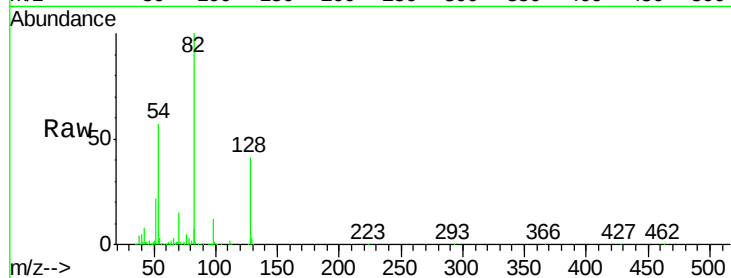

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.44 min Scan# 2000
Delta R.T. -0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Tgt Ion	164	Resp	210612
Ion Ratio	Lower	Upper	
164	100		
162	95.2	74.0	111.0
160	40.4	34.7	52.1


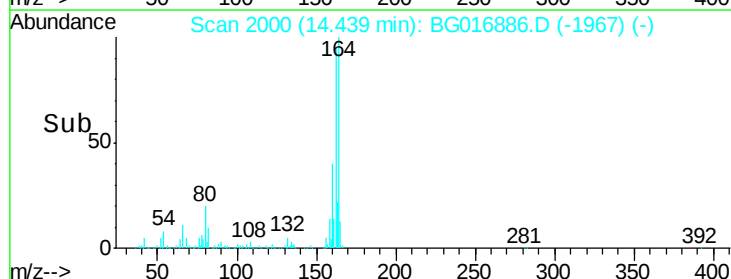
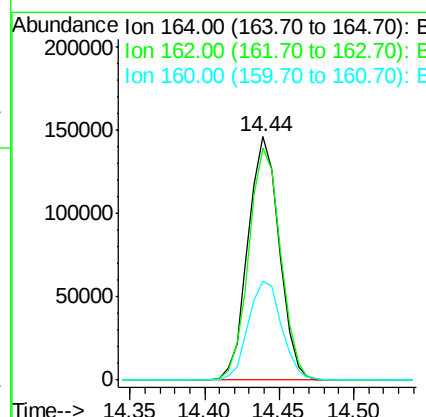
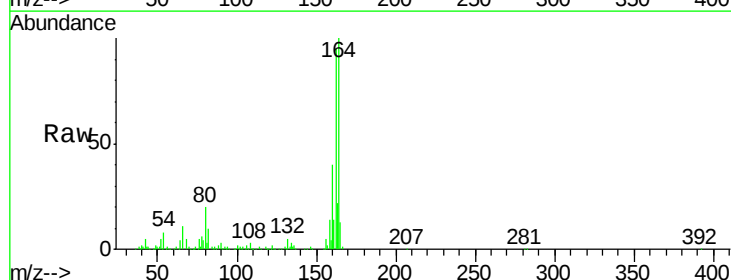


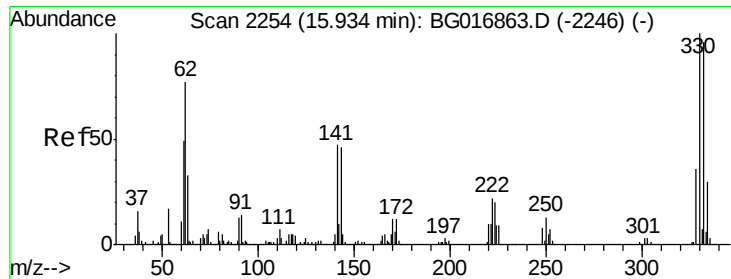

#41
 2,4,6-Tribromophenol
 Concen: 96.38 ng
 RT: 15.93 min Scan# 2253
 Delta R.T. -0.00 min
 Lab File: BG016886.D
 Acq: 6 May 2015 4:57




Instrument :
 BNA_G
 ClientSampleId :
 GRID-3(12-23)


Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	0.0	0.0#
141	51.5	0.0	0.0#

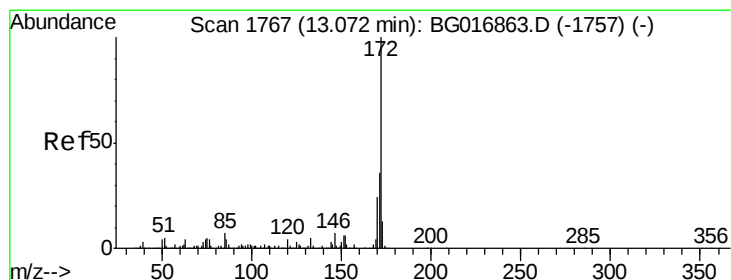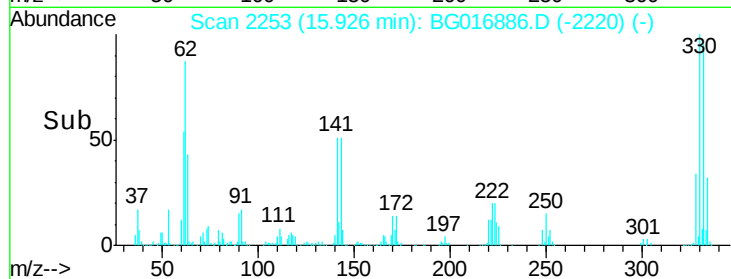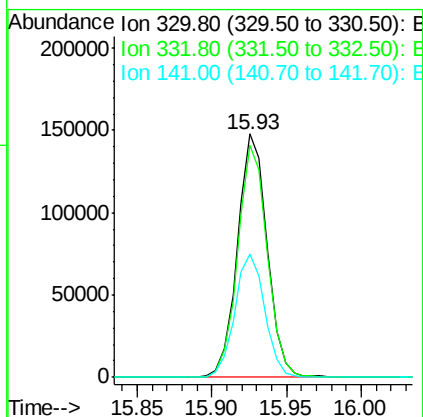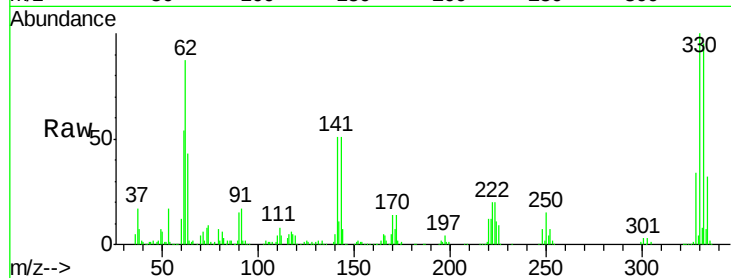

#44
 2-Fluorobiphenyl
 Concen: 53.05 ng
 RT: 13.06 min Scan# 1766
 Delta R.T. -0.00 min
 Lab File: BG016886.D
 Acq: 6 May 2015 4:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.6	29.0	43.4
170	23.0	19.0	28.4

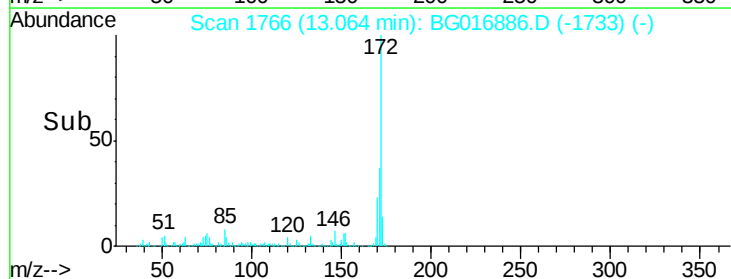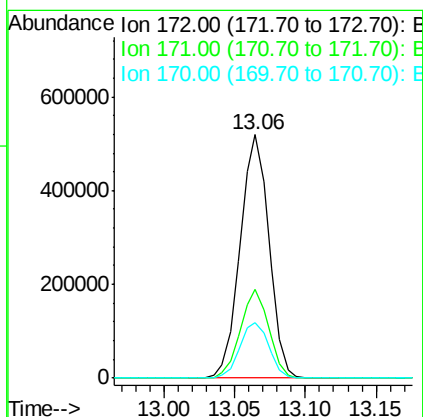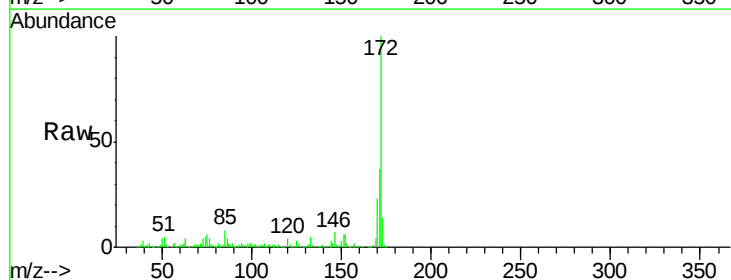


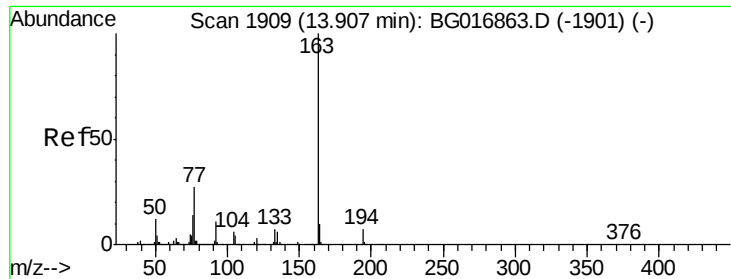




#49
Dimethylphthalate
Concen: 2.76 ng
RT: 13.90 min Scan# 1908
Delta R.T. -0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Instrument :
BNA_G
ClientSampleId :
GRID-3(12-23)

Tot Ion:163 Resp: 43332
Ion Ratio Lower Upper
163 100
194 5.0 5.2 7.8#
164 8.3 8.4 12.6#

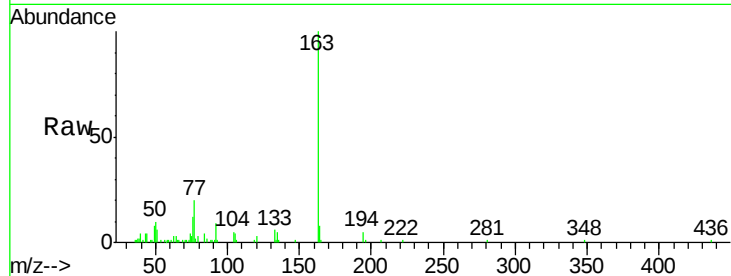


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

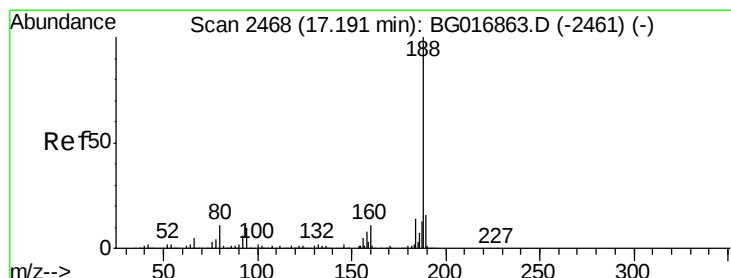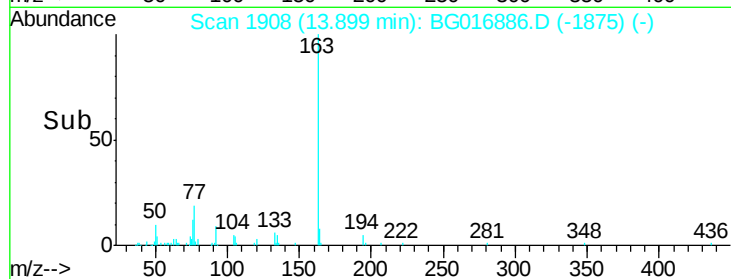
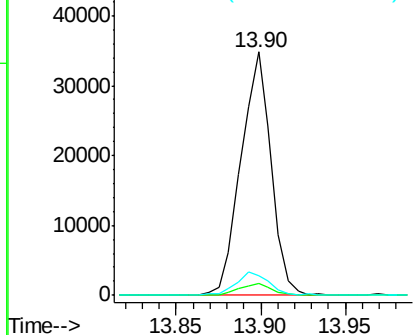



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.18 min Scan# 2467
Delta R.T. -0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Tgt Ion:188 Resp: 473119
Ion Ratio Lower Upper
188 100
94 9.1 8.2 12.4
80 10.7 8.8 13.2

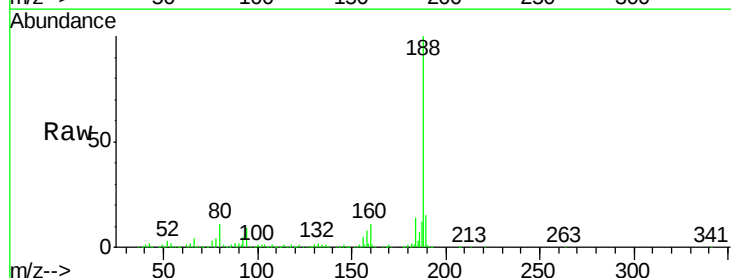

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

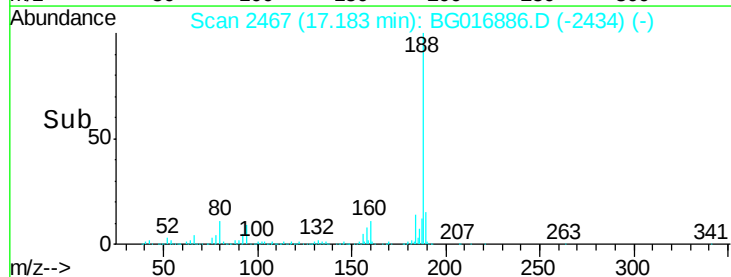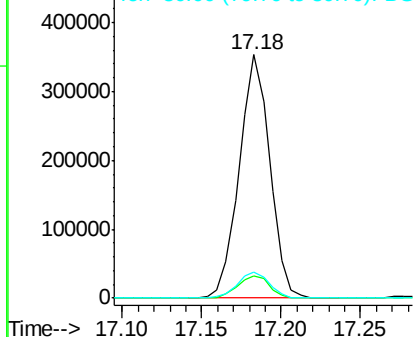

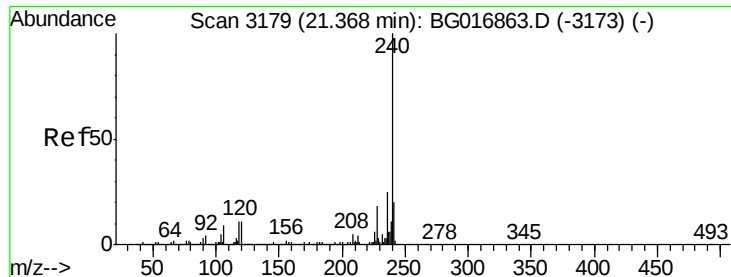

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.36 min Scan# 3178

Delta R.T. -0.00 min

Lab File: BG016886.D

Acq: 6 May 2015 4:57

Instrument :

BNA_G

ClientSampleId :

GRID-3(12-23)


Tot Ion:240 Resp: 484084

Ion Ratio Lower Upper

240 100

120 11.4 9.1 13.7




236 25.6 20.2 30.4

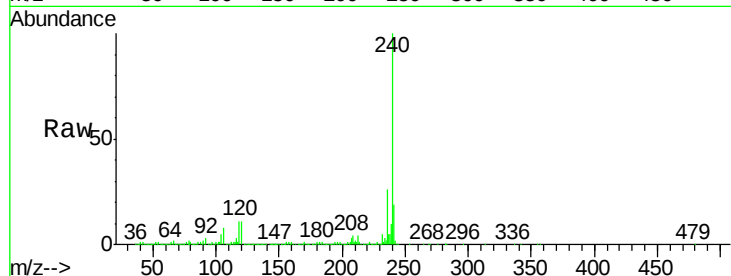

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

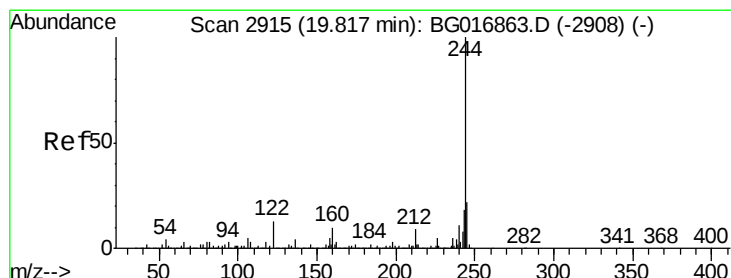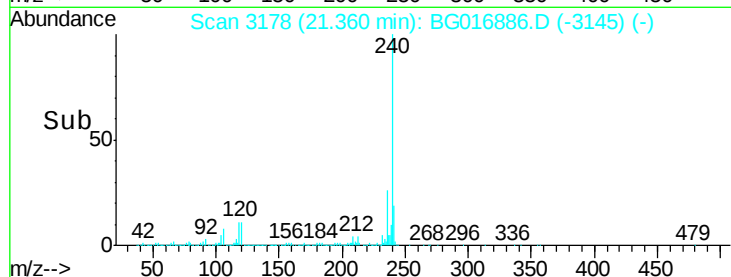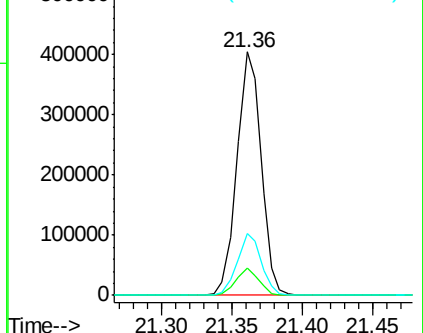

#78

Terphenyl-d14

Concen: 52.38 ng

RT: 19.82 min Scan# 2915

Delta R.T. 0.00 min

Lab File: BG016886.D

Acq: 6 May 2015 4:57


Tgt Ion:244 Resp: 1081729

Ion Ratio Lower Upper

244 100

212 9.1 7.0 10.6



122 11.9 10.4 15.6

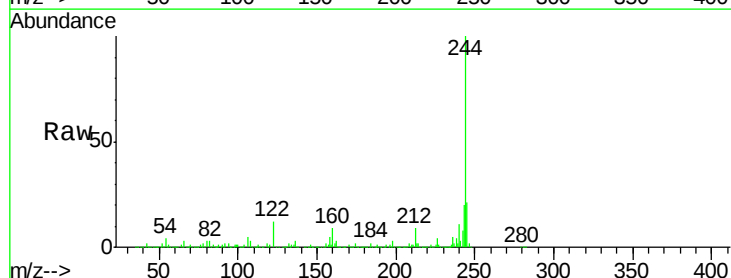


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

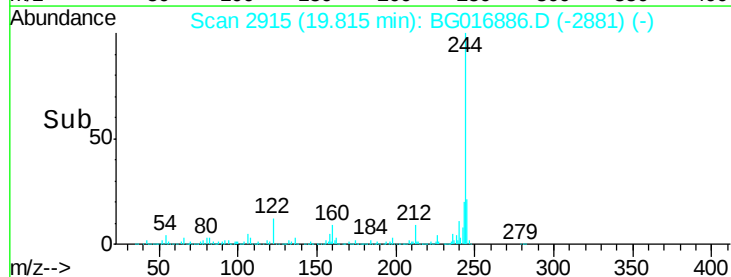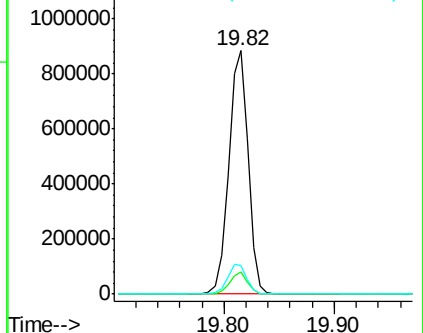

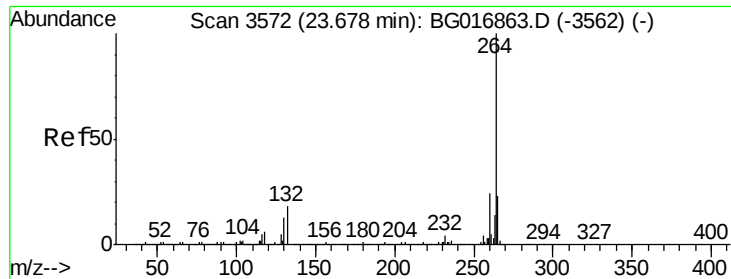

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.67 min Scan# 3571
Delta R.T. 0.00 min
Lab File: BG016886.D
Acq: 6 May 2015 4:57

Instrument :
BNA_G
ClientSampleId :
GRID-3(12-23)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.5	29.3
265	22.8	18.5	27.7

