


Data Path : Z:\HPCHEM1\BNA G\DATA\BG050515\
 Data File : BG016859.D
 Acq On : 5 May 2015 10:36
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 05 16:13:58 2015

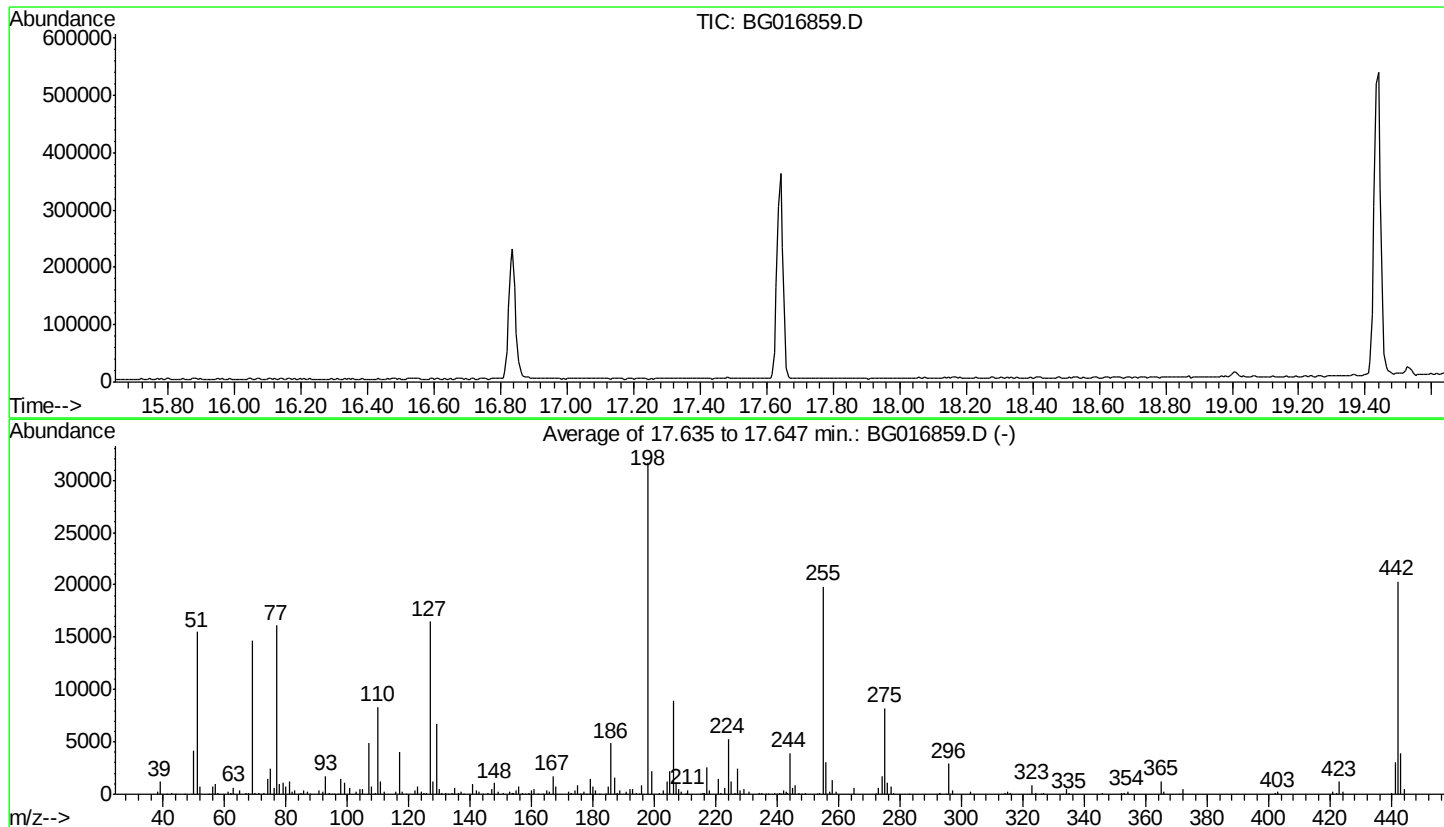

AutoFind: Scans 2544, 2545, 2546; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	15494	PASS
68	69	0.00	2	1.0	153	PASS
69	198	0.00	100	46.2	14621	PASS
70	69	0.00	2	0.5	68	PASS
127	198	10	80	52.1	16488	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31677	PASS
199	198	5	9	7.1	2235	PASS
275	198	10	60	25.9	8204	PASS
365	198	1	100	3.9	1232	PASS
441	442	0.01	24	15.3	3104	PASS
442	198	50	100	64.2	20345	PASS
443	442	15	24	19.5	3958	PASS