


Hexachlorobutadiene

Response Ratio

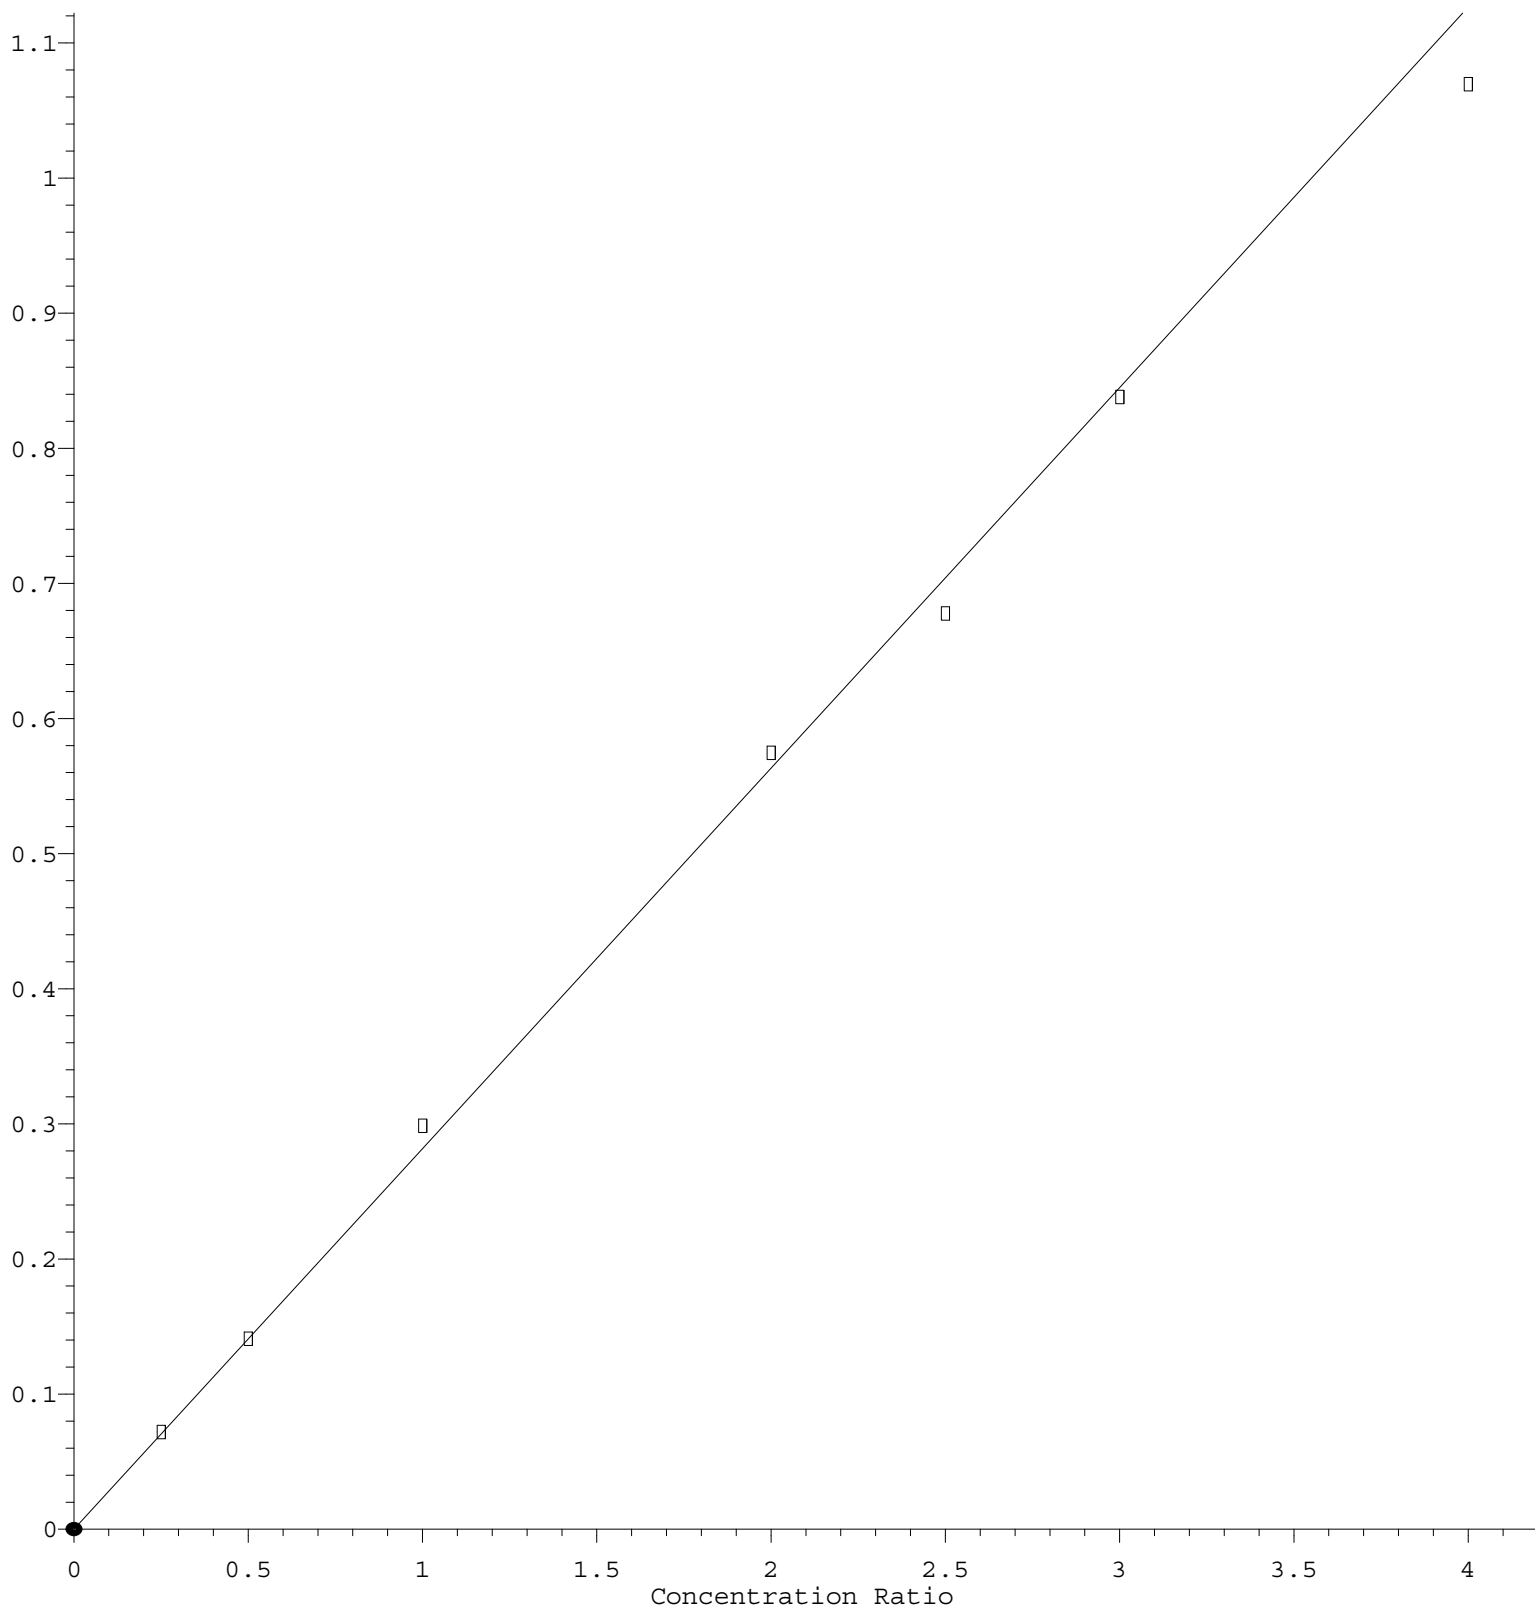

$$\text{Response} = 2.818\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 3.761% Curve Fit: Avg RF

Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG050522.M

Calibration Table Last Updated: Thu May 05 02:13:53 2022

Hexachlorocyclopentadiene

Response Ratio

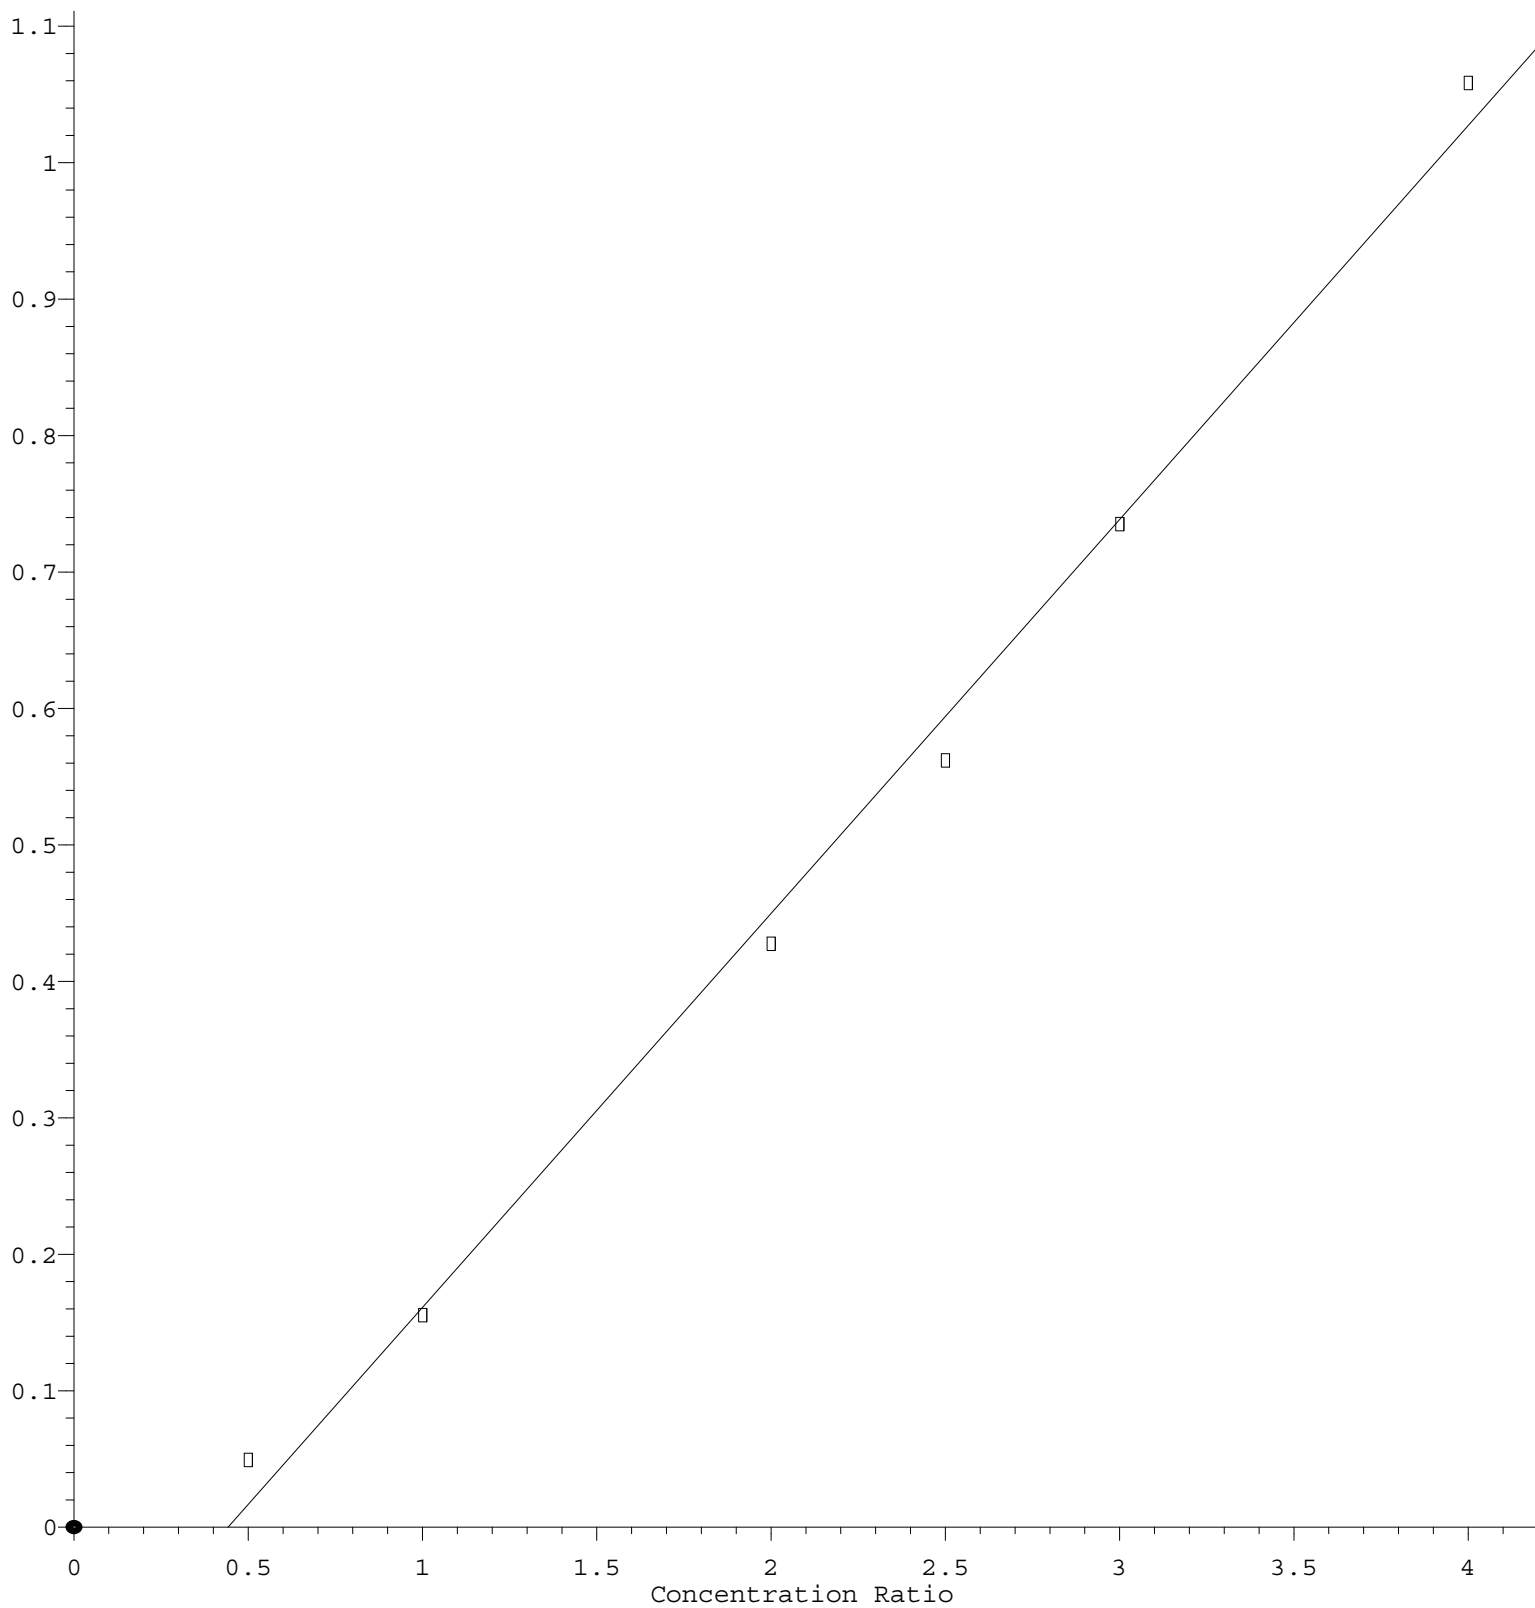


$$\text{Response} = 2.887\text{e-}001 * \text{Amt} - 1.275\text{e-}001$$

Coef of Det (r^2) = 0.994832 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG050522.M


Calibration Table Last Updated: Thu May 05 02:13:53 2022

2,4-Dinitrophenol

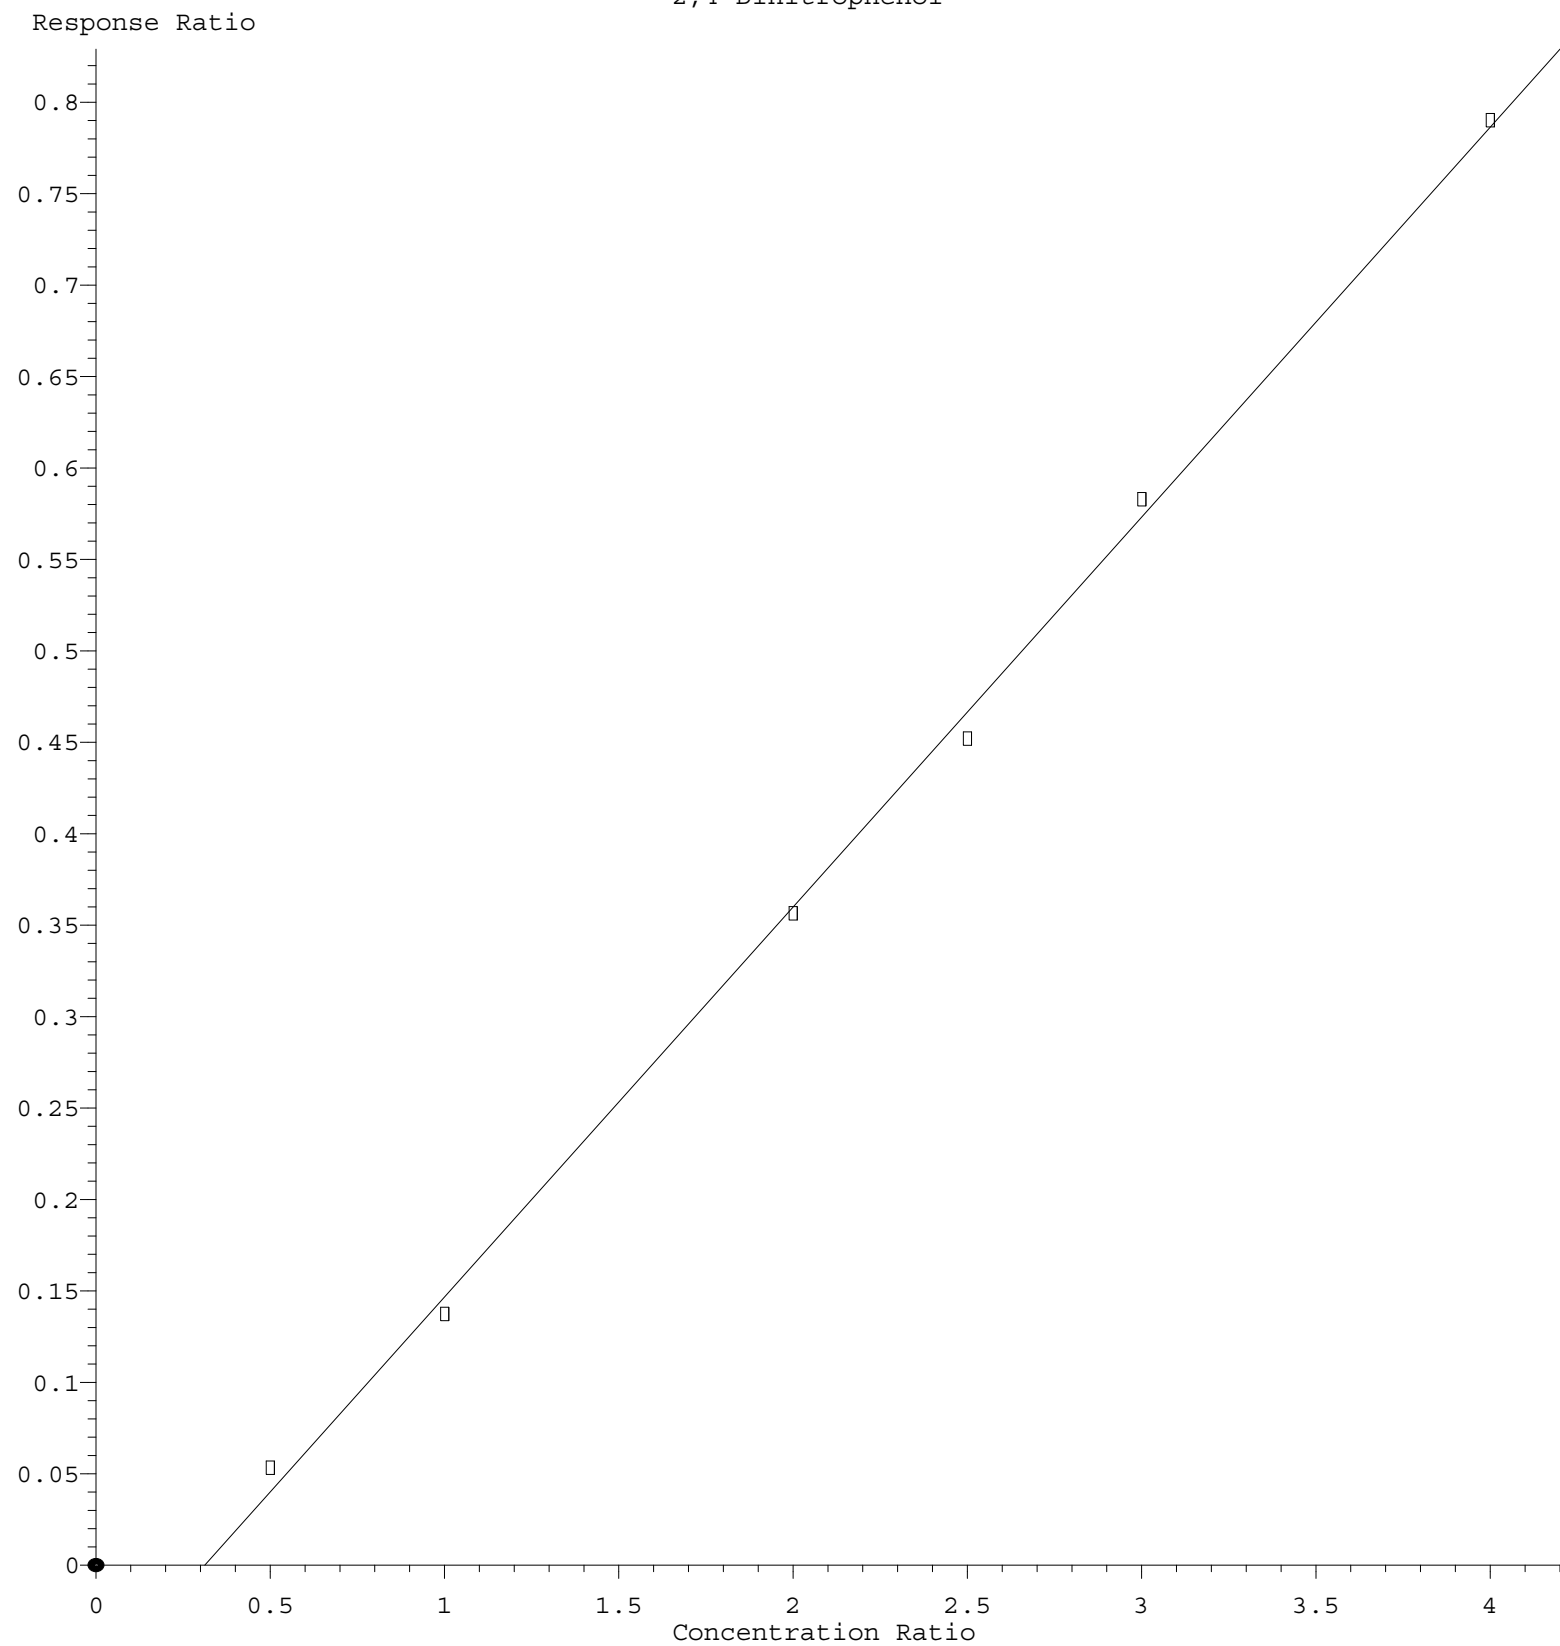

Response = $2.132 \times 10^{-1} \times \text{Amt} - 6.656 \times 10^{-2}$
 Coef of Det (r^2) = 0.998434 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG050522.M
 Calibration Table Last Updated: Thu May 05 02:13:53 2022

Pentachlorophenol

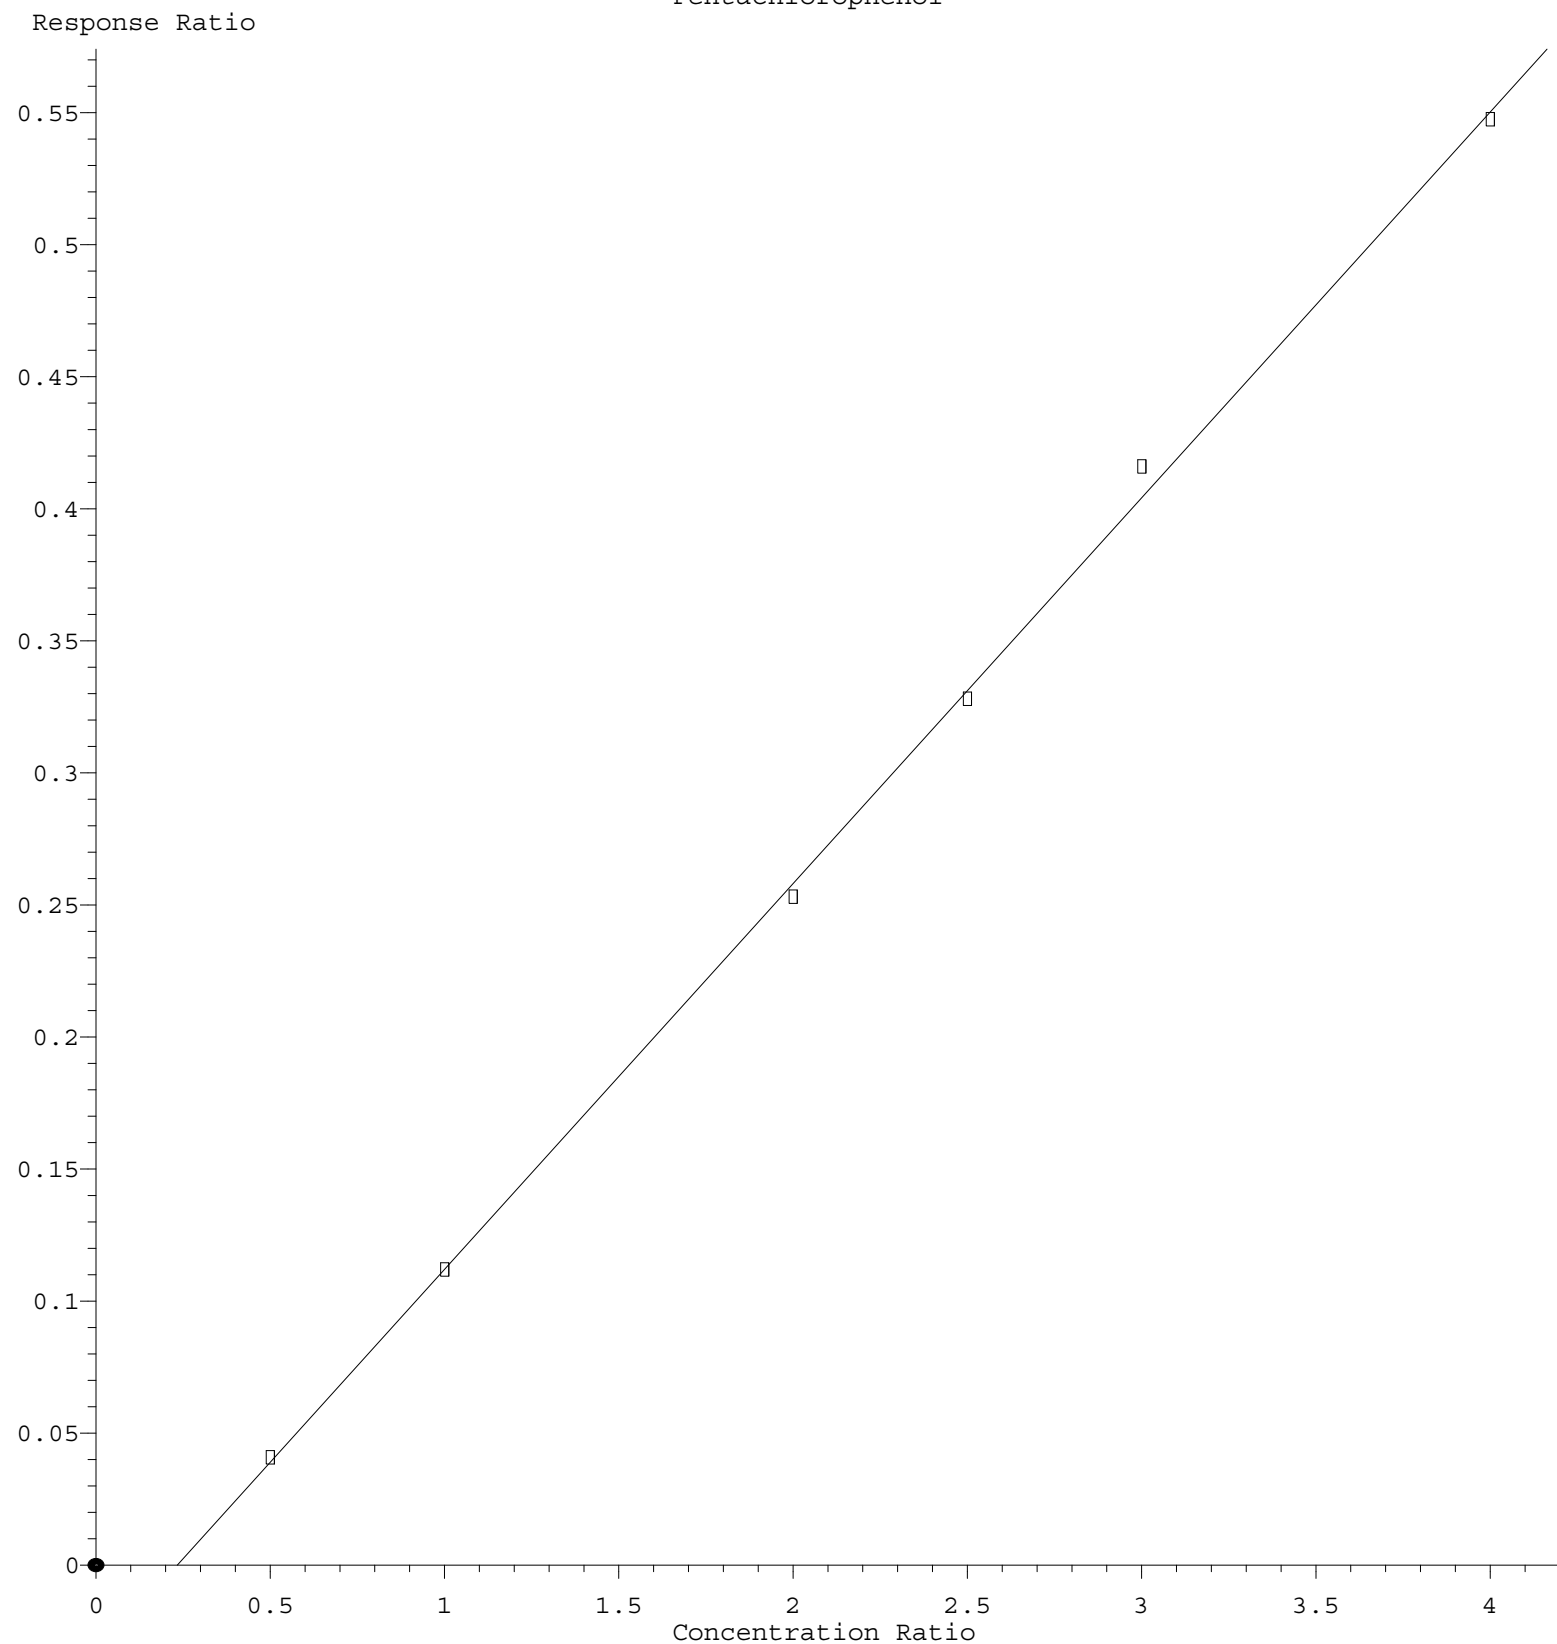

Response = 1.463e-001 * Amt - 3.401e-002
 Coef of Det (r^2) = 0.998966 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA G\Methods\8270-BG050522.M
 Calibration Table Last Updated: Thu May 05 02:13:53 2022