
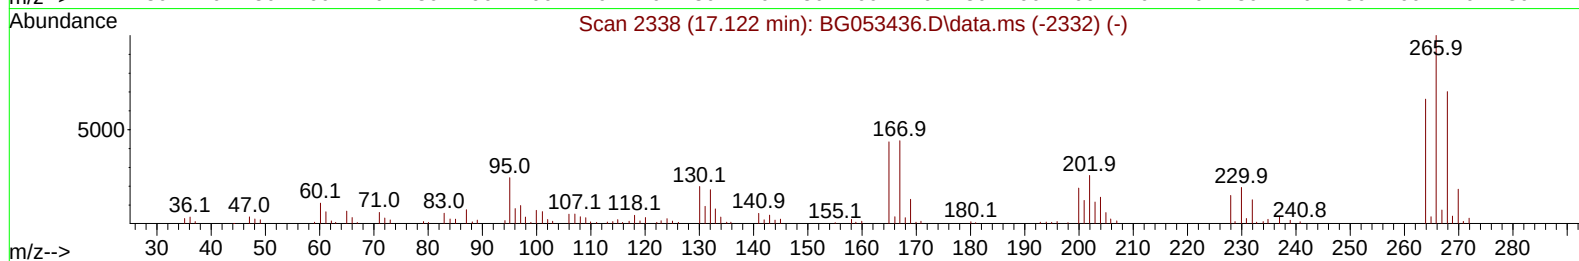
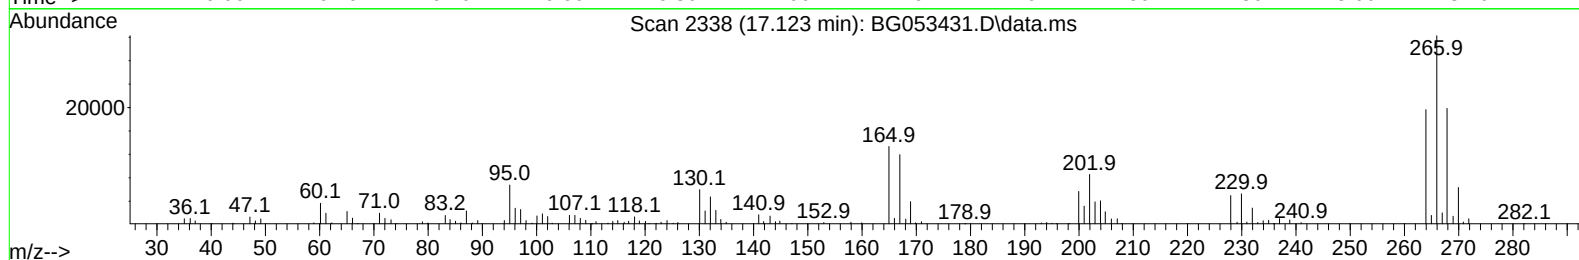


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053431.D
Acq On : 4 May 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 06:36:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

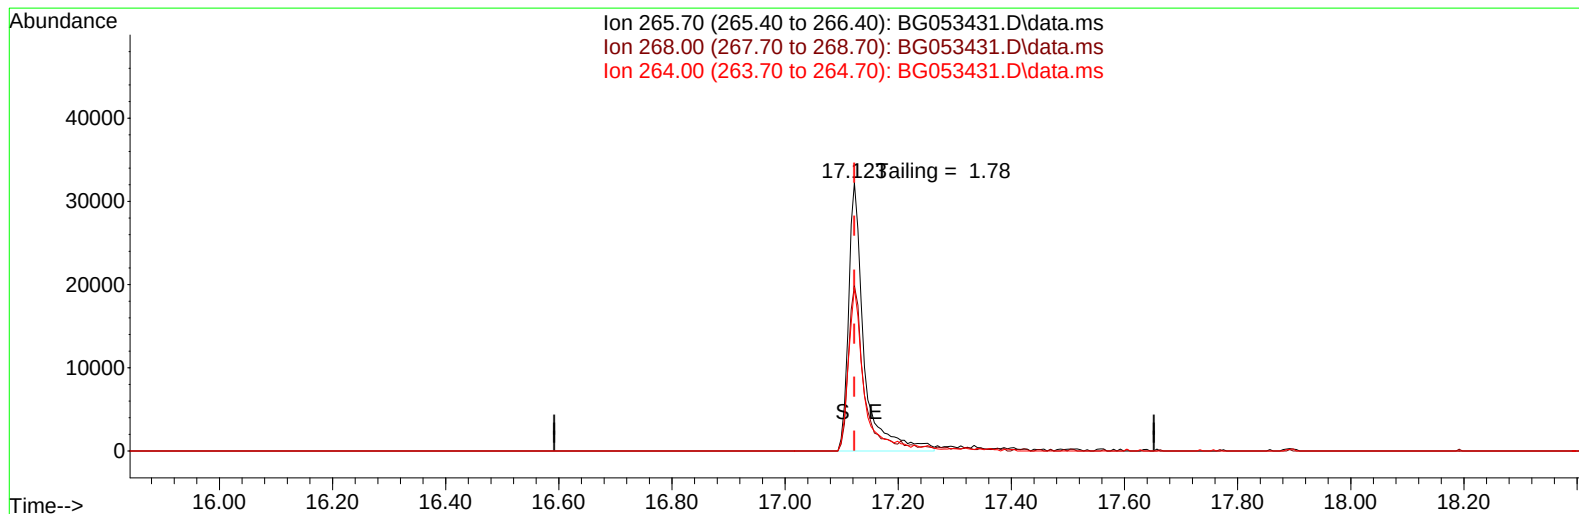

TIC: BG053431.D\data.ms

(70) Pentachlorophenol (C)




17.123min (+ 0.001) 20690.52 ng

response 60512

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.51
264.00	66.20	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053431.D
Acq On : 4 May 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 05 06:36:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

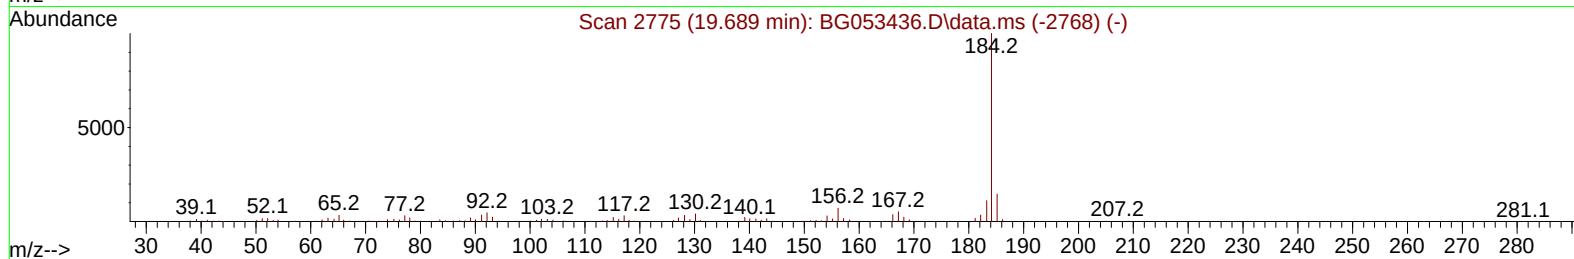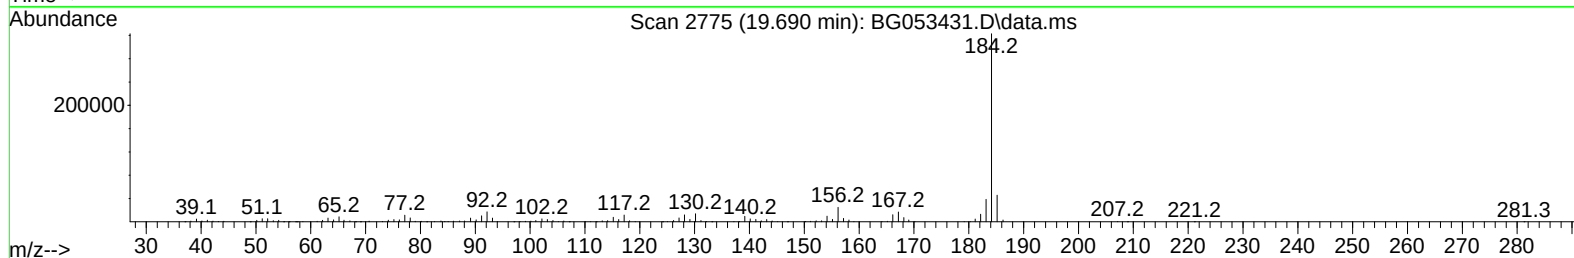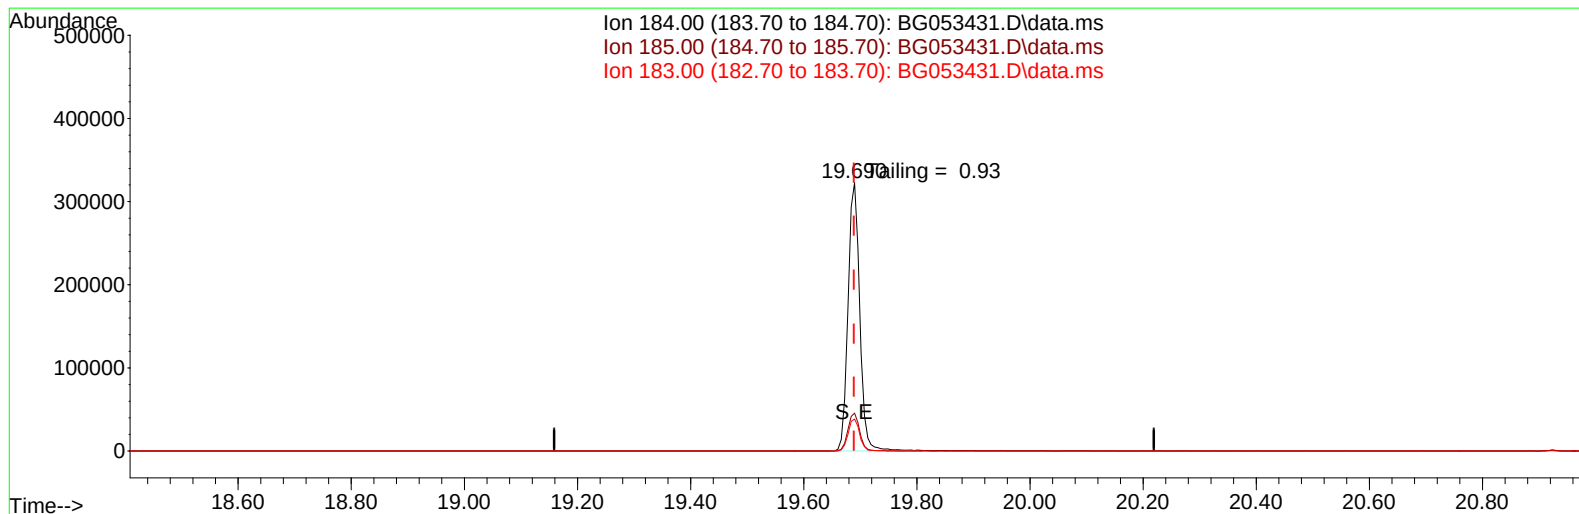

TIC: BG053431.D\data.ms

(77) Benzidine**19.690min (+ 0.001) 139835.00 ng****response 464150**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.16
183.00	11.10	11.97
0.00	0.00	0.00