
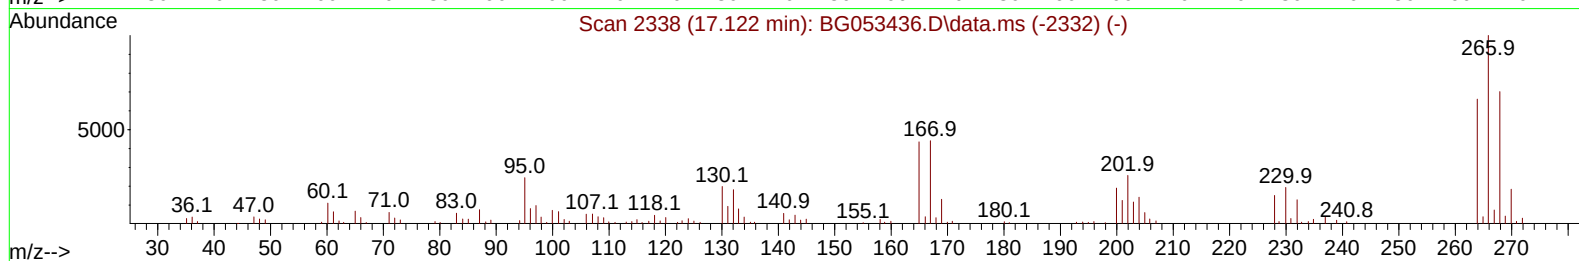
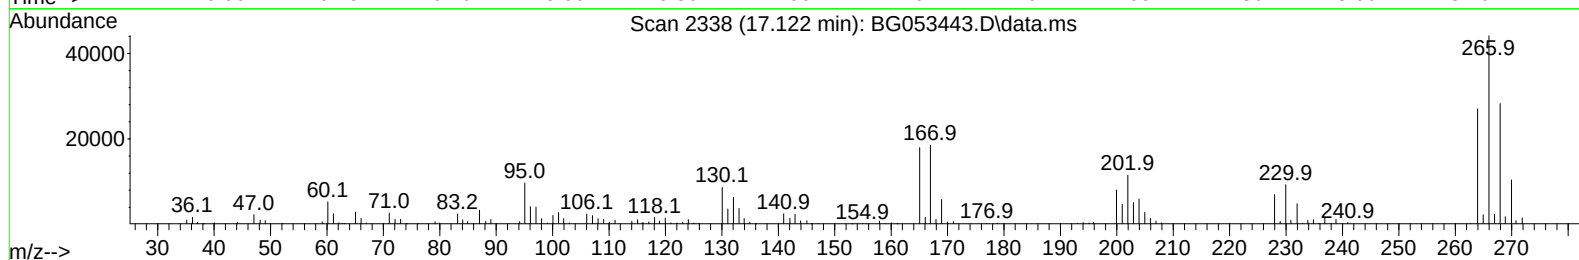


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053443.D
Acq On : 5 May 2022 8:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 06:15:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

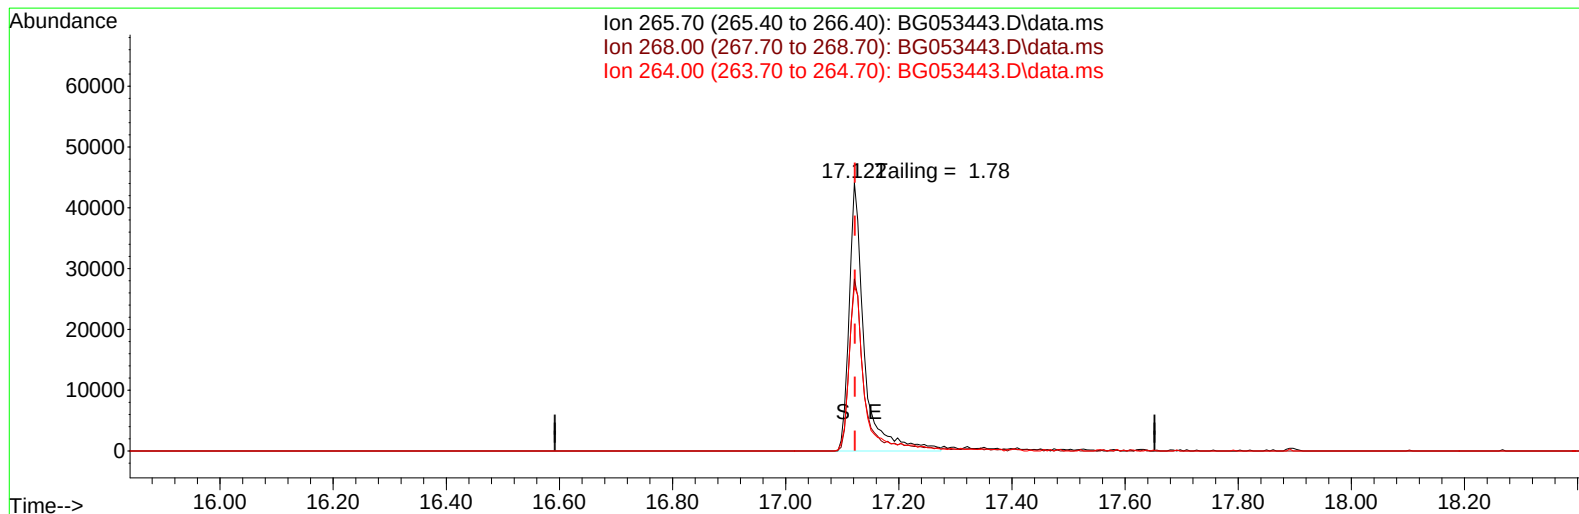

TIC: BG053443.D\data.ms

(70) Pentachlorophenol (C)




17.122min (-0.000) 21631.19 ng

response 82401

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.08
264.00	66.20	61.22
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\  
Data File : BG053443.D  
Acq On    : 5 May 2022    8:41  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 06 06:15:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

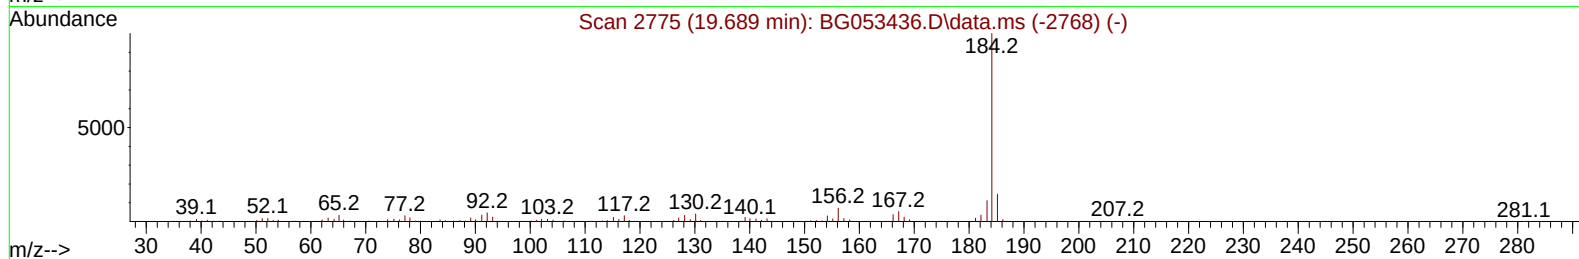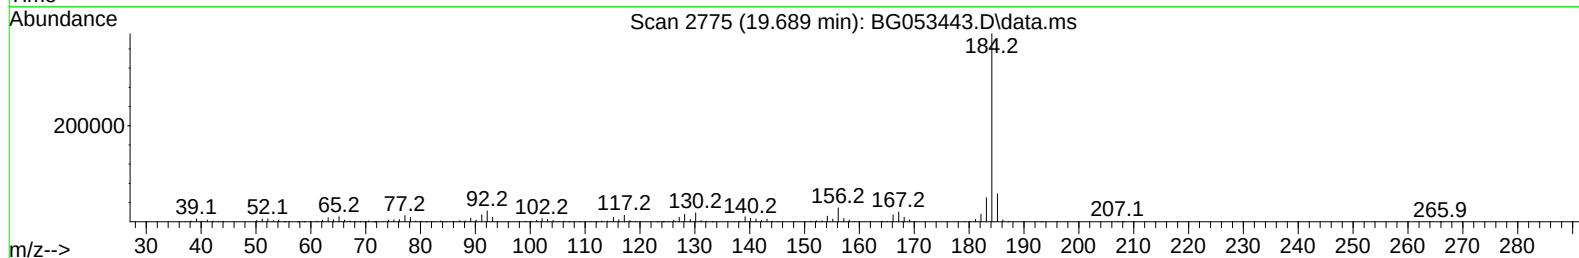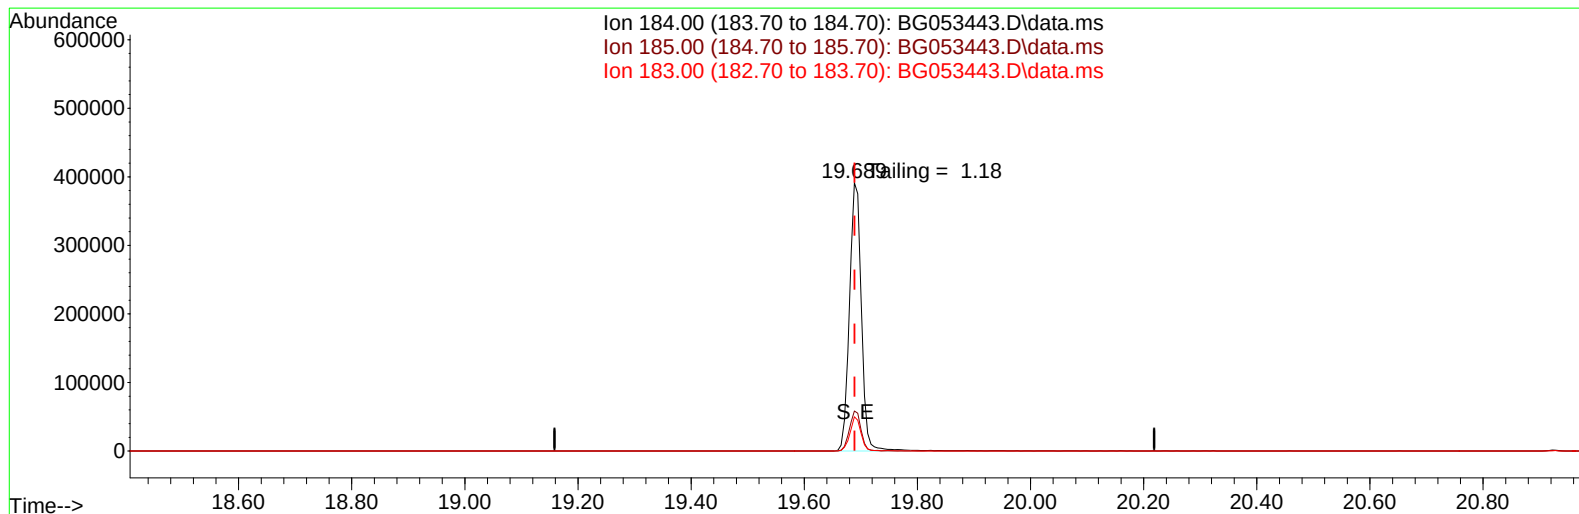

TIC: BG053443.D\data.ms

(77) Benzidine

19.689min (-0.000) 55567.00 ng

response **573686**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.89
183.00	11.10	12.80
0.00	0.00	0.00