


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
 Data File : BG053431.D
 Acq On : 4 May 2022 16:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 02:13:53 2022

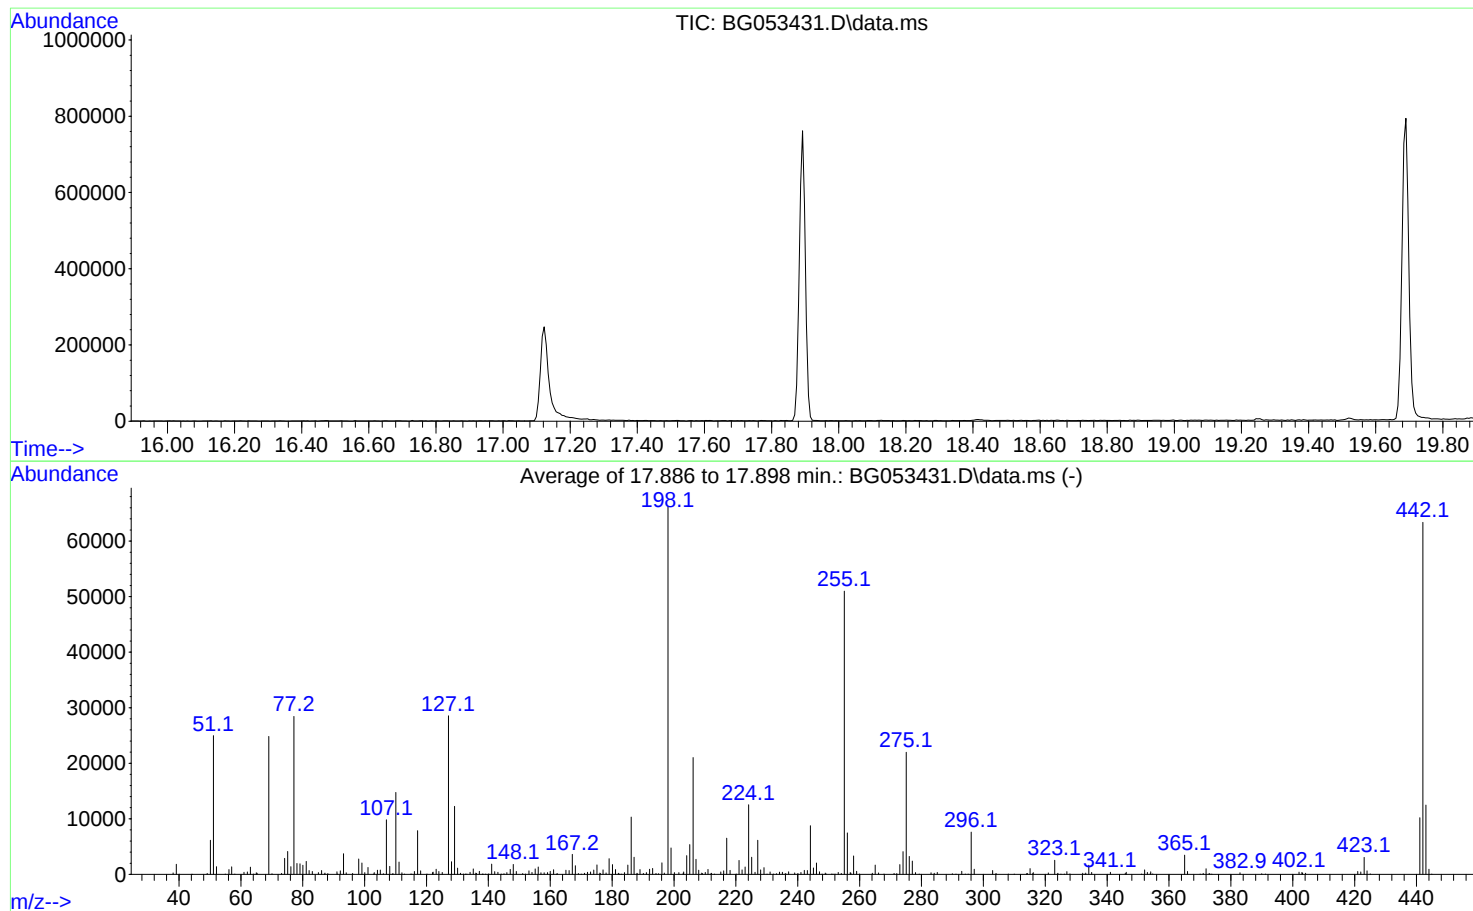




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	24979	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	24843	PASS
70	69	0.00	2	0.5	129	PASS
127	198	10	80	43.1	28560	PASS
197	198	0.00	2	0.4	243	PASS
198	198	100	100	100.0	66229	PASS
199	198	5	9	7.2	4744	PASS
275	198	10	60	33.2	21987	PASS
365	198	1	100	5.2	3472	PASS
441	198	0.01	100	15.4	10203	PASS
442	442	50	100	100.0	63379	PASS
443	442	15	24	19.7	12479	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053431.D
Acq On : 4 May 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 05 06:36:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

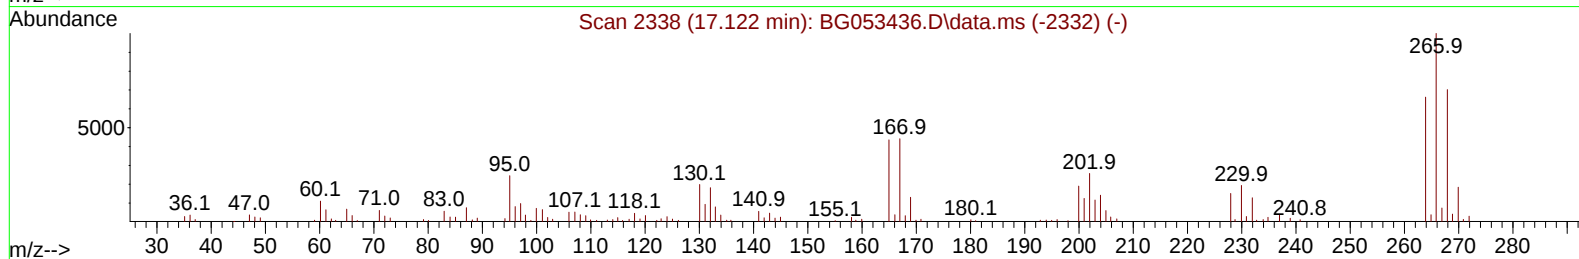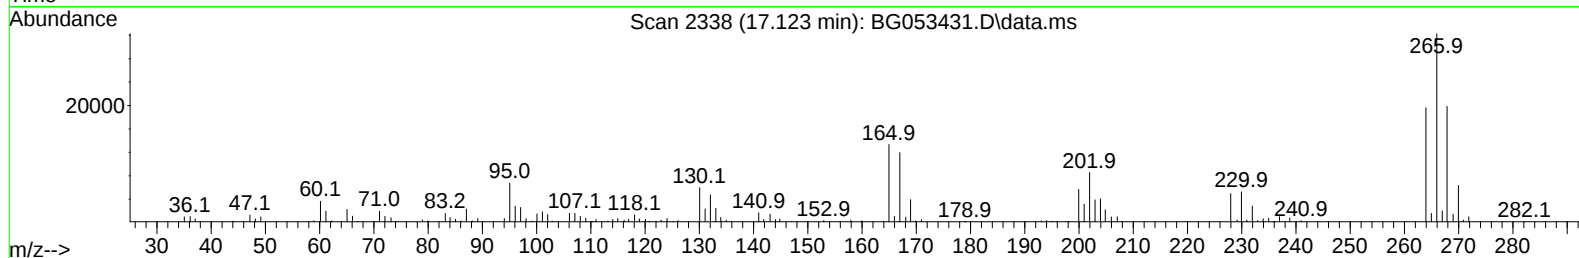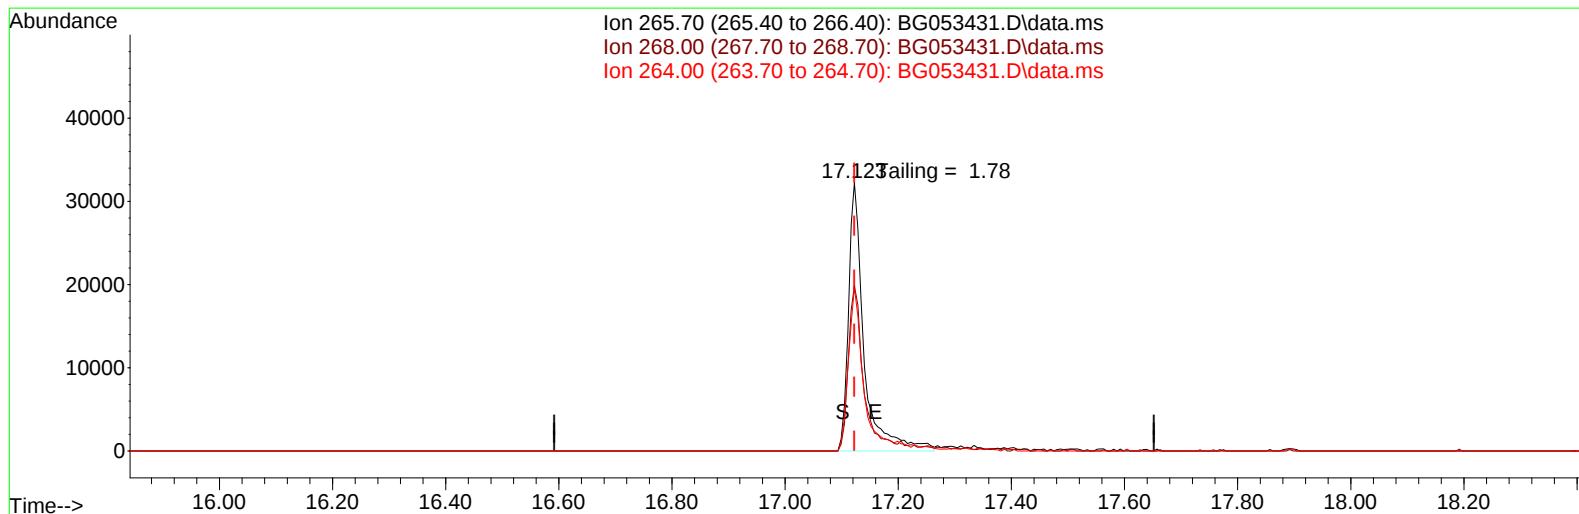

TIC: BG053431.D\data.ms

(70) Pentachlorophenol (C)

17.123min (+ 0.001) 20690.52 ng




response 60512

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	61.51
264.00	66.20	60.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053431.D
Acq On : 4 May 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 05 06:36:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

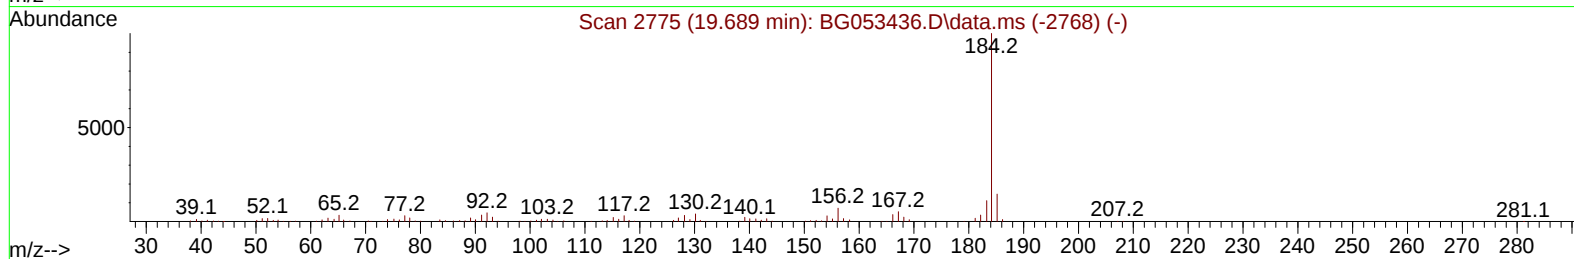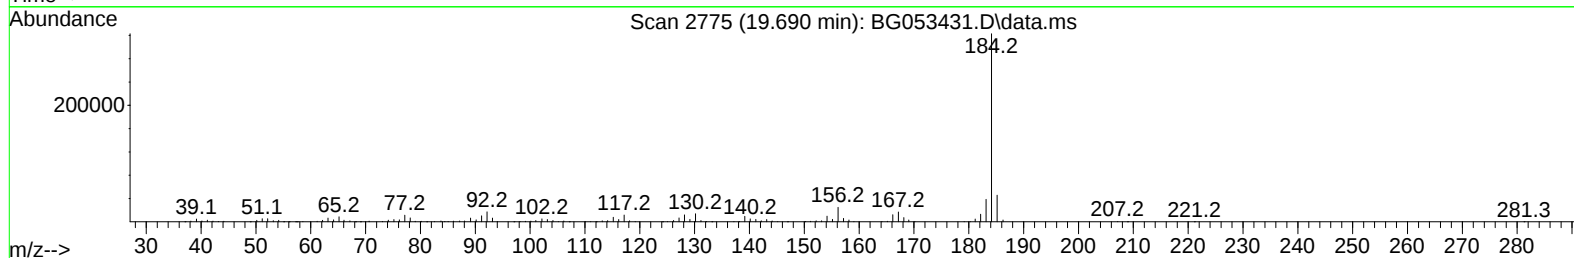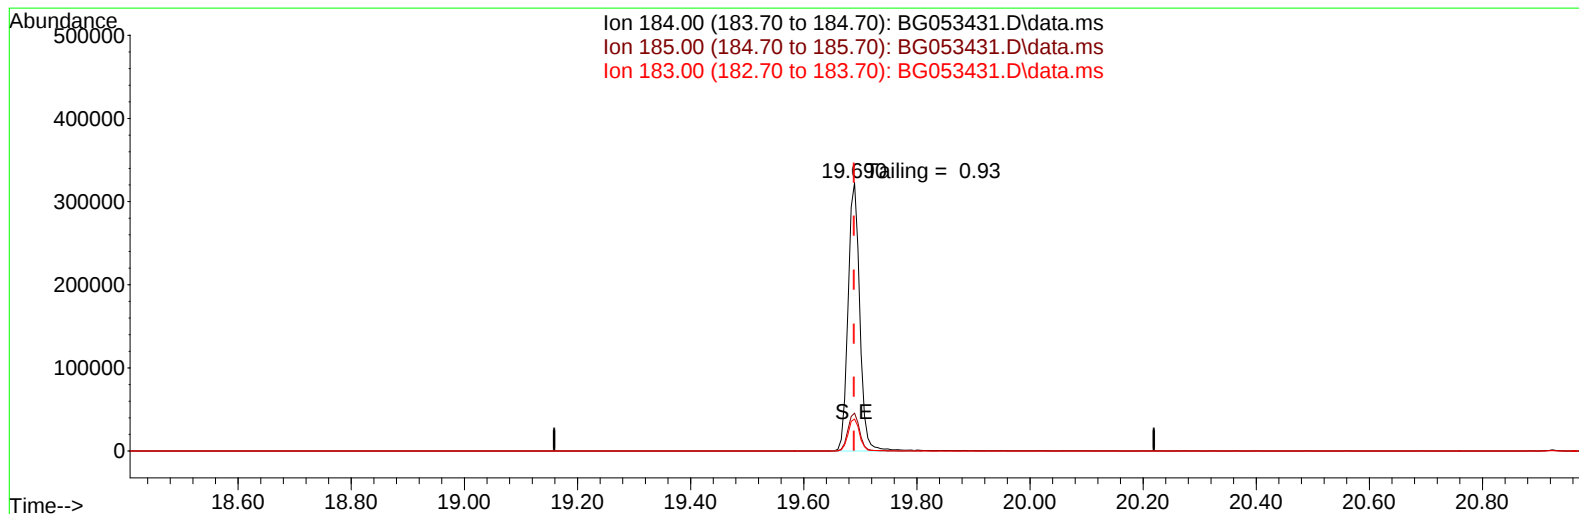

TIC: BG053431.D\data.ms

(77) Benzidine

19.690min (+ 0.001) 139835.00 ng

response 464150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.16
183.00	11.10	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/5/2022	BNA_G	<u>BG053431.D</u>
Compound Name	Response	Retention Time
DDT	252391	20.923
DDD	2741	20.53
DDE	84	20.001
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2825	255216	1.11

Instrument :
BNA_G
ClientSampleId :
DFTPP