
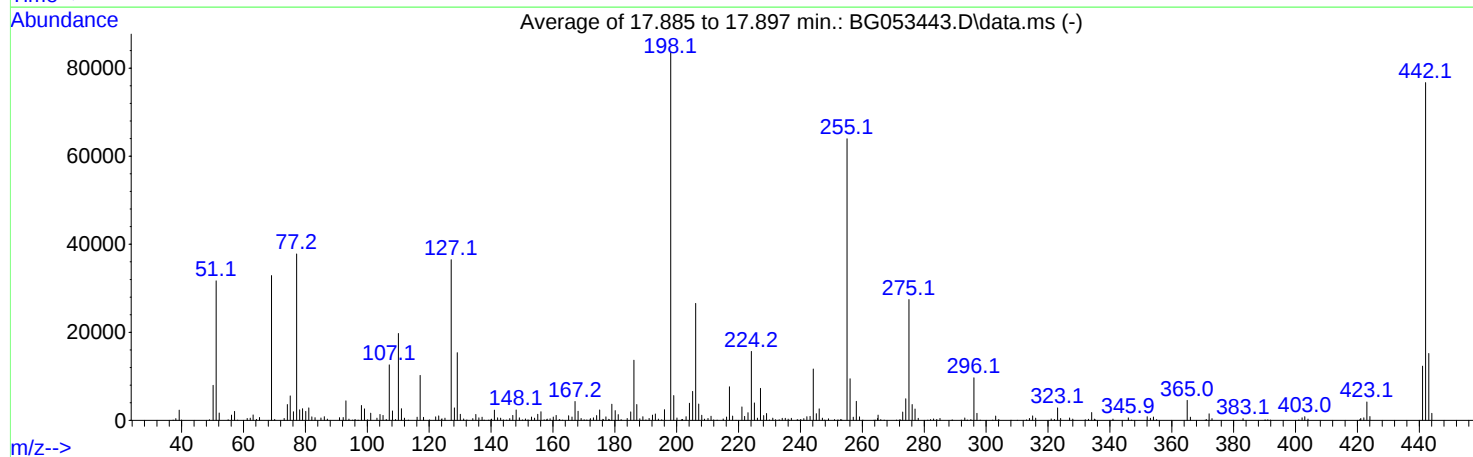


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
 Data File : BG053443.D
 Acq On : 5 May 2022 8:41
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 02:13:53 2022

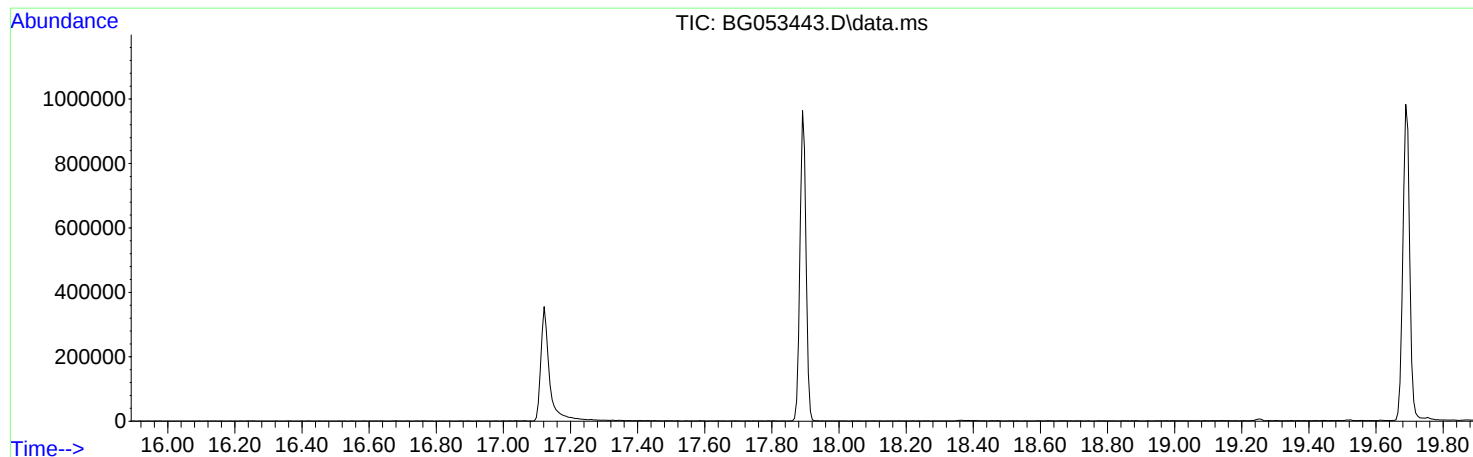




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	31704	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.4	32904	PASS
70	69	0.00	2	0.6	204	PASS
127	198	10	80	43.7	36477	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83557	PASS
199	198	5	9	6.7	5622	PASS
275	198	10	60	32.8	27437	PASS
365	198	1	100	5.4	4531	PASS
441	198	0.01	100	14.8	12327	PASS
442	442	50	100	100.0	76739	PASS
443	442	15	24	19.8	15197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053443.D
Acq On : 5 May 2022 8:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 06:15:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

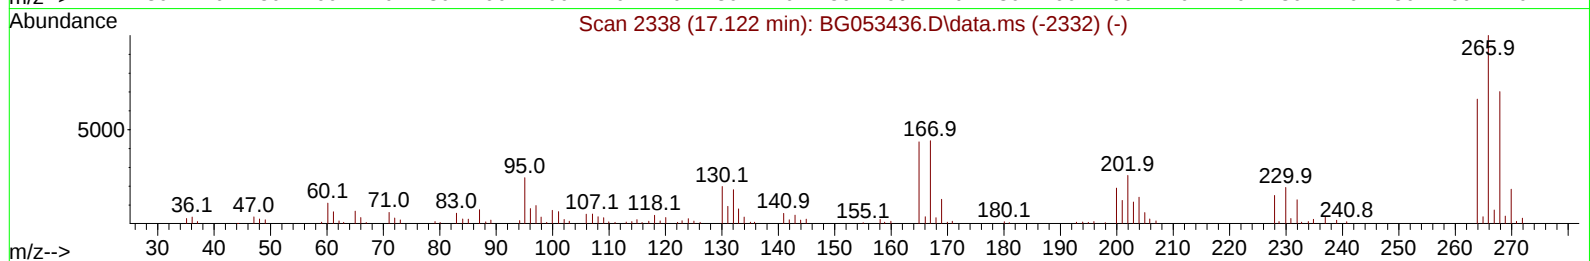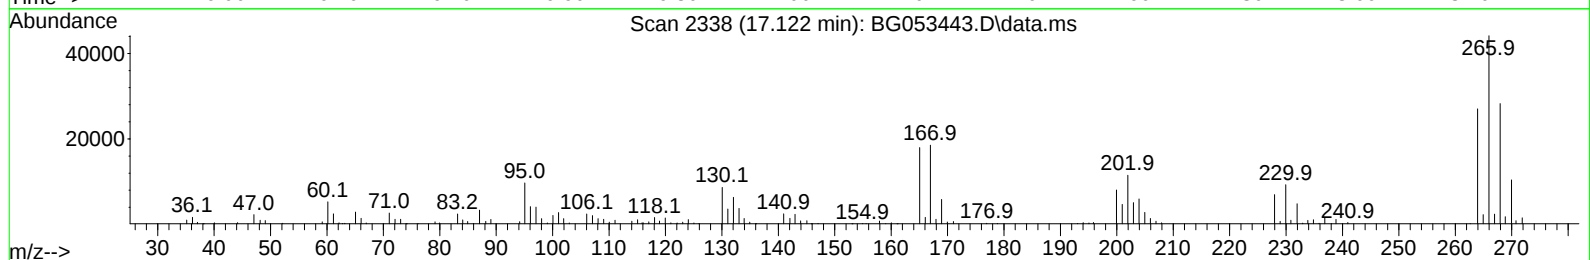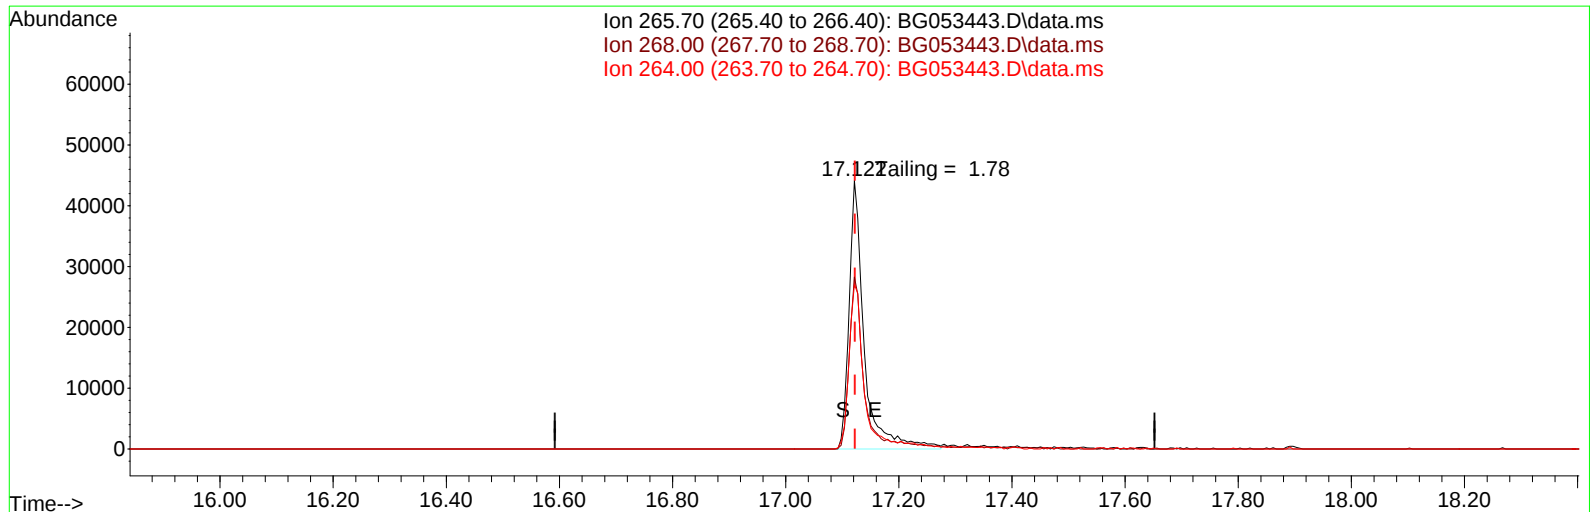

TIC: BG053443.D\data.ms

(70) Pentachlorophenol (C)

17.122min (-0.000) 21631.19 ng




response 82401

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	64.08
264.00	66.20	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053443.D
Acq On : 5 May 2022 8:41
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 06:15:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

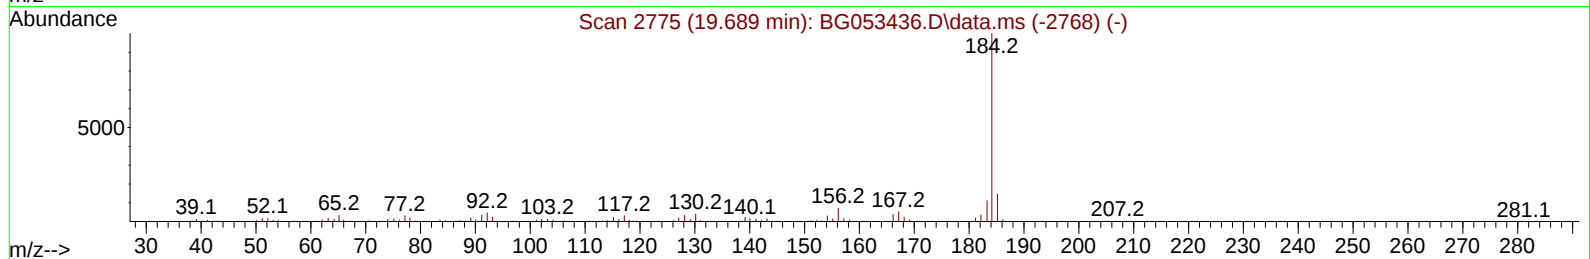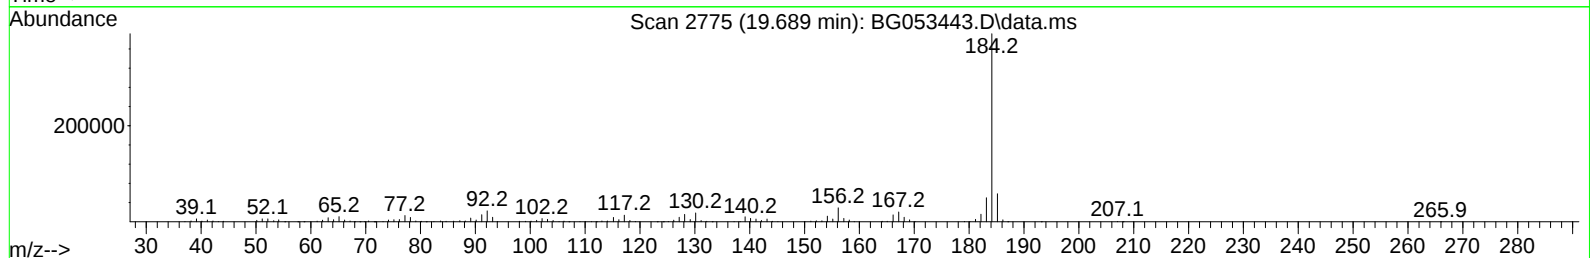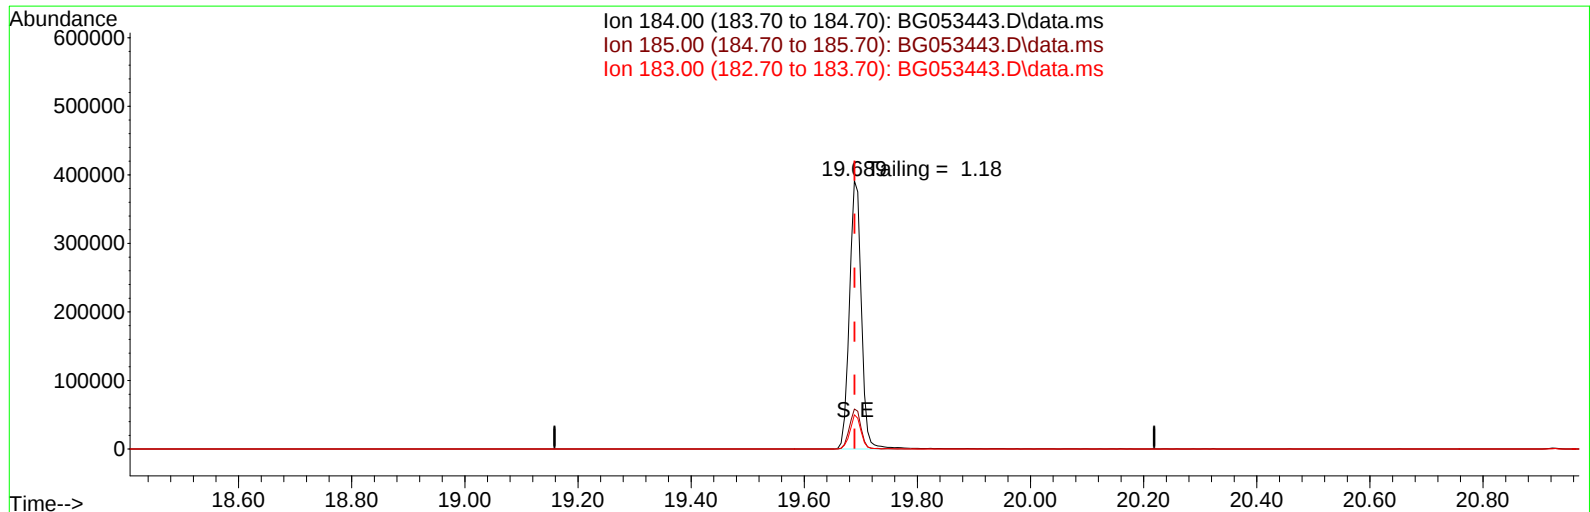

TIC: BG053443.D\data.ms

(77) Benzidine

19.689min (-0.000) 55567.00 ng

response 573686

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.89
183.00	11.10	12.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/5/2022	BNA_G	<u>BG053443.D</u>
Compound Name	Response	Retention Time
DDT	320118	20.922
DDD	4511	20.476
DDE	224	19.976
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4735	324853	1.46

Instrument :
BNA_G
ClientSampleId :
DFTPP