
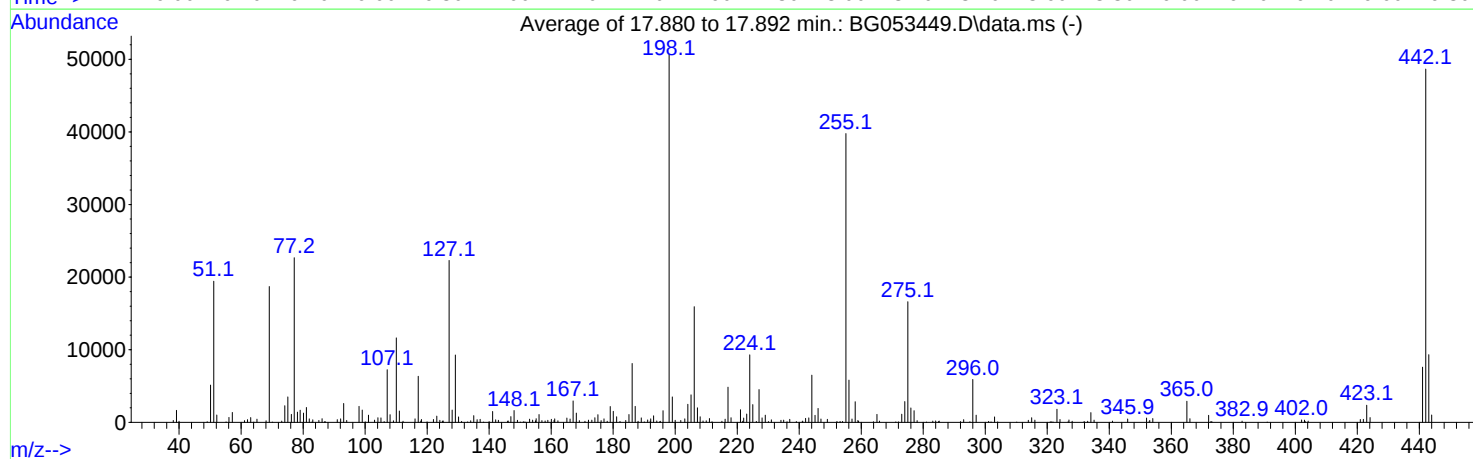


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
 Data File : BG053449.D
 Acq On : 5 May 2022 14:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 02:13:53 2022

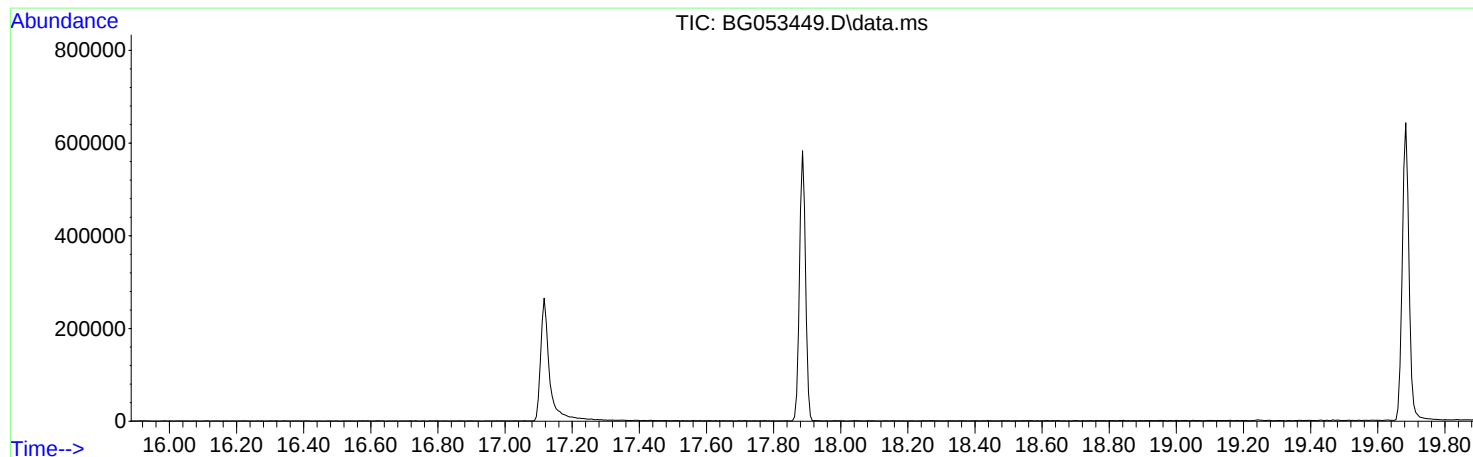




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	19435	PASS
68	69	0.00	2	1.2	220	PASS
69	198	0.00	100	37.0	18719	PASS
70	69	0.00	2	0.3	51	PASS
127	198	10	80	44.0	22299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	50659	PASS
199	198	5	9	6.9	3515	PASS
275	198	10	60	32.8	16604	PASS
365	198	1	100	5.8	2921	PASS
441	198	0.01	100	15.0	7597	PASS
442	442	50	100	100.0	48659	PASS
443	442	15	24	19.2	9324	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\
Data File : BG053449.D
Acq On : 5 May 2022 14:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 06:28:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

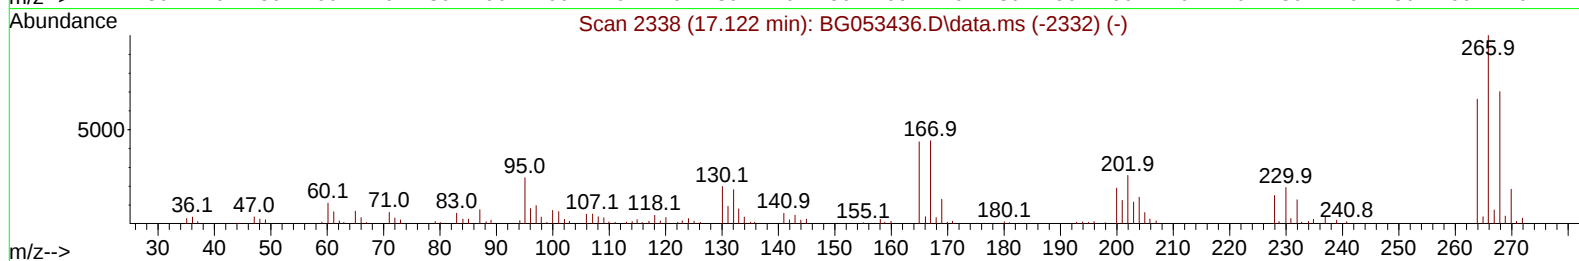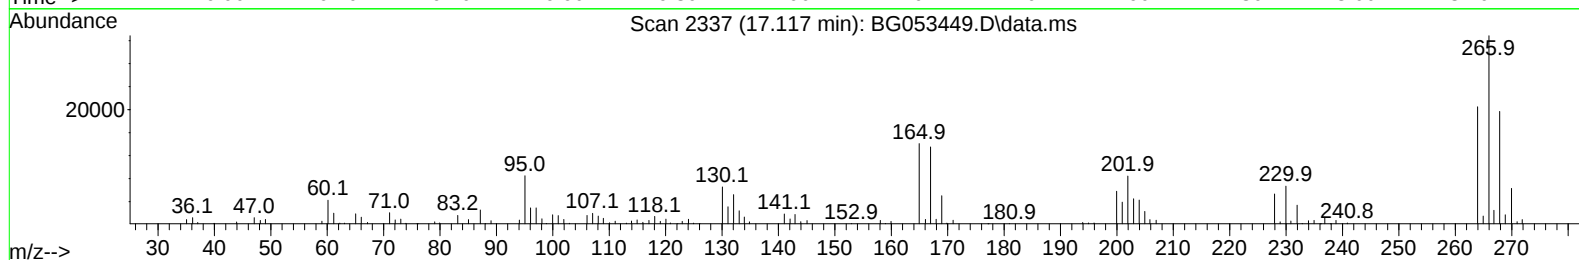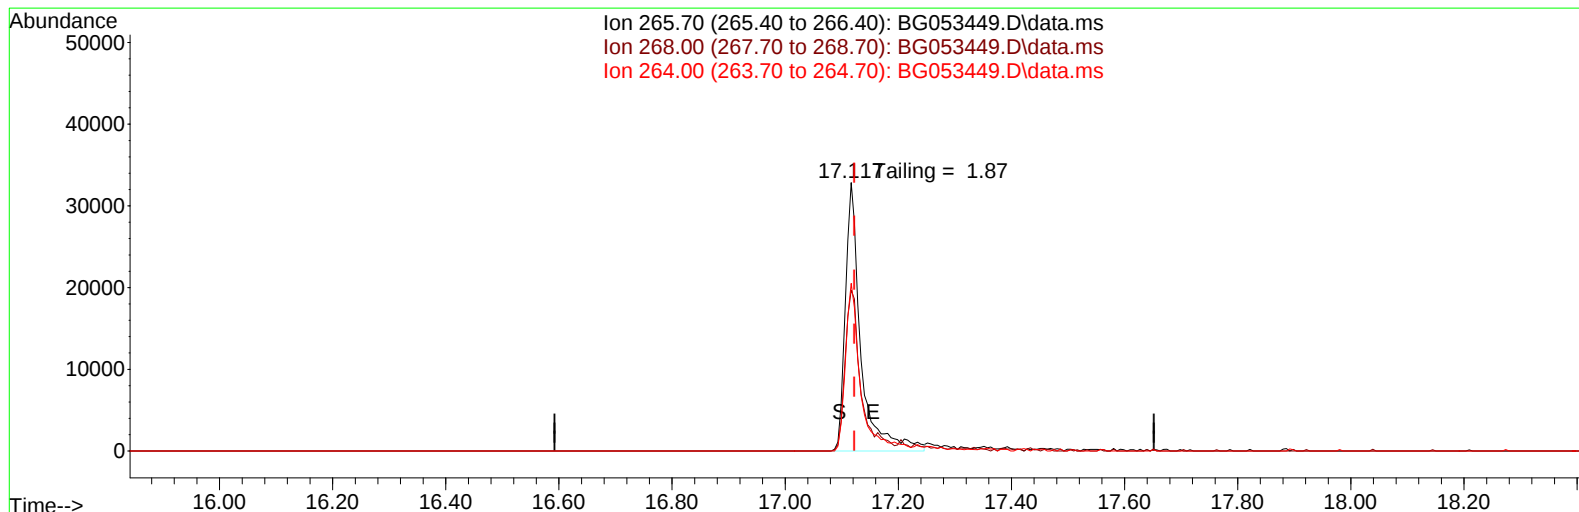

TIC: BG053449.D\data.ms

(70) Pentachlorophenol (C)

17.117min (-0.005) 36822.67 ng




response 60583

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	59.91
264.00	66.20	62.42
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050522\  
Data File : BG053449.D  
Acq On    : 5 May 2022 14:01  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 06:28:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

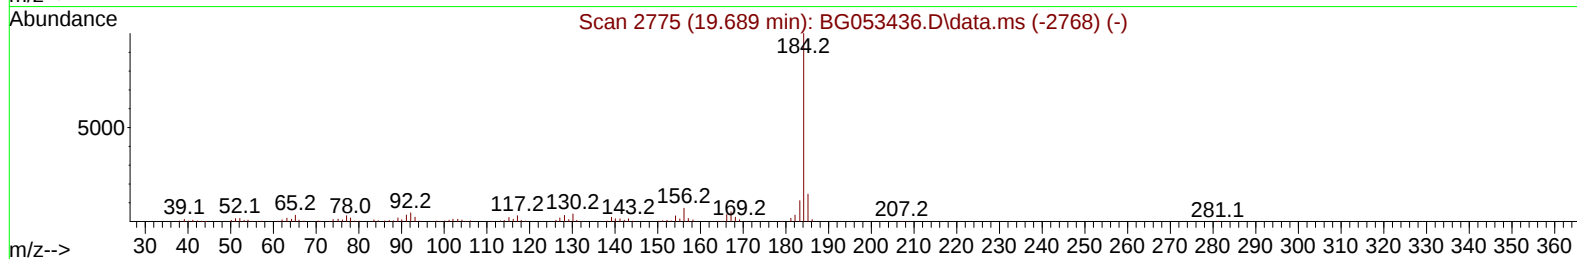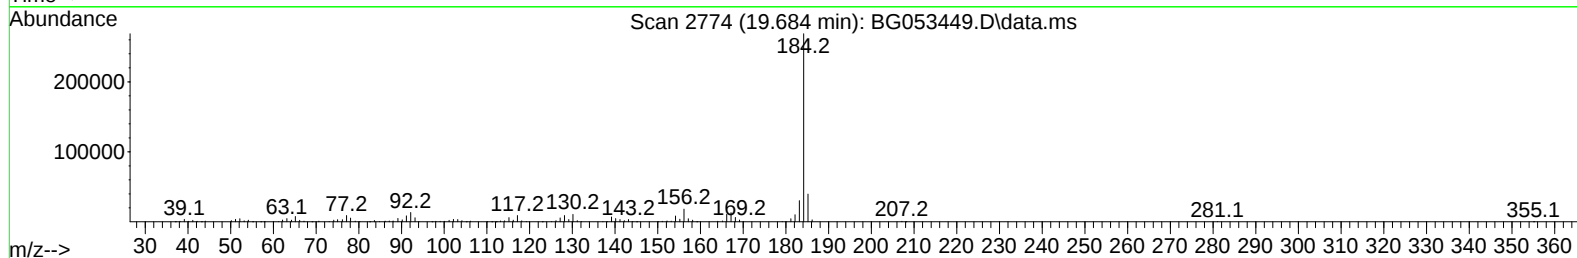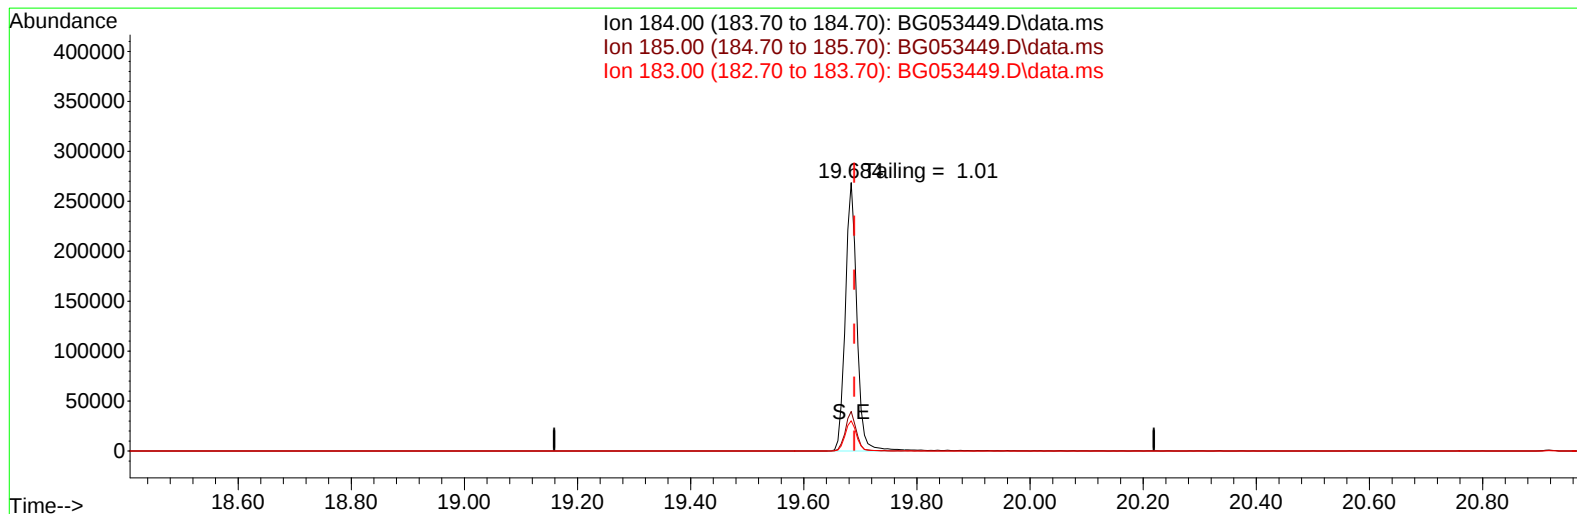

TIC: BG053449.D\data.ms

(77) Benzidine

19.684min (-0.005) 0.00 ng

response **379556**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.77
183.00	11.10	11.28
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/5/2022	BNA_G	<u>BG053449.D</u>
Compound Name	Response	Retention Time
DDT	199109	20.917
DDD	3012	20.477
DDE	139	19.977
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3151	202260	1.56

Instrument :
BNA_G
ClientSampleId :
DFTPP