




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
 Data File : BG057317.D
 Acq On : 5 May 2023 13:35
 Operator : CG/JU
 Sample : 02479-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
 Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 05 23:54:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 11:20:08 2023
 Response via : Initial Calibration

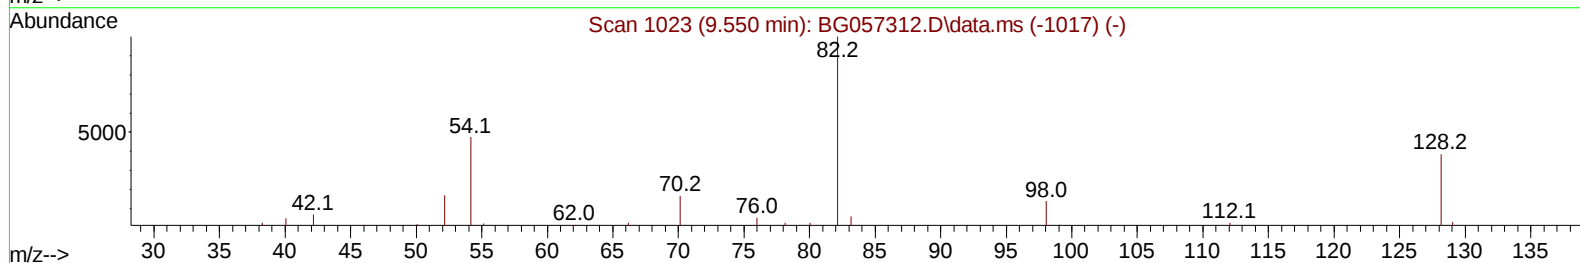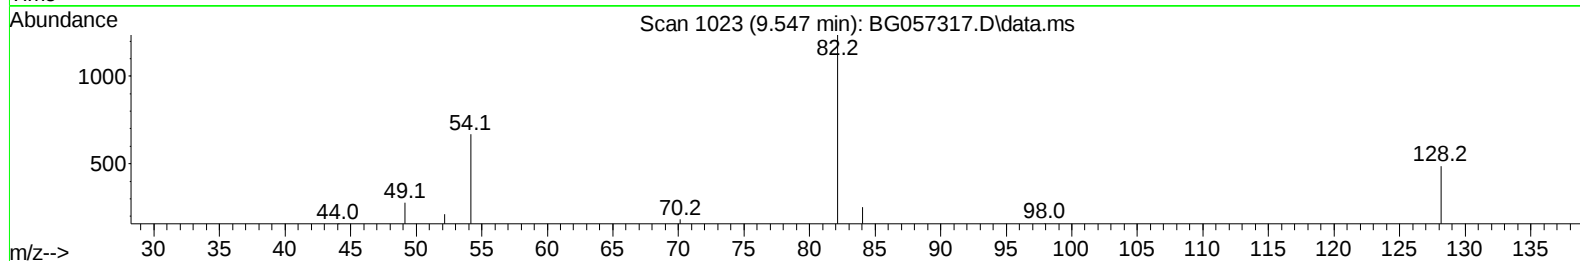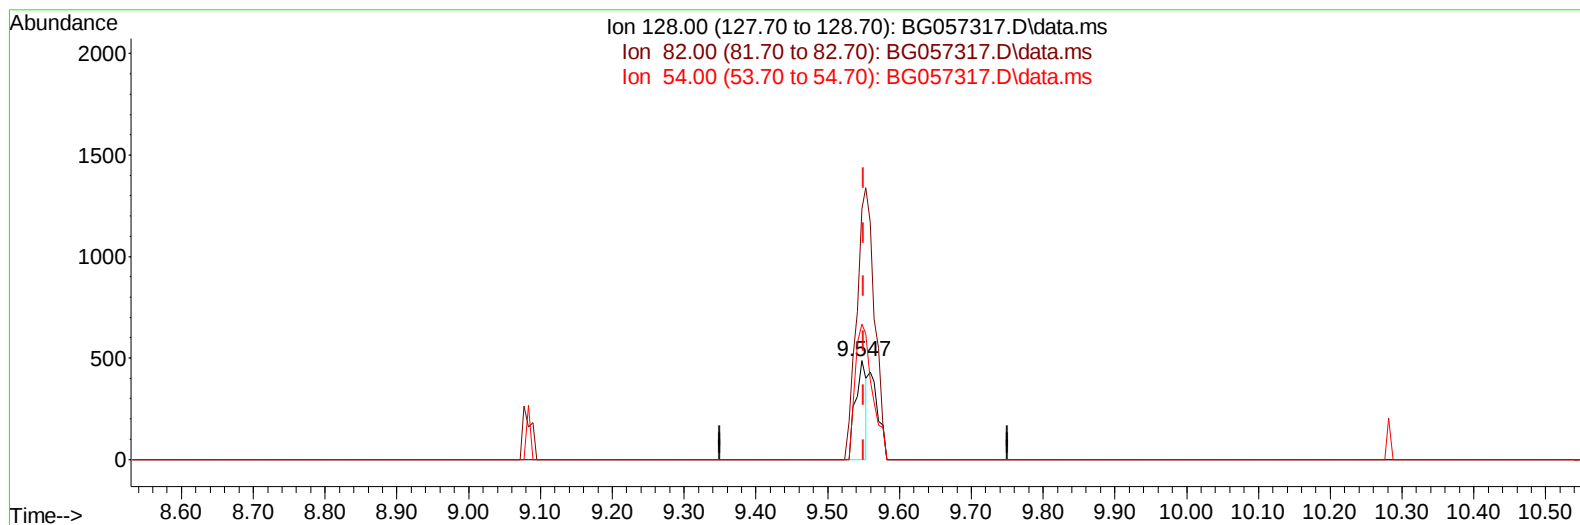

TIC: BG057317.D\data.ms

(21) Nitrobenzene-d5 (S)

9.547min (-0.003) 0.79 ng/u1

response 513

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	259.80	254.12
54.00	119.00	137.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
Data File : BG057317.D
Acq On : 5 May 2023 13:35
Operator : CG/JU
Sample : 02479-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 05 23:54:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 11:20:08 2023
Response via : Initial Calibration

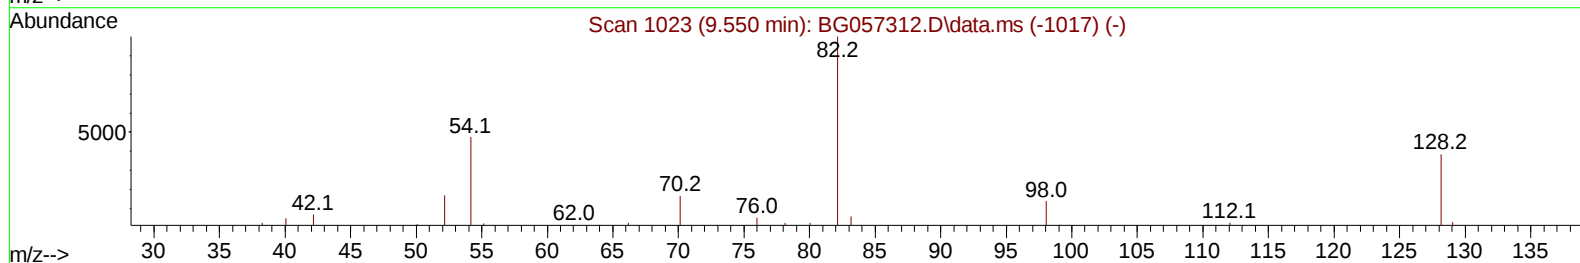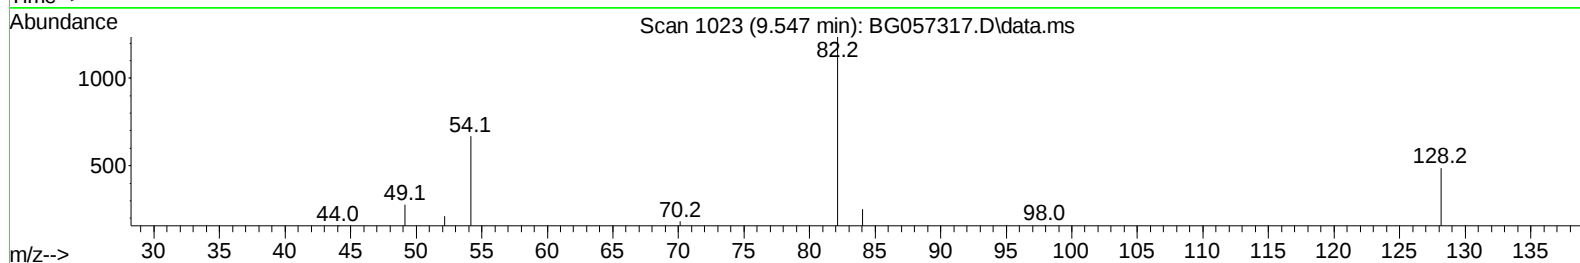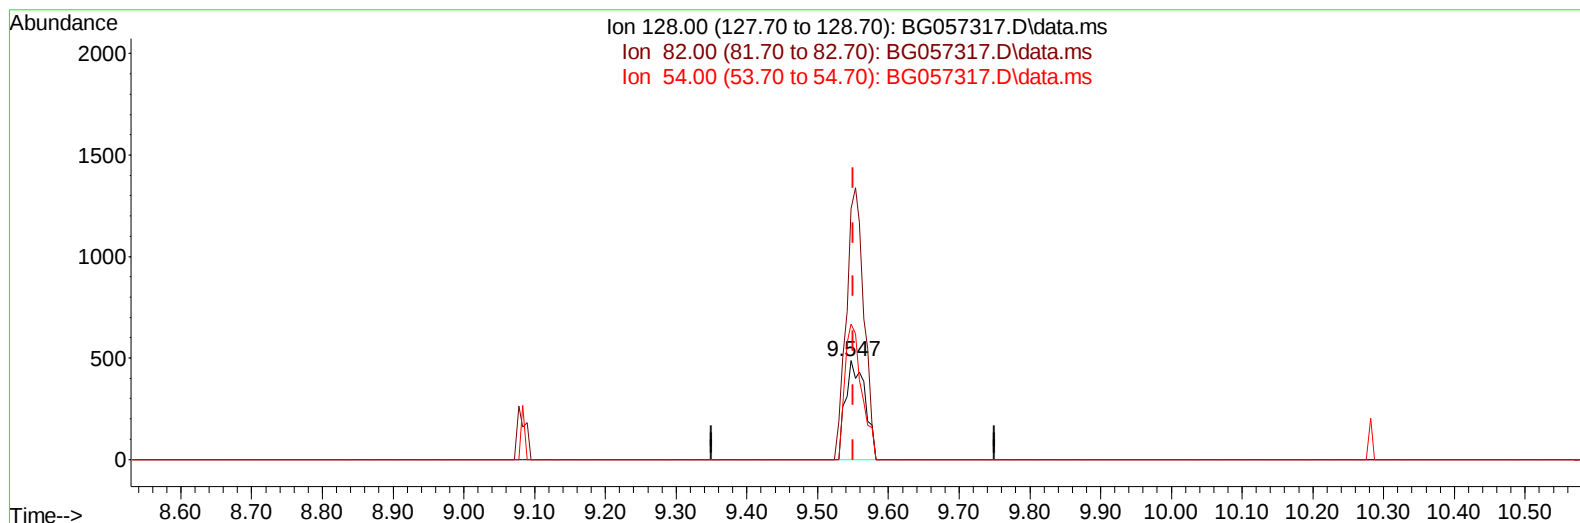

TIC: BG057317.D\data.ms

(21) Nitrobenzene-d5 (S)

9.547min (-0.003) 1.42 ng/ul m

response 925

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	259.80	254.12
54.00	119.00	137.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
Data File : BG057317.D
Acq On : 5 May 2023 13:35
Operator : CG/JU
Sample : 02479-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 06 00:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 11:20:08 2023
Response via : Initial Calibration

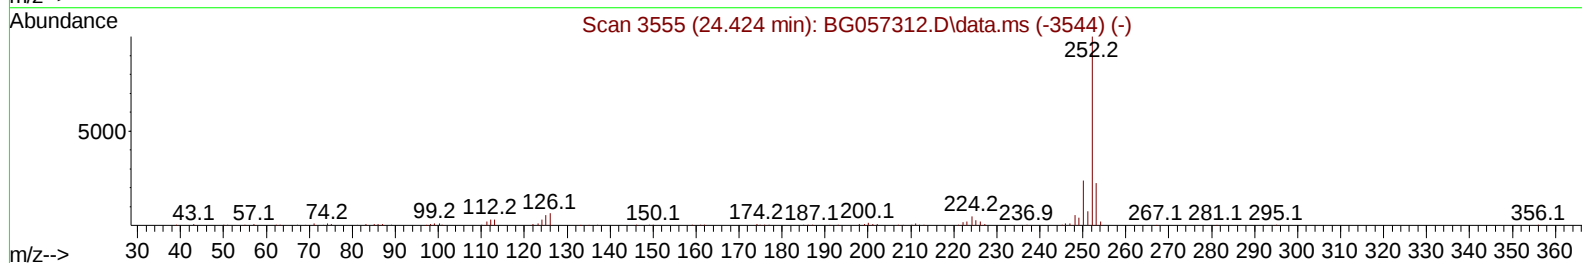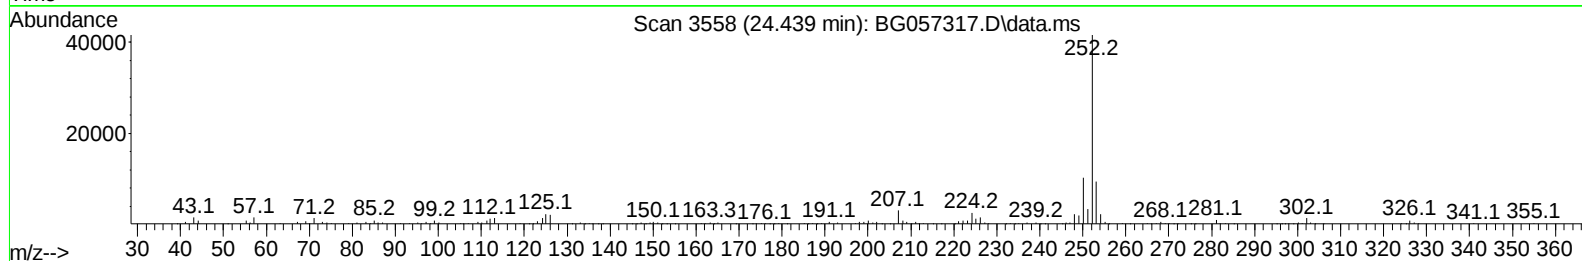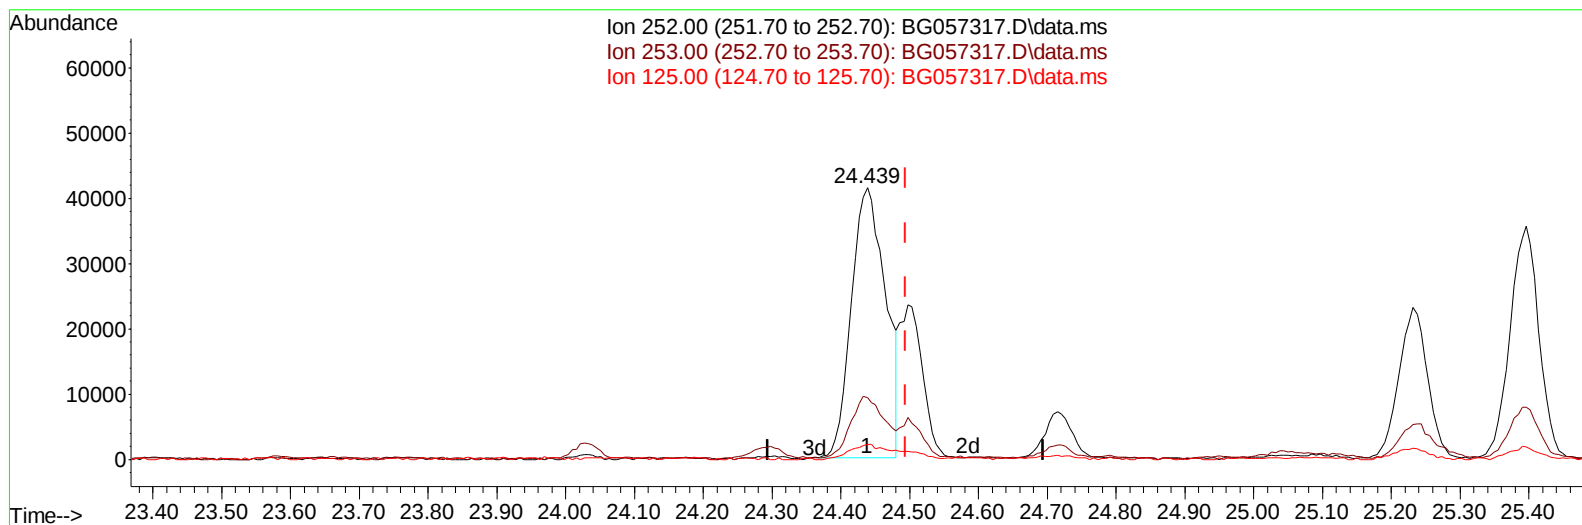

TIC: BG057317.D\data.ms

(91) Benzo(k)fluoranthene

24.439min (-0.056) 15.74 ng/u1

response 143325

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	22.81
125.00	5.60	5.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
Data File : BG057317.D
Acq On : 5 May 2023 13:35
Operator : CG/JU
Sample : 02479-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 06 00:37:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 11:20:08 2023
Response via : Initial Calibration

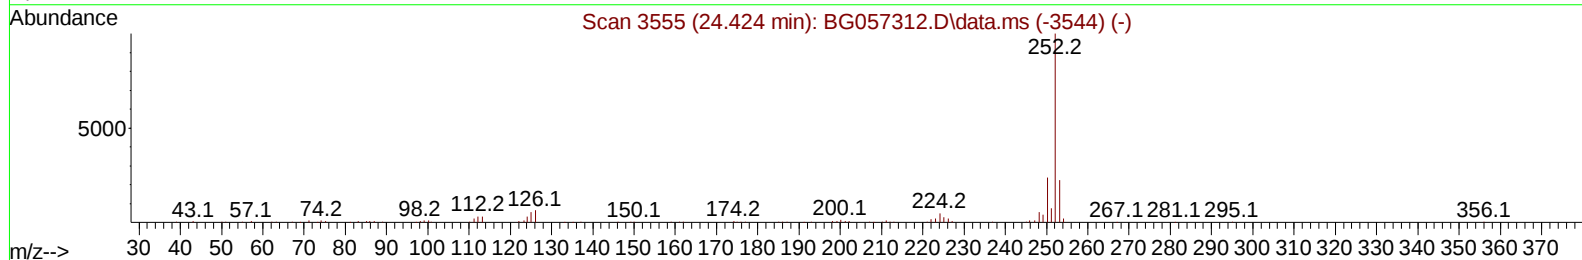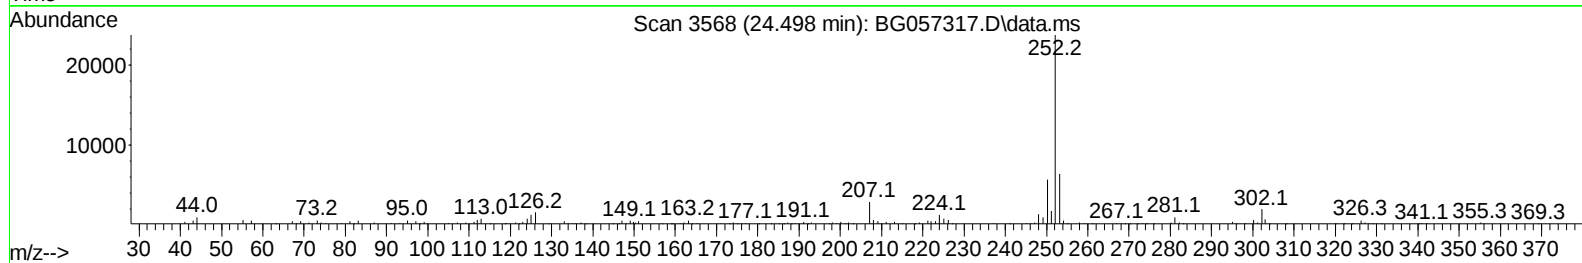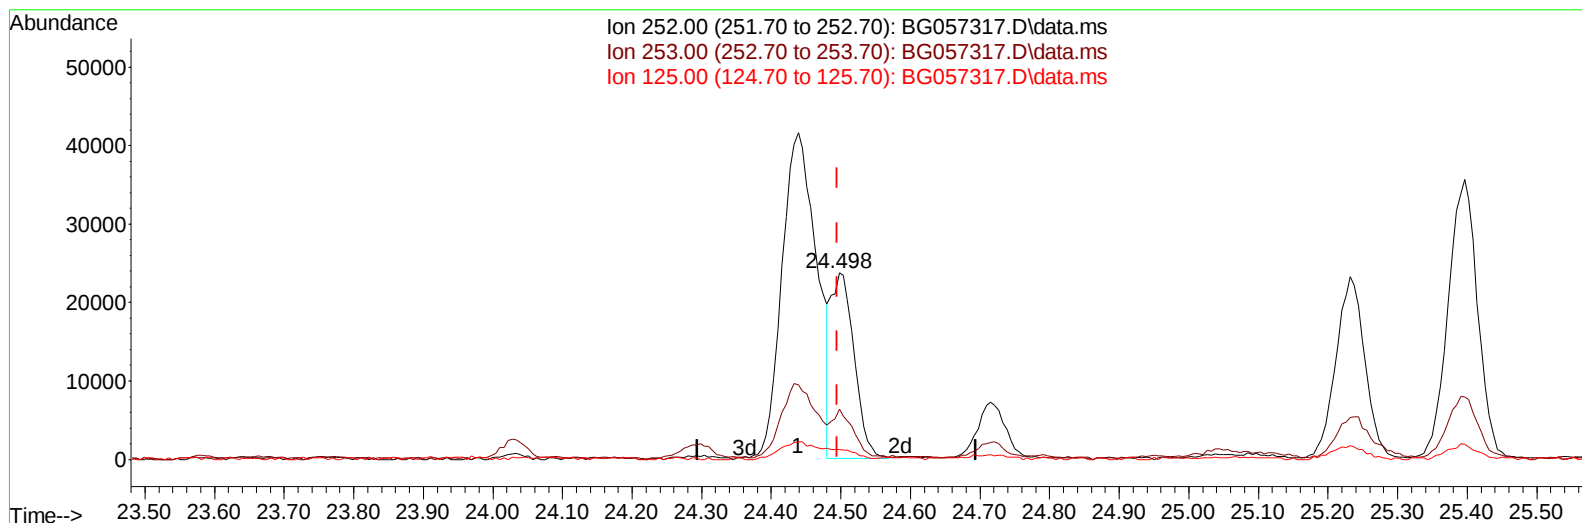

TIC: BG057317.D\data.ms

(91) Benzo(k)fluoranthene

24.498min (+ 0.003) 5.94 ng/u1 m

response 54043

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	22.10	26.94#
125.00	5.60	5.27
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
 Data File : BG057317.D
 Acq On : 5 May 2023 13:35
 Operator : CG/JU
 Sample : 02479-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Quant Time: May 06 00:38:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 11:20:08 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/08/2023
 Supervised By :Jagrut Upadhyay 05/08/2023

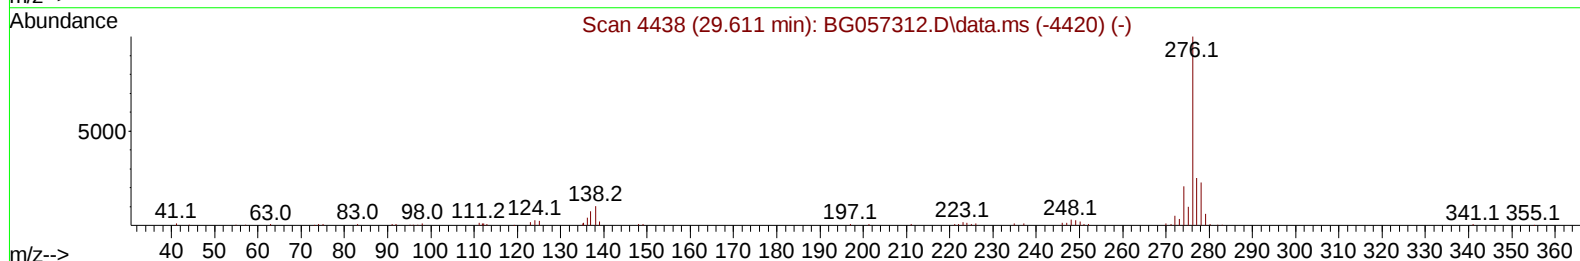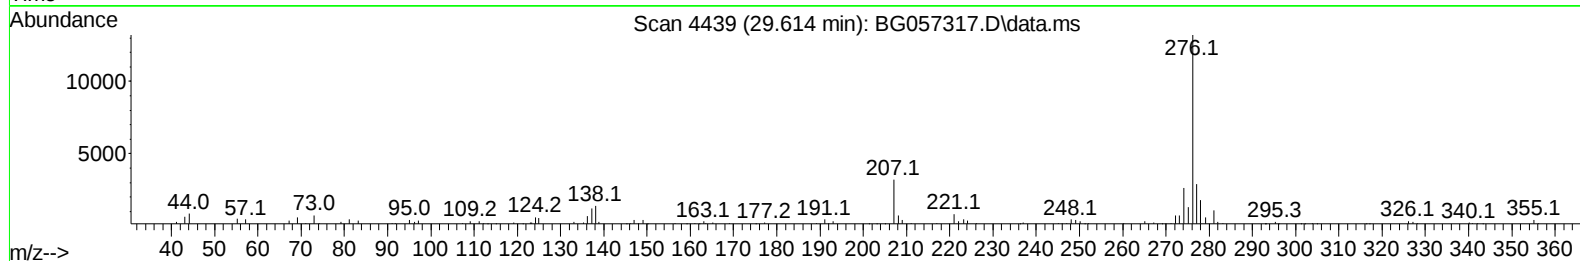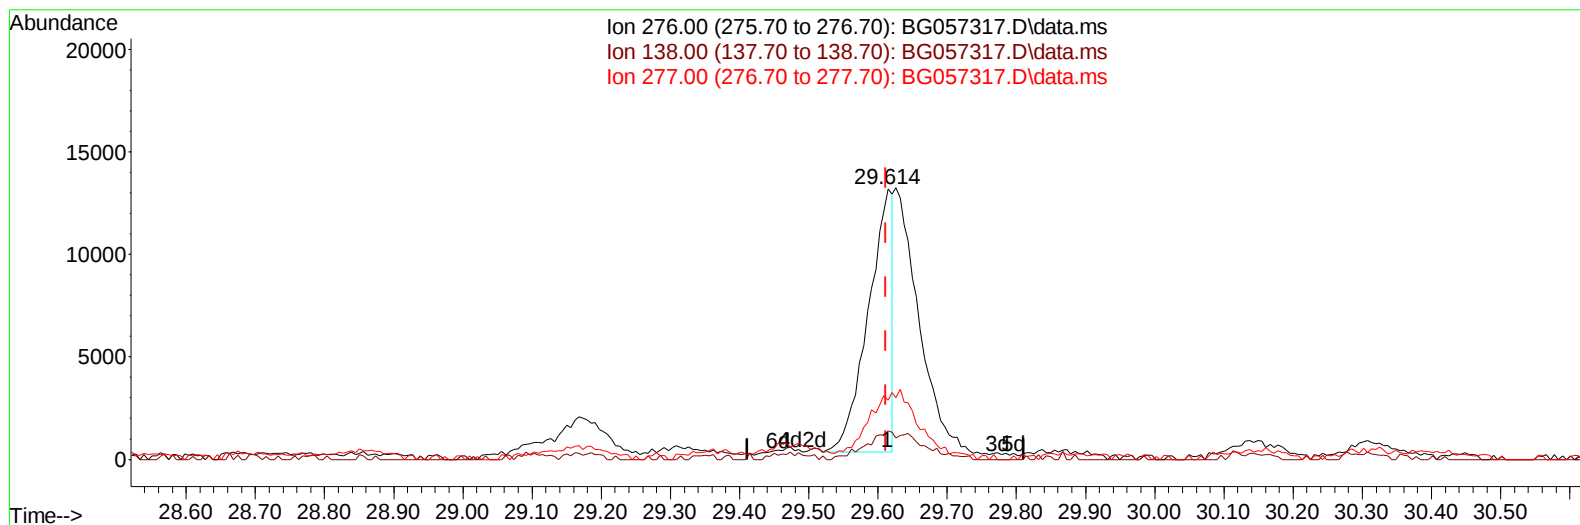

TIC: BG057317.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.614min (+ 0.003) 3.13 ng/u1

response 31618

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	11.80	10.51
277.00	23.30	22.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
Data File : BG057317.D
Acq On : 5 May 2023 13:35
Operator : CG/JU
Sample : 02479-07 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 06 00:38:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 05 11:20:08 2023
Response via : Initial Calibration

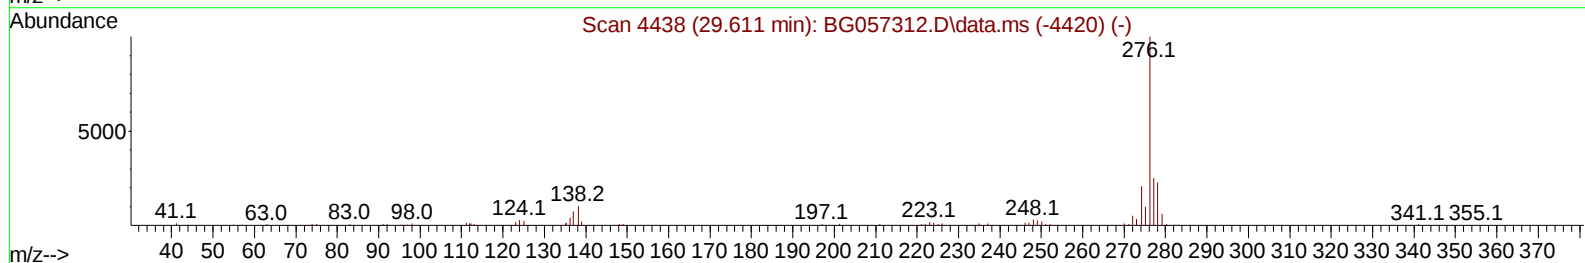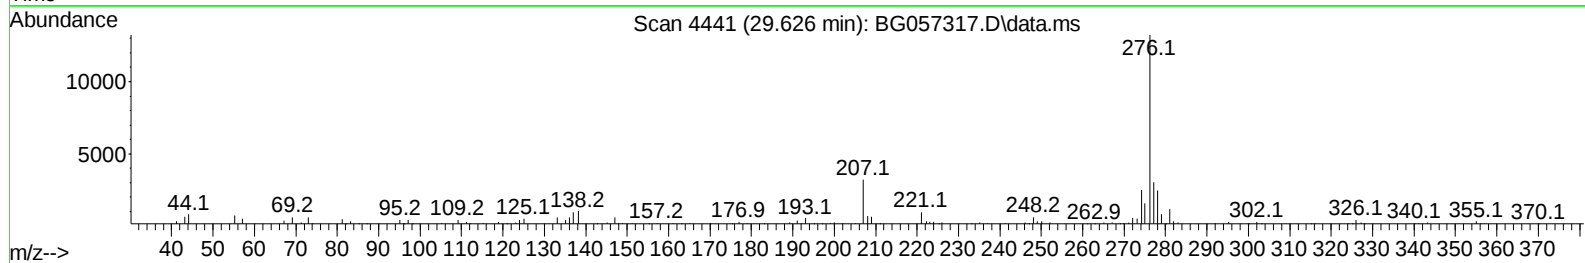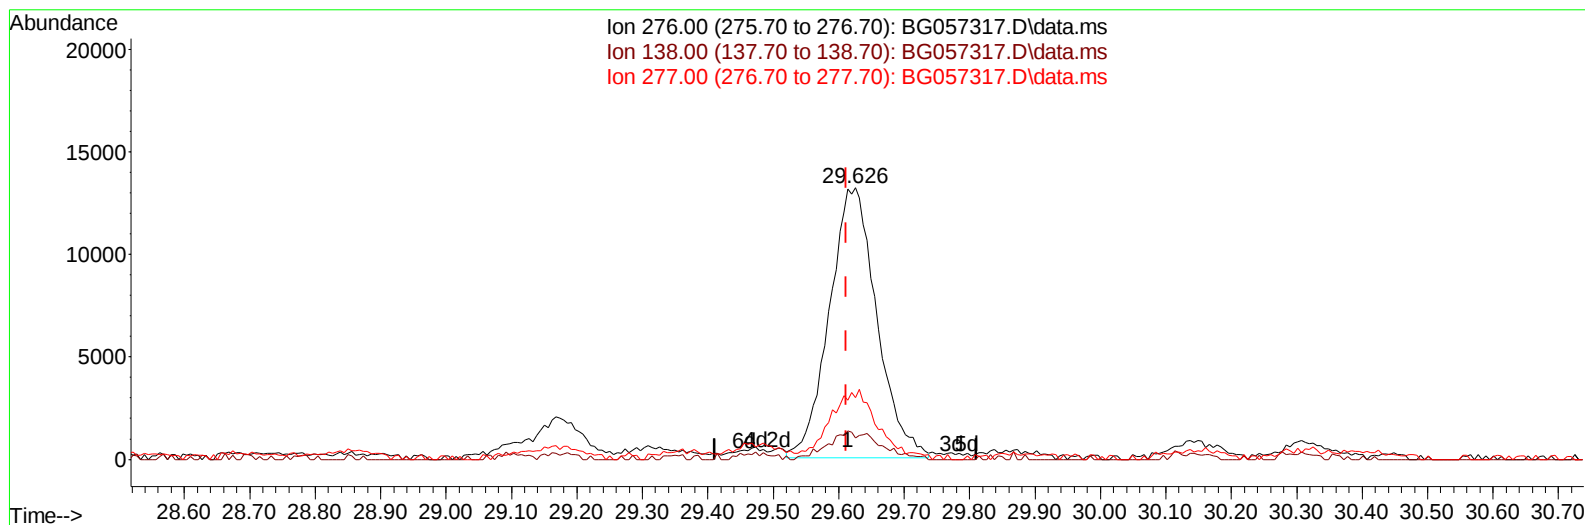

TIC: BG057317.D\data.ms

(94) Indeno(1,2,3-cd)pyrene

29.626min (+ 0.015) 6.55 ng/ul m

response 66192

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	11.80	7.83#
277.00	23.30	22.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
 Data File : BG057317.D
 Acq On : 5 May 2023 13:35
 Operator : CG/JU
 Sample : 02479-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
 Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 06 00:38:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 11:20:08 2023
 Response via : Initial Calibration

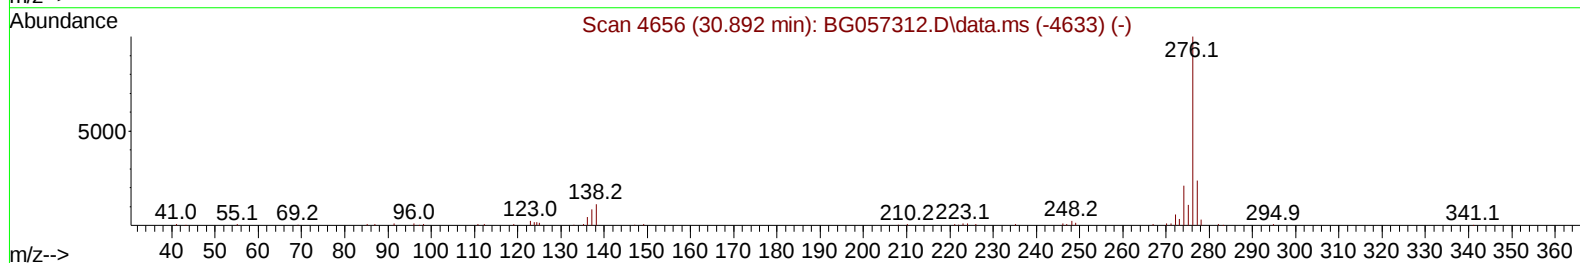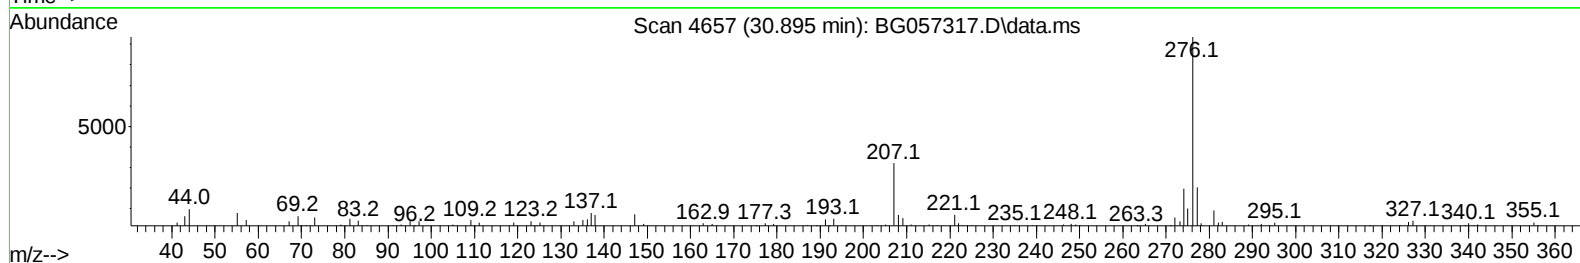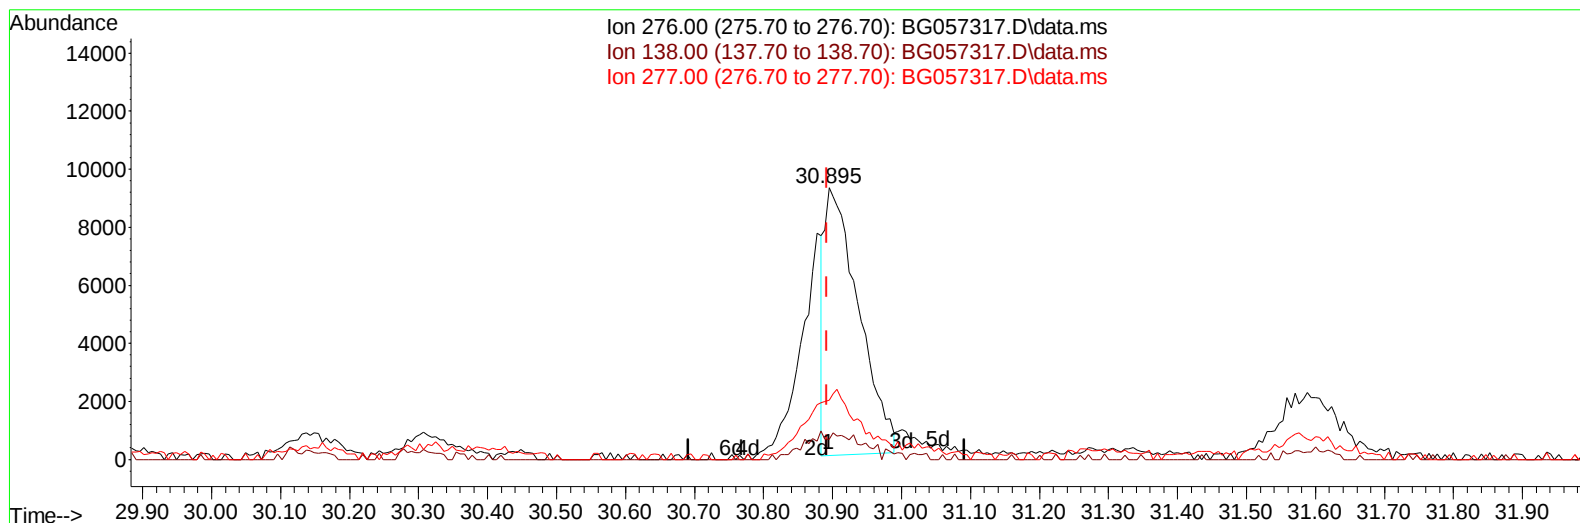

TIC: BG057317.D\data.ms

(96) Benzo(g,h,i)perylene

30.895min (+ 0.003) 3.84 ng/u1

response 31421

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.90	7.40#
277.00	23.00	21.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
 Data File : BG057317.D
 Acq On : 5 May 2023 13:35
 Operator : CG/JU
 Sample : 02479-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 05/08/2023
 Supervised By :Jagrut Upadhyay 05/08/2023

Quant Time: May 06 00:38:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 11:20:08 2023
 Response via : Initial Calibration

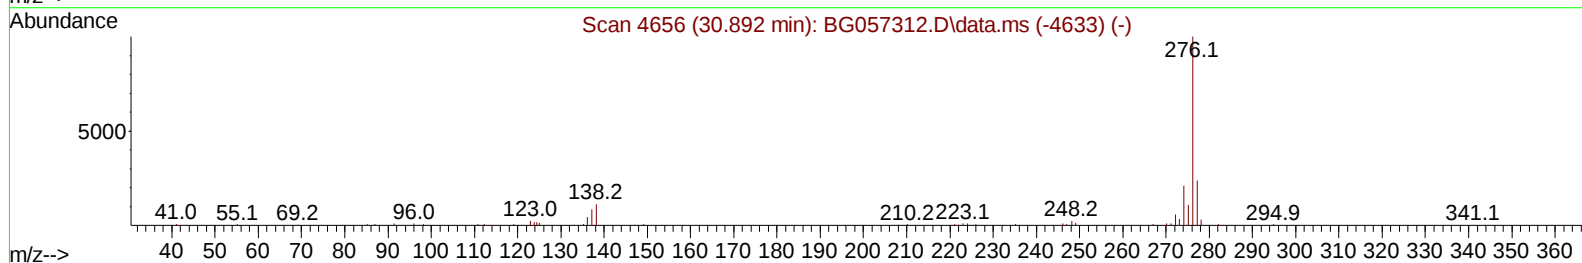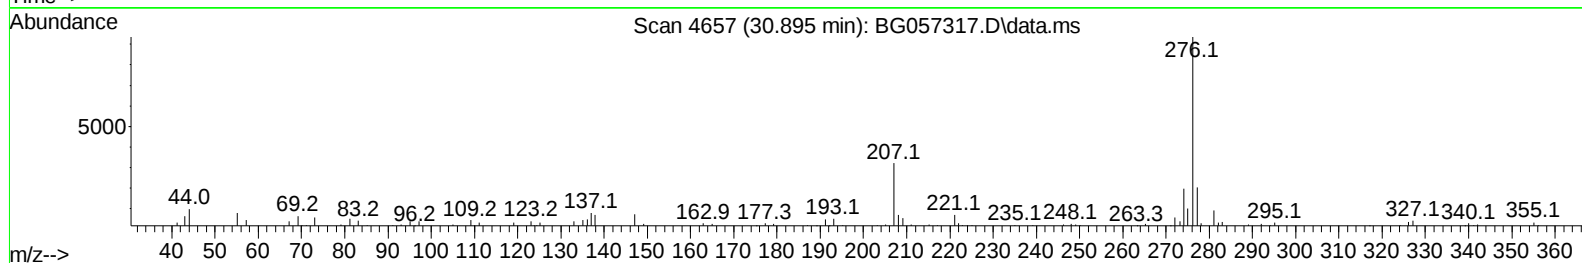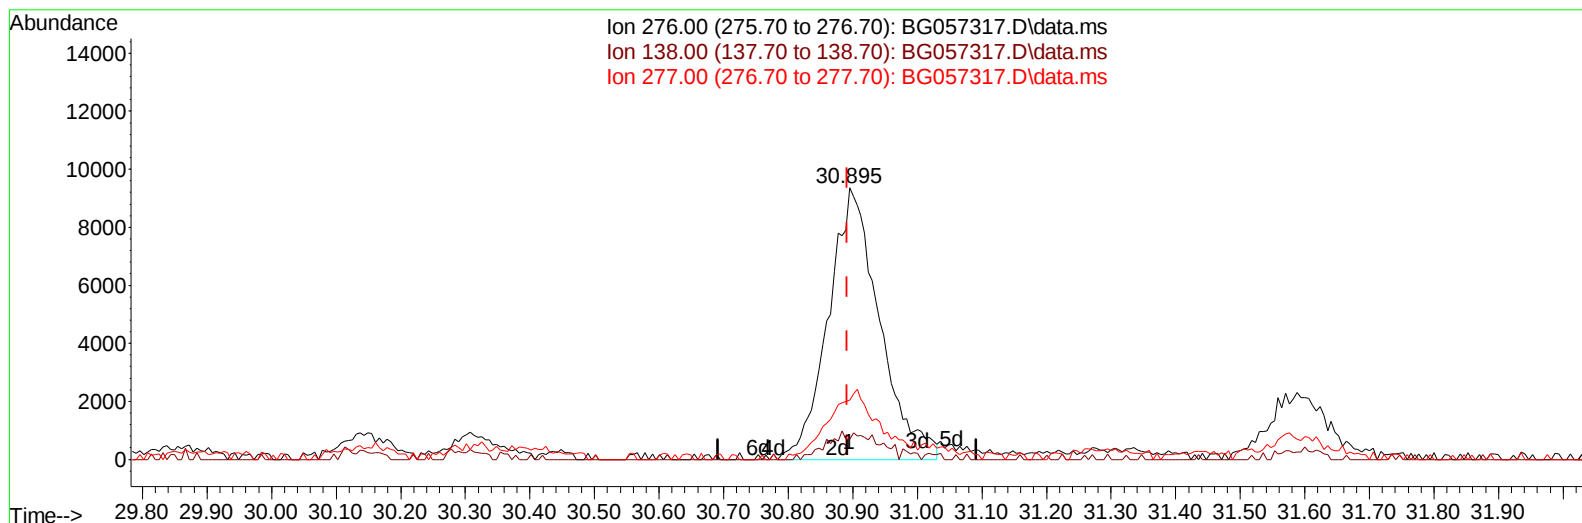

TIC: BG057317.D\data.ms

(96) Benzo(g,h,i)perylene

30.895min (+ 0.003) 6.29 ng/ul m

response 51402

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	10.90	7.40#
277.00	23.00	21.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050523\
 Data File : BG057317.D
 Acq On : 5 May 2023 13:35
 Operator : CG/JU
 Sample : 02479-07 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EW948

Manual IntegrationsAPPROVED

Quant Time: May 06 00:39:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG042823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 05 11:20:08 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 05/08/2023
 Supervised By :Jagrut Upadhyay 05/08/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.372	152		18144	20.000	ng/ul	0.00
20) Naphthalene-d8	11.210	136		81981	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.987	164		66466	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.730	188		148947	20.000	ng/ul	0.00
79) Chrysene-d12	22.042	240		126025	20.000	ng/ul	# 0.00
88) Perylene-d12	25.567	264		135128	20.000	ng/ul	0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	0.000	96		0	0.000	ng/uL	
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.515	99		1945	1.134	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.679	67		1410	1.397	ng/ul	0.00
11) 2-Chlorophenol-d4	7.902	132		1463	1.294	ng/ul	0.00
15) 4-Methylphenol-d8	9.083	113		1594	1.222	ng/ul	0.00
21) Nitrobenzene-d5	9.547	128		925m	1.417	ng/ul	0.00
24) 2-Nitrophenol-d4	10.282	143		736	0.966	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.834	165		1656	1.127	ng/ul	0.00
31) 4-Chloroaniline-d4	11.345	131		1373	0.705	ng/ul	0.00
46) Dimethylphthalate-d6	14.370	166		7612	1.445	ng/ul	0.00
49) Acenaphthylene-d8	14.682	160		9135	1.543	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143		0	0.000	ng/ul	
60) Fluorene-d10	15.968	176		7354	1.499	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200		0	0.000	ng/ul	
73) Anthracene-d10	17.824	188		11496	1.691	ng/ul	0.00
81) Pyrene-d10	20.092	212		13152	1.758	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.314	264		12463	1.810	ng/ul	0.00
Target Compounds							
						Qvalue	
30) Naphthalene	11.263	128		8989	1.997	ng/ul	98
52) Acenaphthene	15.052	153		18831	4.394	ng/ul	98
56) Dibenzofuran	15.381	168		13753	2.222	ng/ul	90
61) Fluorene	16.027	166		20239	3.867	ng/ul	98
72) Phenanthrene	17.771	178		228092	29.407	ng/ul	99
74) Anthracene	17.860	178		58868	7.556	ng/ul	97
77) Carbazole	18.124	167		26811	4.118	ng/ul	98
80) Fluoranthene	19.763	202		307400	34.594	ng/ul	97
82) Pyrene	20.121	202		242493	26.957	ng/ul	98
85) Benzo(a)anthracene	22.019	228		129412	14.519	ng/ul	98
87) Chrysene	22.089	228		124573	14.814	ng/ul	96
90) Benzo(b)fluoranthene	24.439	252		143325	15.317	ng/ul	96
91) Benzo(k)fluoranthene	24.498	252		54043m	5.936	ng/ul	
93) Benzo(a)pyrene	25.396	252		104157	12.893	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	29.626	276		66192m	6.555	ng/ul	
95) Dibenzo(a,h)anthracene	29.649	278		16748	2.000	ng/ul#	82
96) Benzo(g,h,i)perylene	30.895	276		51402m	6.289	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

