

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050615\
 Data File : BG016898.D
 Acq On : 6 May 2015 14:25
 Operator : TP/IZ
 Sample : G2124-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK

Quant Time: May 07 04:16:54 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 07 03:57:31 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	64252	20.00	ng	0.00
21) Naphthalene-d8	10.59	136	301216	20.00	ng	0.00
38) Acenaphthene-d10	14.44	164	203420	20.00	ng	0.00
63) Phenanthrene-d10	17.18	188	454747	20.00	ng	0.00
75) Chrysene-d12	21.36	240	448040	20.00	ng	0.00
86) Perylene-d12	23.66	264	437507	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	6.87	99	61	0.01	ng	-0.10
23) Nitrobenzene-d5	8.95	82	68	0.01	ng	0.00
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	13.03	172	59	0.00	ng	-0.03
78) Terphenyl-d14	19.78	244	68	0.00	ng	-0.03
Target Compounds						
32) Benzoic acid	9.75	122	63	Below Cal		
						Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050615\
Data File : BG016898.D
Acq On : 6 May 2015 14:25
Operator : TP/IZ
Sample : G2124-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Quant Time: May 07 04:16:54 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 07 03:57:31 2015
Response via : Initial Calibration

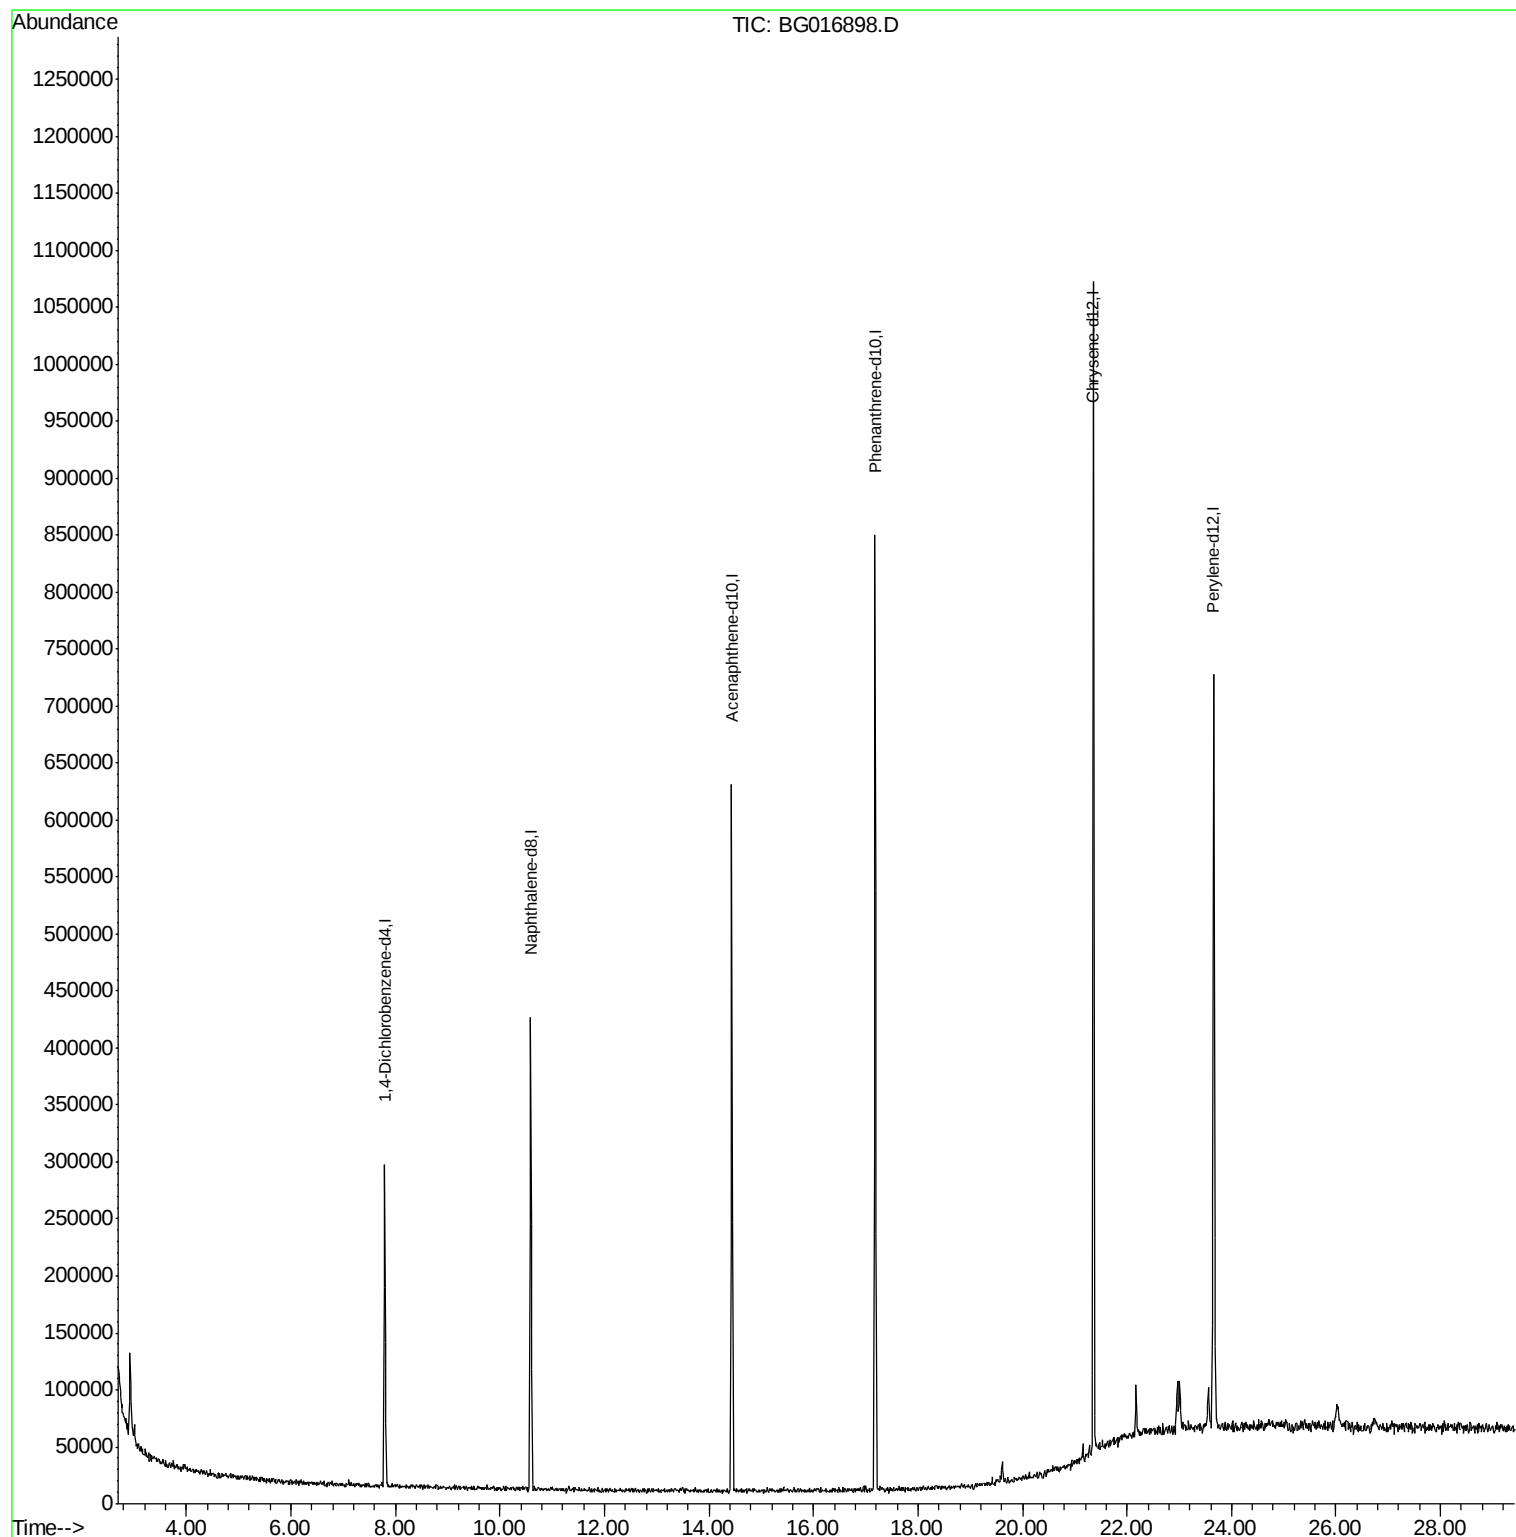




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.80 min Scan# 869
Delta R.T. -0.00 min
Lab File: BG016898.D
Acq: 6 May 2015 14:25

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK

Tgt Ion:152 Resp: 64252
Ion Ratio Lower Upper
152 100
150 143.7 121.0 181.4
115 62.2 50.5 75.7

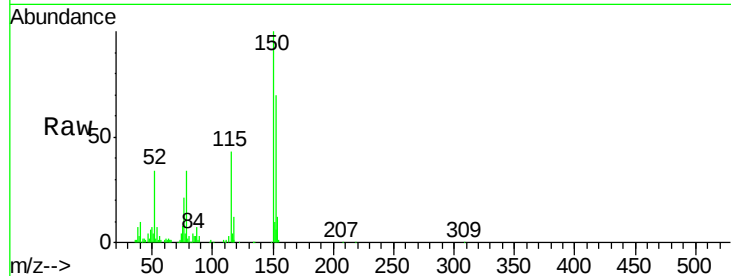

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

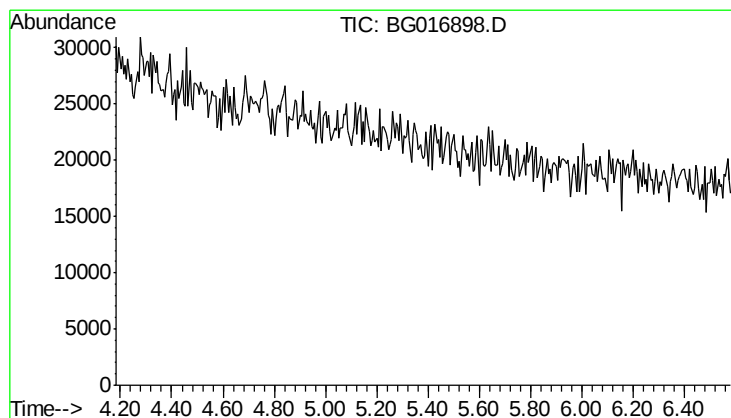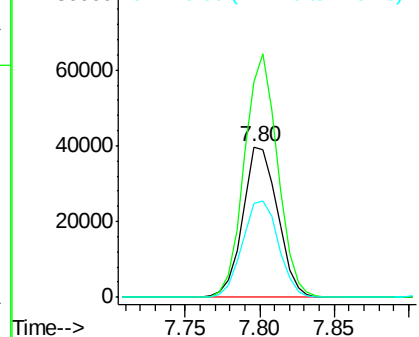



#5

2-Fluorophenol
Concen: 0.00 ng
Expected RT: 5.38 min

Lab File: BG016898.D
Acq: 6 May 2015 14:25

Tgt Ion: 112
Sig Exp Ratio
112 100
64 64.3
63 35.1

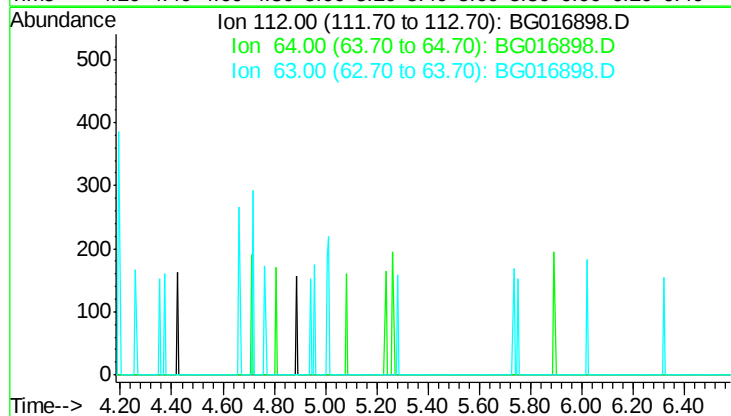

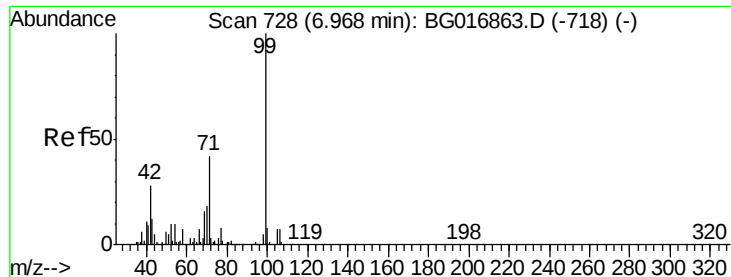

#7

Phenol-d6

Concen: 0.01 ng

RT: 6.87 min Scan# 711

Delta R.T. -0.10 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25

Instrument :

BNA_G

ClientSampleId :

SVOC-GPC-BLANK


Tgt Ion: 99 Resp: 61

Ion Ratio Lower Upper




99 100

42 0.0 22.1 33.1#

71 0.0 33.4 50.0#

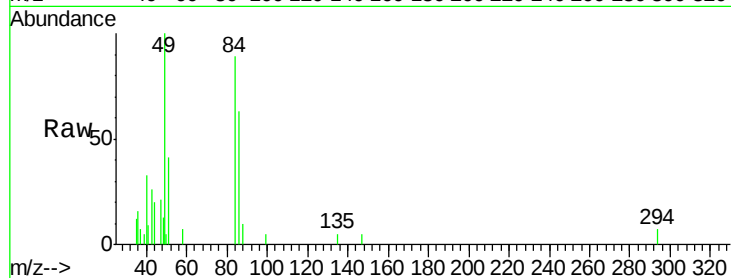

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

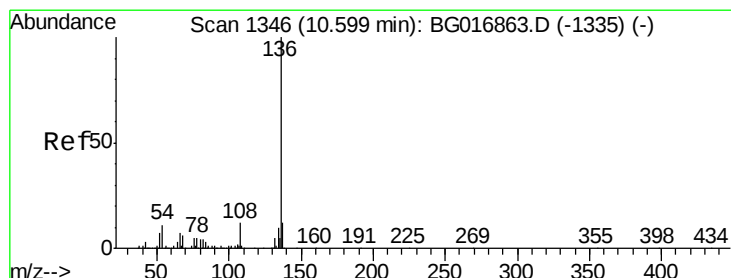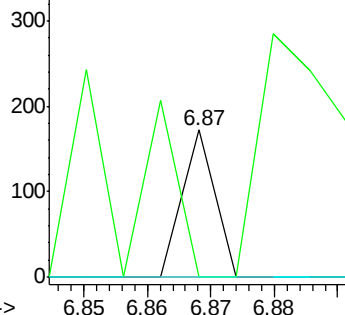

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.59 min Scan# 1345

Delta R.T. 0.00 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25

Tgt Ion: 136 Resp: 301216


Ion Ratio Lower Upper

136 100



137 11.4 9.8 14.8


54 11.1 8.7 13.1

68 6.2 5.0 7.4

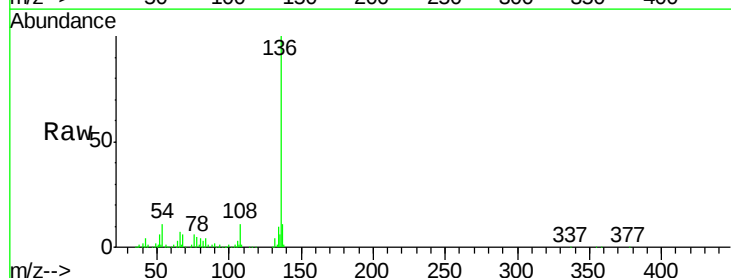

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



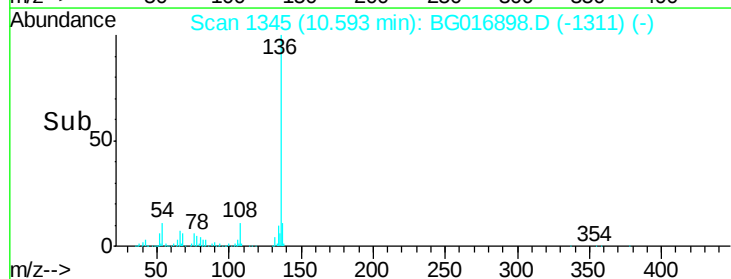
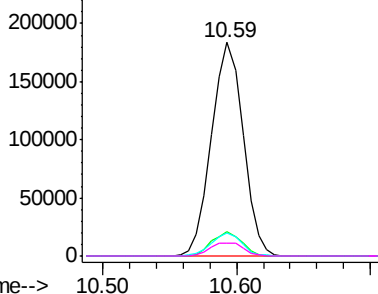




#23
Nitrobenzene-d5
Concen: 0.01 ng
RT: 8.95 min Scan# 1066
Delta R.T. -0.00 min
Lab File: BG016898.D
Acq: 6 May 2015 14:25




Instrument :
BNA_G
ClientSampleId :
SVOC-GPC-BLANK


Tgt Ion: 82 Resp: 68
Ion Ratio Lower Upper
82 100
128 0.0 33.2 49.8#
54 0.0 48.6 72.8#

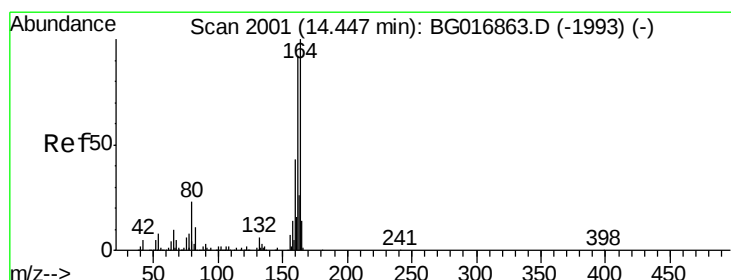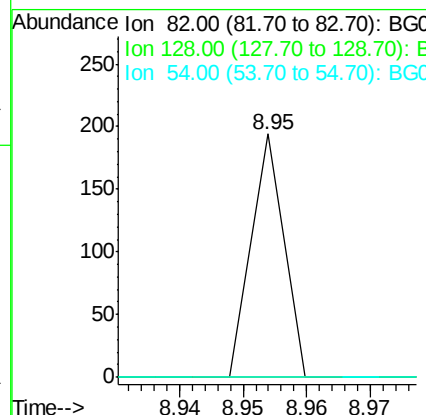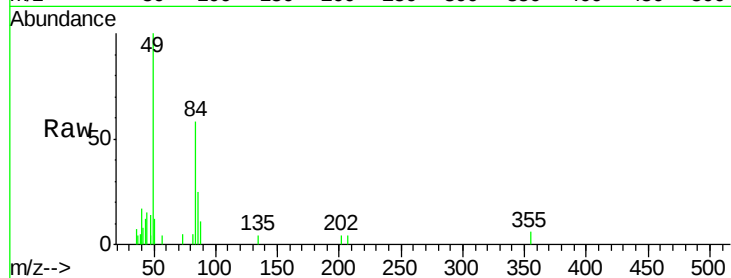

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.44 min Scan# 1999
Delta R.T. -0.00 min
Lab File: BG016898.D
Acq: 6 May 2015 14:25

Tgt Ion: 164 Resp: 203420
Ion Ratio Lower Upper
164 100
162 95.6 74.0 111.0
160 39.2 34.7 52.1

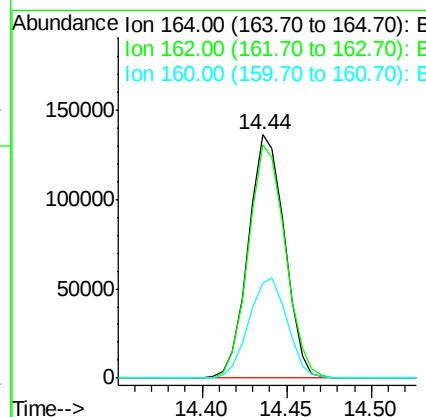
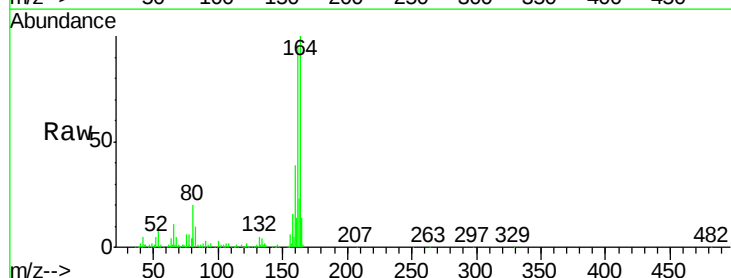


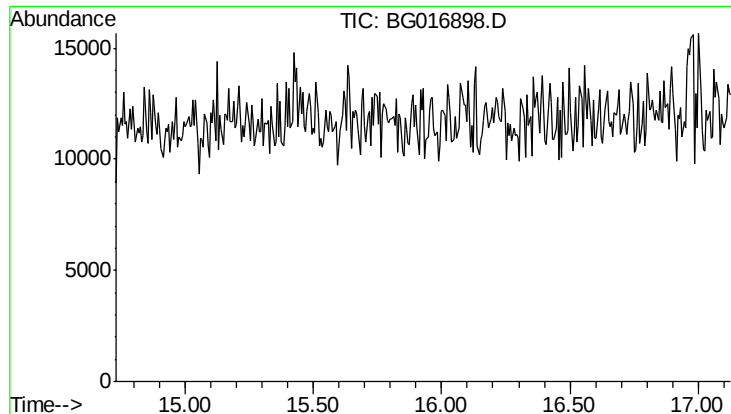

#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 15.93 min
 Lab File: BG016898.D
 Acq: 6 May 2015 14:25




Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC-BLANK


Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 0.0
 141 0.0

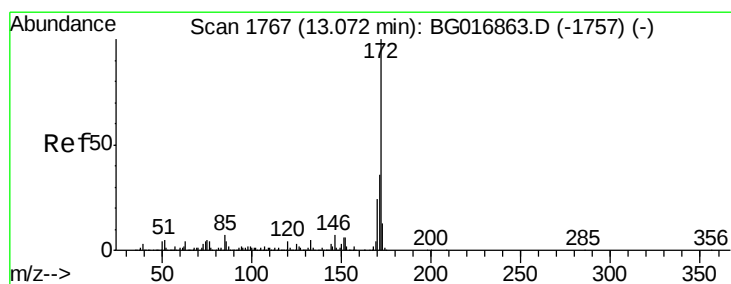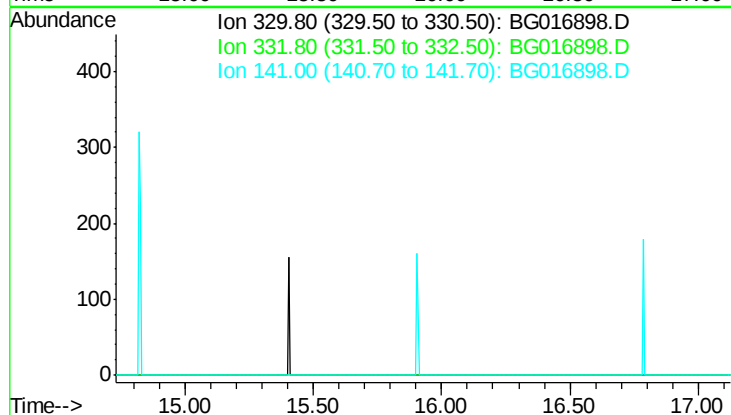

#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 RT: 13.03 min Scan# 1760
 Delta R.T. -0.03 min
 Lab File: BG016898.D
 Acq: 6 May 2015 14:25

Tgt Ion: 172 Resp: 59
 Ion Ratio Lower Upper
 172 100
 171 0.0 29.0 43.4#
 170 0.0 19.0 28.4#

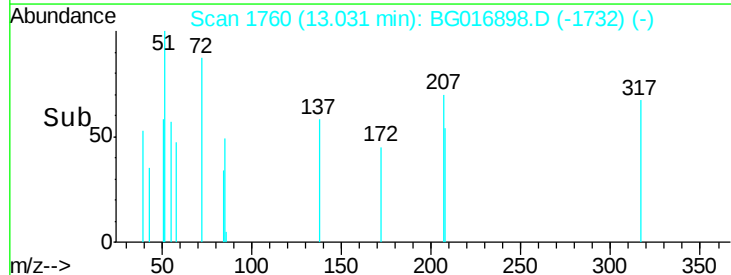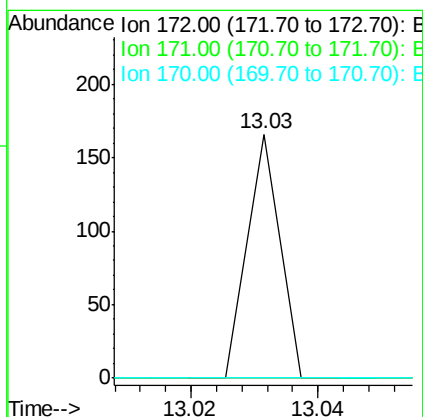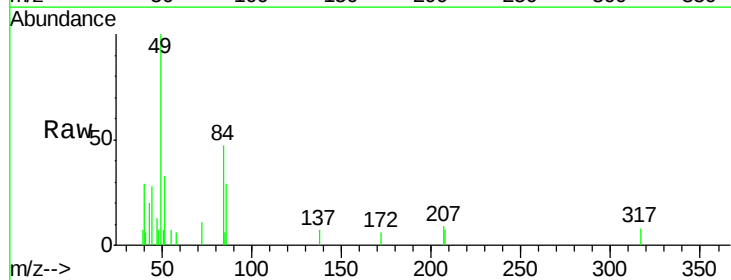

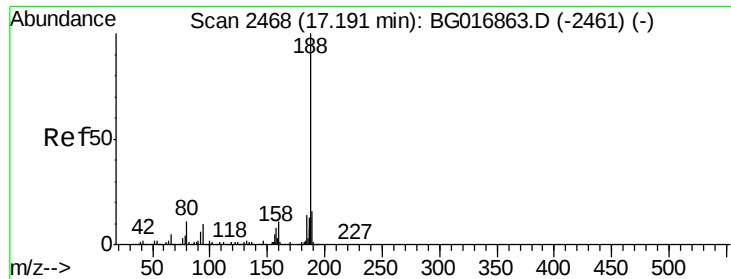

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.18 min Scan# 2466

Delta R.T. -0.00 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25

Instrument :

BNA_G

ClientSampleId :

SVOC-GPC-BLANK


Tgt Ion:188 Resp: 454747

Ion Ratio Lower Upper

188 100

94 10.4 8.2 12.4

80 11.1 8.8 13.2

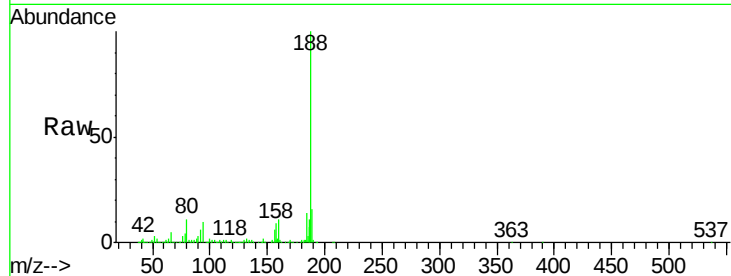



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): B

Ion 80.00 (79.70 to 80.70): B

17.18

Time-->

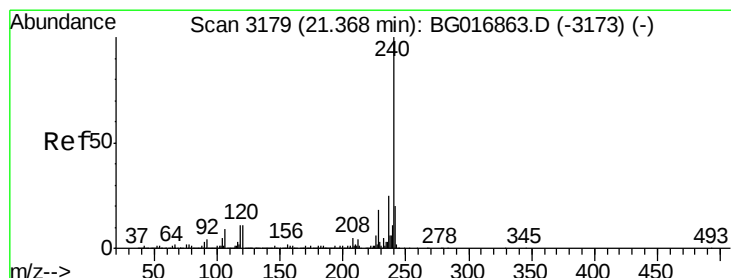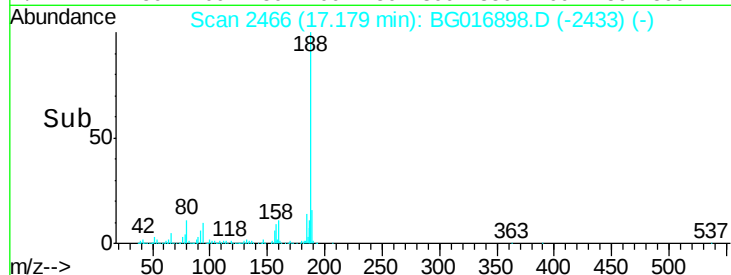

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.36 min Scan# 3177

Delta R.T. -0.00 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25


Tgt Ion:240 Resp: 448040

Ion Ratio Lower Upper

240 100

120 12.4 9.1 13.7

236 26.4 20.2 30.4

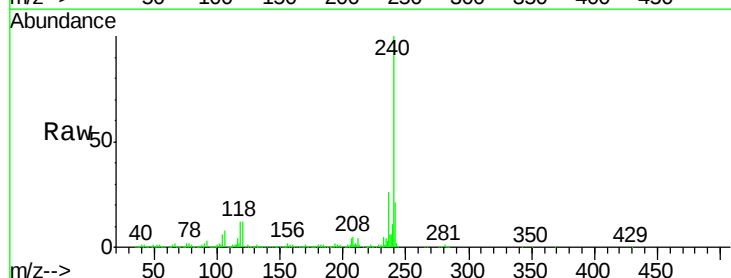


Abundance Ion 240.00 (239.70 to 240.70): E


Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

21.36

Time-->





#78

Terphenyl-d14

Concen: 0.00 ng

RT: 19.78 min Scan# 2908

Delta R.T. -0.03 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25

Instrument :

BNA_G

ClientSampleId :

SVOC-GPC-BLANK


Tgt Ion:244 Resp: 68

Ion Ratio Lower Upper

244 100

212 0.0 7.0 10.6#




122 0.0 10.4 15.6#

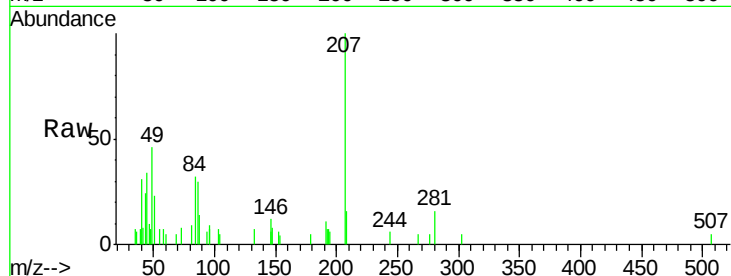

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

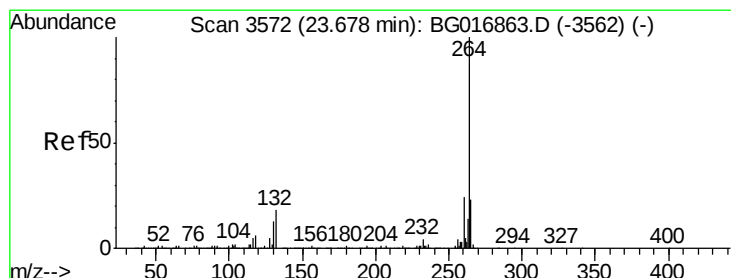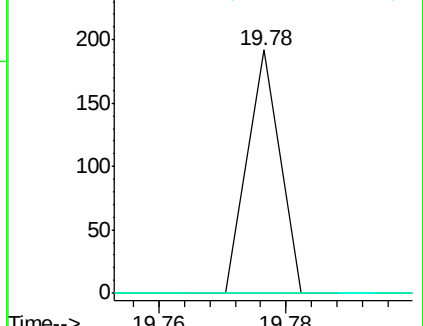

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.66 min Scan# 3569

Delta R.T. -0.00 min

Lab File: BG016898.D

Acq: 6 May 2015 14:25


Tgt Ion:264 Resp: 437507

Ion Ratio Lower Upper

264 100

260 23.5 19.5 29.3

265 22.6 18.5 27.7

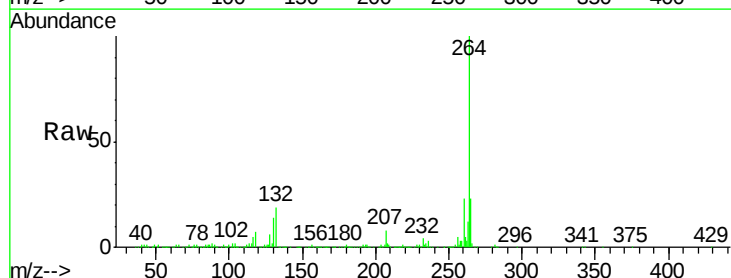

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

