

Data File : BG026883.D
Acq On : 6 May 2017 15:28
Operator : SJ/MA
Sample : I2884-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
YAB36

Quant Time: May 08 01:29:54 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon May 08 01:28:58 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.01	152	190815	20.00	ng/ul	0.00
18) Naphthalene-d8	10.81	136	920024	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.62	164	486544	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.35	188	897934	20.00	ng/ul	0.00
75) Chrysene-d12	21.60	240	819481	20.00	ng/ul	0.00
83) Perylene-d12	24.77	264	838227	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.43	96	16086	3.80	ng/uL	0.00
5) Phenol-d5	7.18	99	452123	26.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.33	67	258794	25.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.55	132	365059	25.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.72	113	353144	24.99	ng/ul	0.00
19) Nitrobenzene-d5	9.16	128	184908	24.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.89	143	196938	23.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	328276	24.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.94	131	331932	18.66	ng/ul	0.00
43) Dimethylphthalate-d6	14.02	166	831843	21.24	ng/ul	0.00
46) Acenaphthylene-d8	14.32	160	1291172	26.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	122832	17.40	ng/ul	0.00
57) Fluorene-d10	15.61	176	823194	24.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.73	200	59487	10.91	ng/ul	0.00
70) Anthracene-d10	17.45	188	1110942	25.49	ng/ul	0.00
76) Pyrene-d10	19.73	212	1113491	25.74	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.55	264	1065534	26.89	ng/ul	0.00

Target Compounds						Qvalue
6) Phenol	7.21	94	30405	1.76	ng/ul	87
44) Dimethylphthalate	14.07	163	311519	8.13	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG026883.D

Acq On : 6 May 2017 15:28

Operator : SJ/MA

Sample : I2884-03

Misc :

ALS Vial : 11 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

YAB36


Quant Time: May 08 01:29:54 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG042717.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon May 08 01:28:58 2017

Response via : Initial Calibration

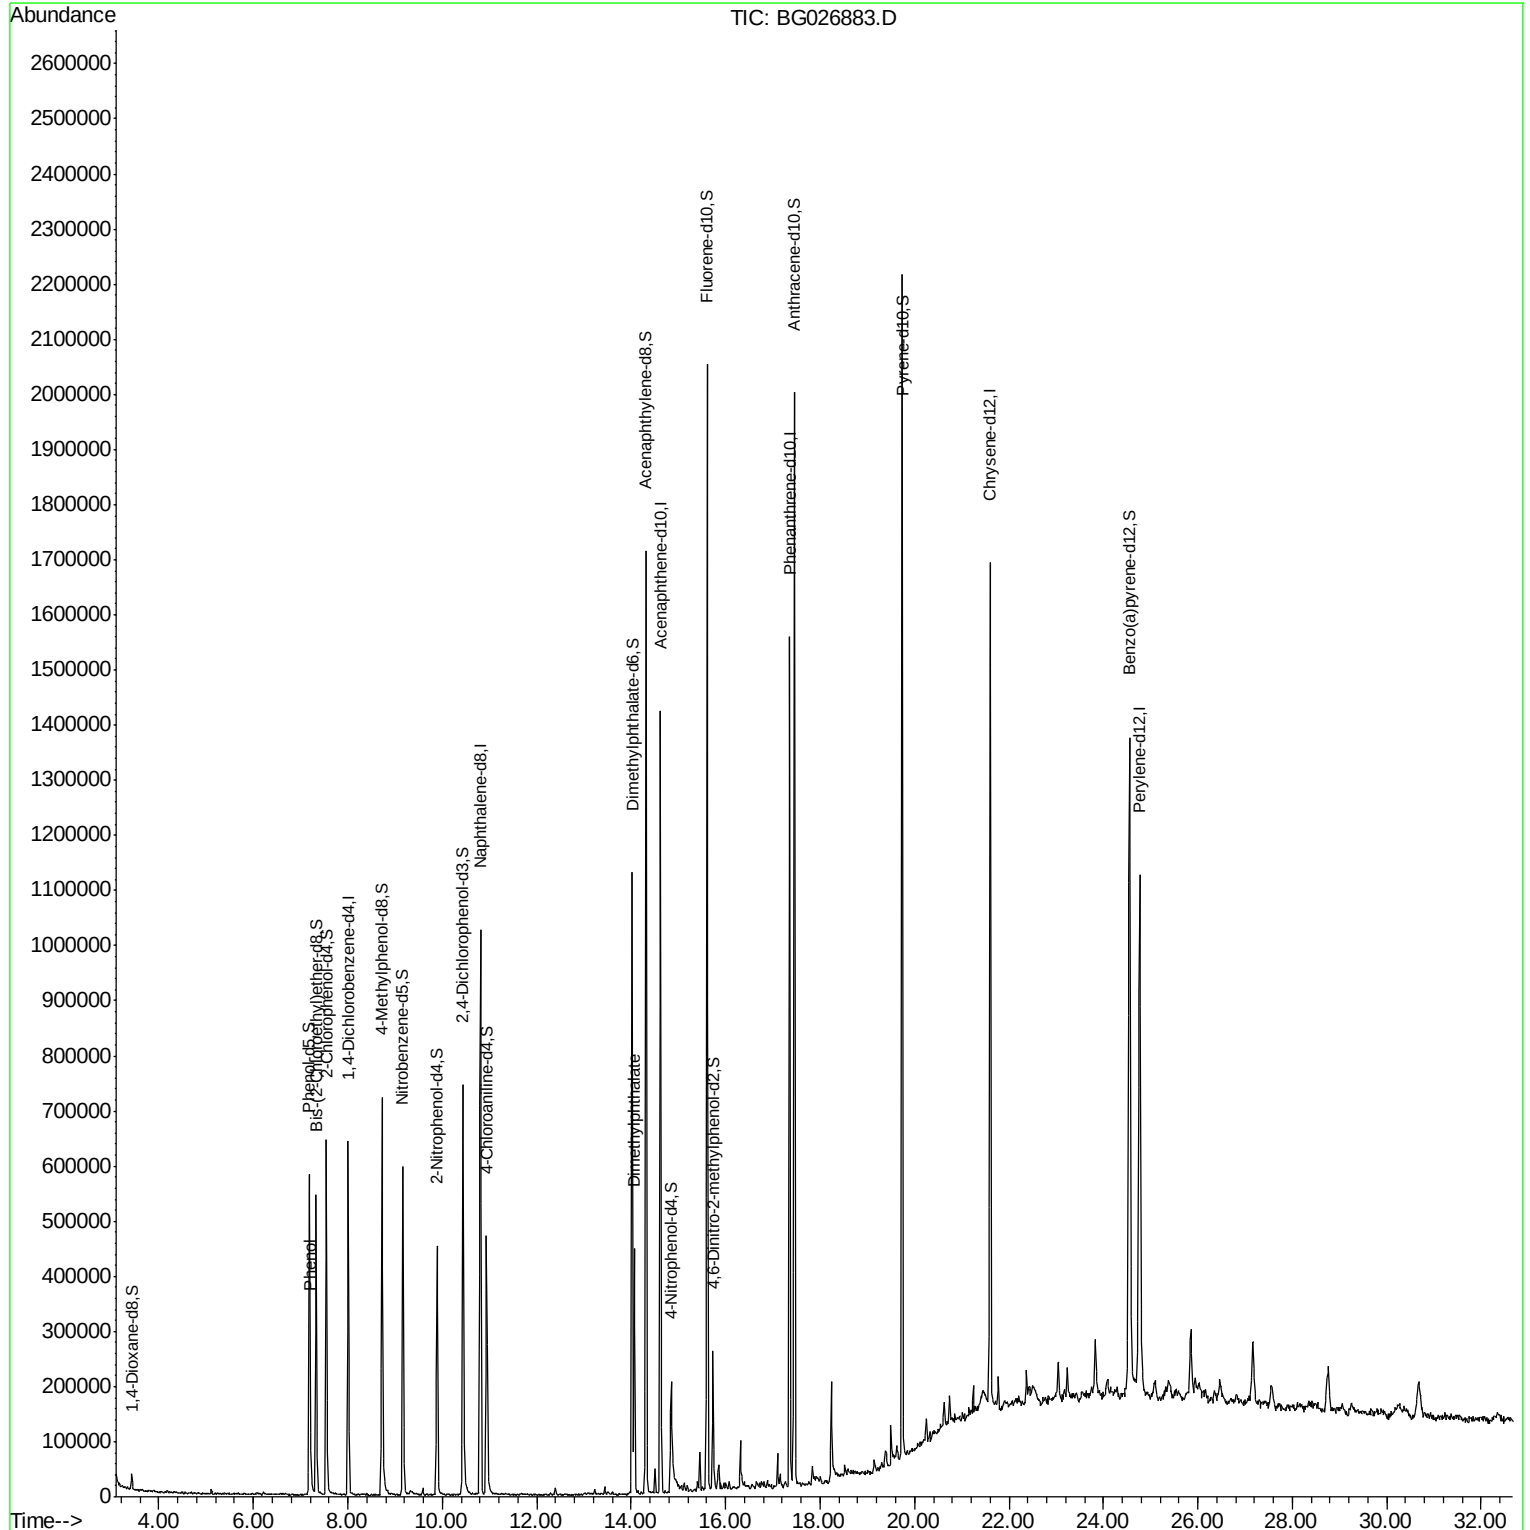

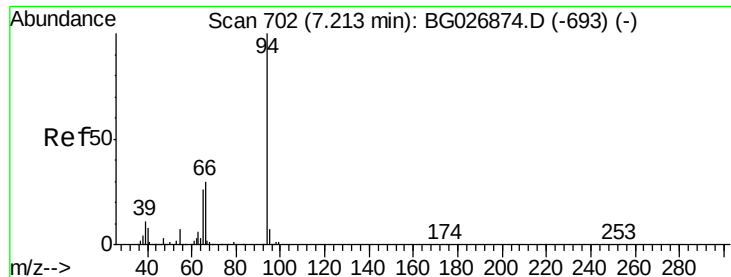

#6

Phenol

Concen: 1.76 ng/ul

RT: 7.21 min Scan# 701

Delta R.T. -0.01 min

Lab File: BG026883.D

Acq: 6 May 2017 15:28

Instrument :

BNA_G

ClientSampleId :

YAB36


Tgt Ion: 94 Resp: 30405

Ion Ratio Lower Upper




94 100

65 27.4 26.8 40.2

66 44.7 44.4 66.6

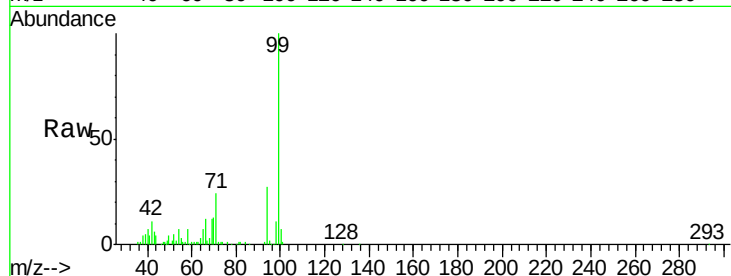

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

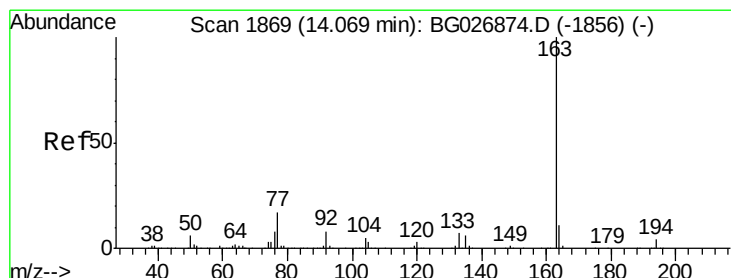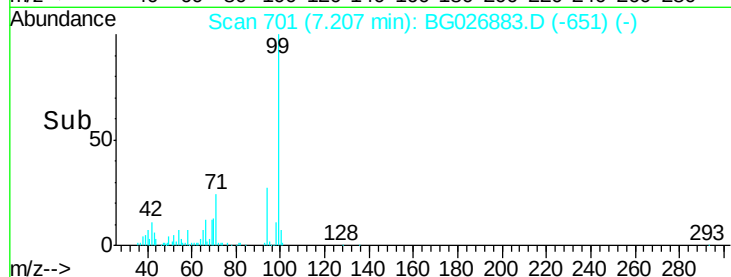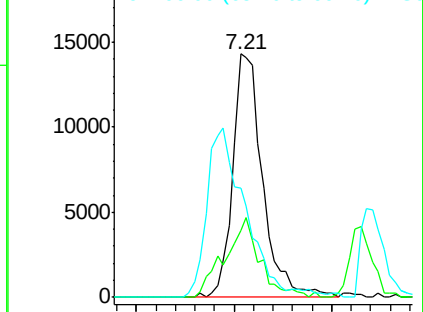

#44

Dimethylphthalate

Concen: 8.13 ng/ul

RT: 14.07 min Scan# 1869

Delta R.T. -0.00 min

Lab File: BG026883.D

Acq: 6 May 2017 15:28


Tgt Ion: 163 Resp: 311519

Ion Ratio Lower Upper

163 100

194 3.4 3.4 5.0

164 9.3 9.0 13.4

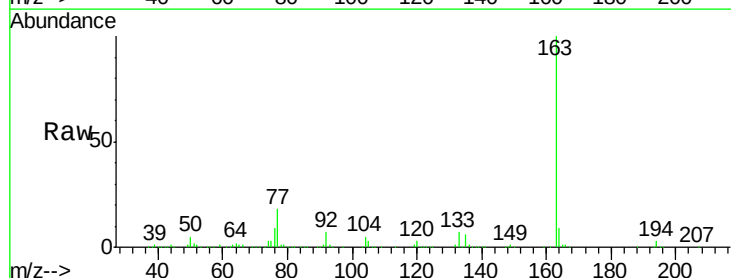

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

