


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050622\
 Data File : BG053468.D
 Acq On : 6 May 2022 9:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 05 02:13:53 2022

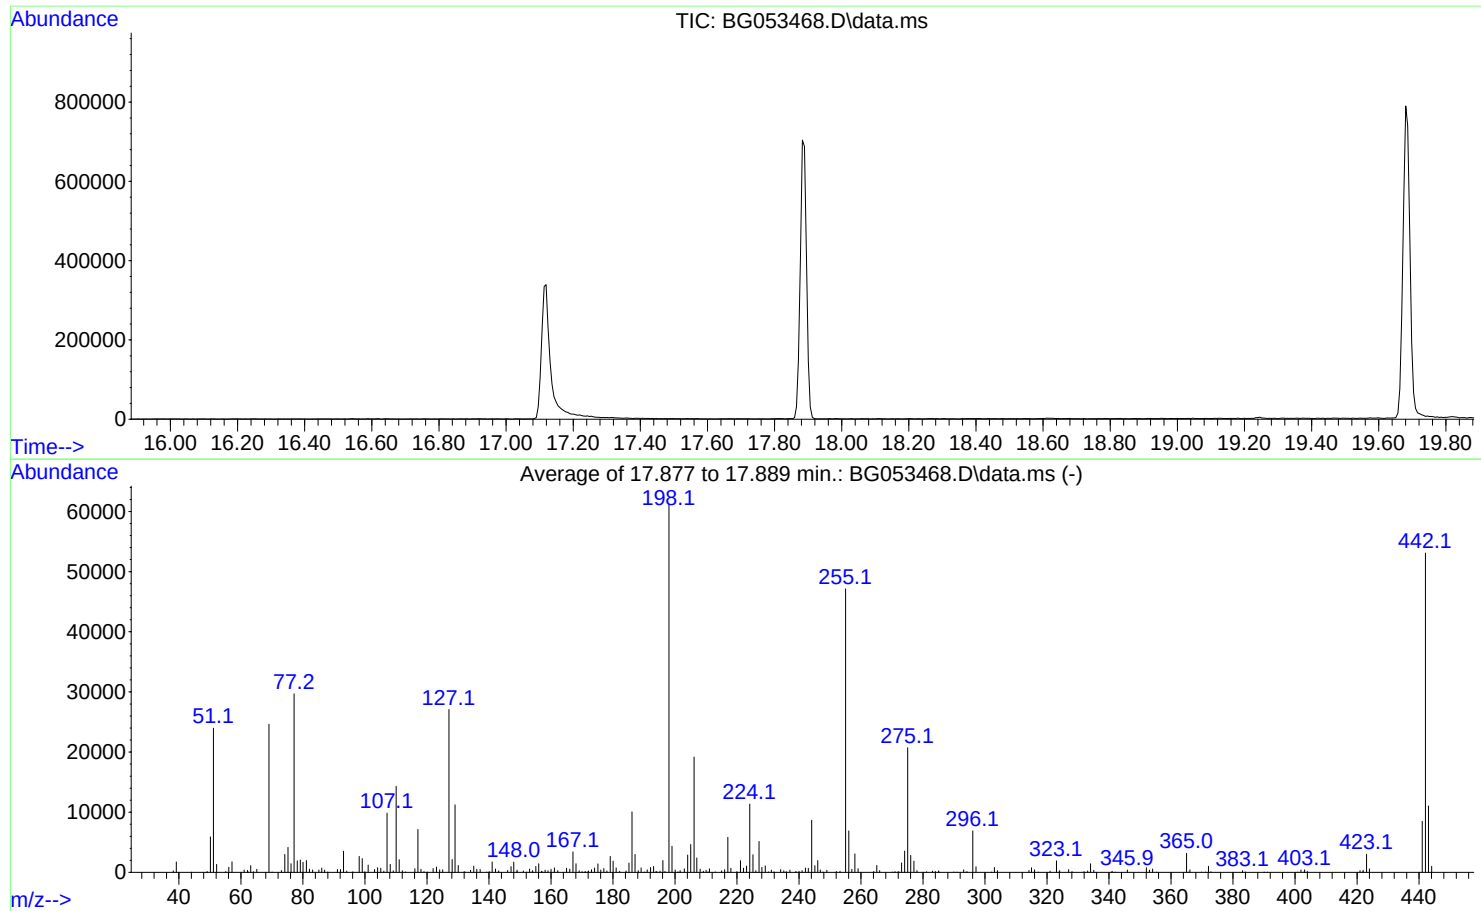




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	23981	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.3	24629	PASS
70	69	0.00	2	0.2	52	PASS
127	198	10	80	44.3	27072	PASS
197	198	0.00	2	0.3	166	PASS
198	198	100	100	100.0	61165	PASS
199	198	5	9	7.1	4336	PASS
275	198	10	60	33.9	20732	PASS
365	198	1	100	5.2	3171	PASS
441	198	0.01	100	13.9	8478	PASS
442	442	50	100	100.0	53109	PASS
443	442	15	24	20.8	11032	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050622\
Data File : BG053468.D
Acq On : 6 May 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 07 00:17:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

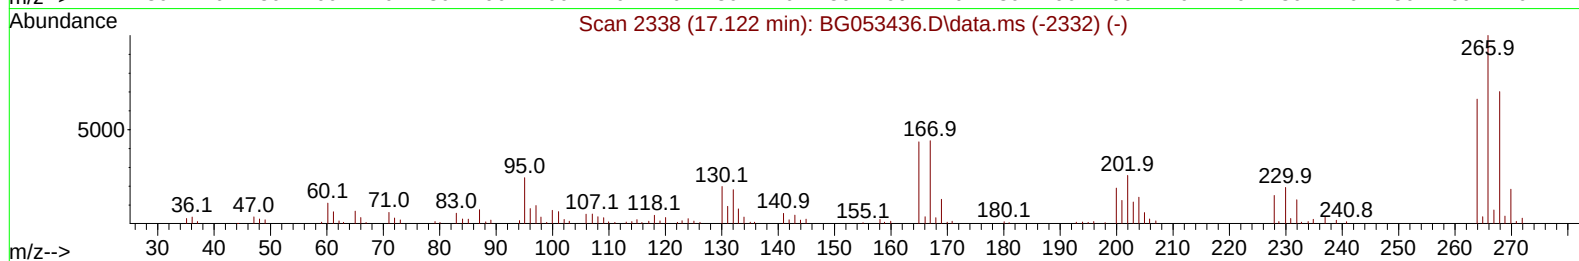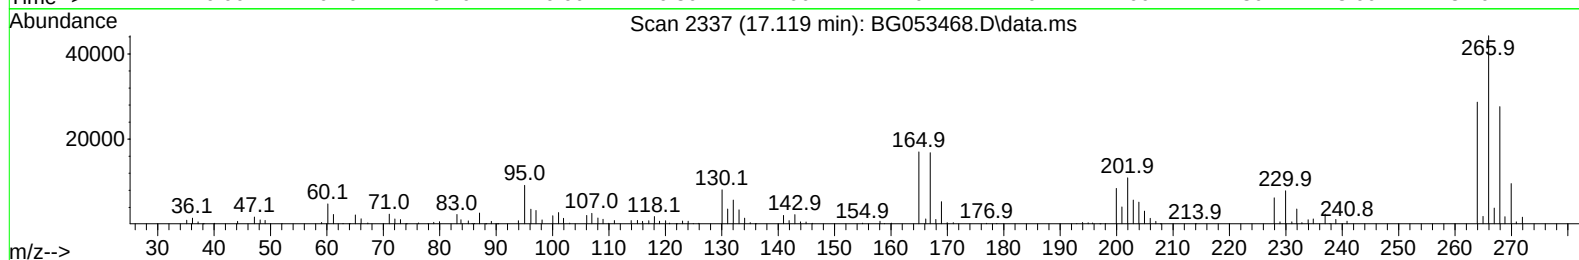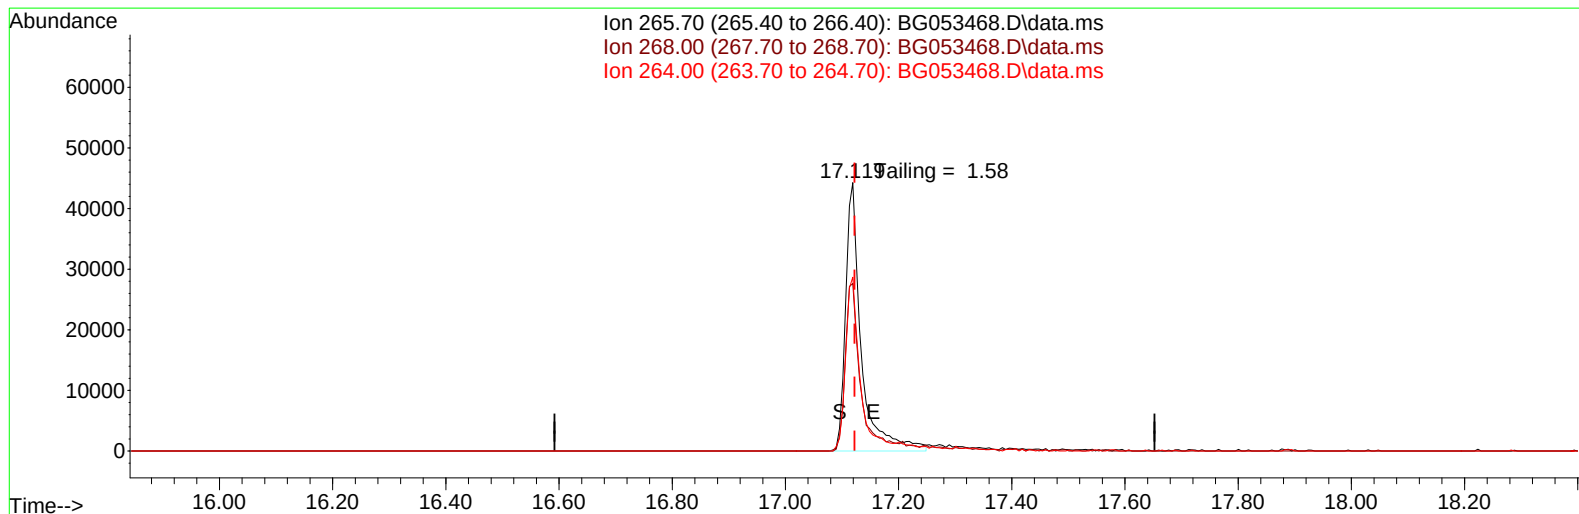

TIC: BG053468.D\data.ms

(70) Pentachlorophenol (C)

17.119min (-0.003) 187517.03 ng




response 82279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	62.43
264.00	66.20	64.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050622\
Data File : BG053468.D
Acq On : 6 May 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 07 00:17:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG050522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 05 02:13:53 2022
Response via : Initial Calibration

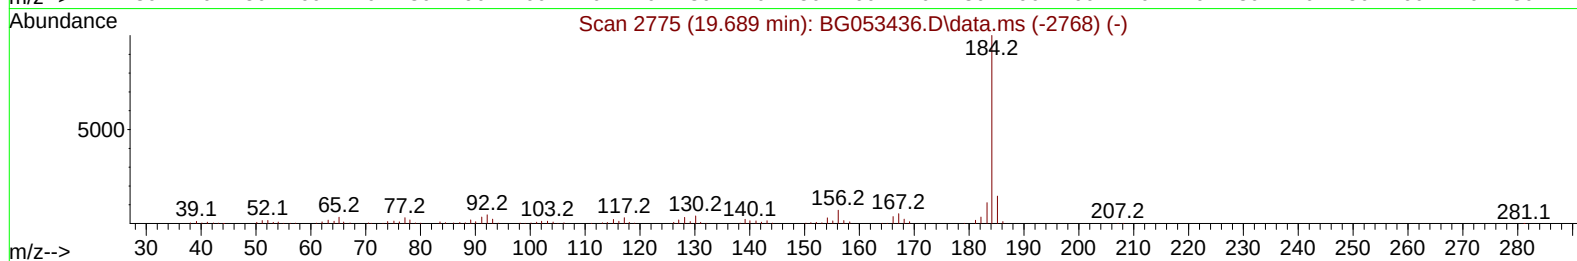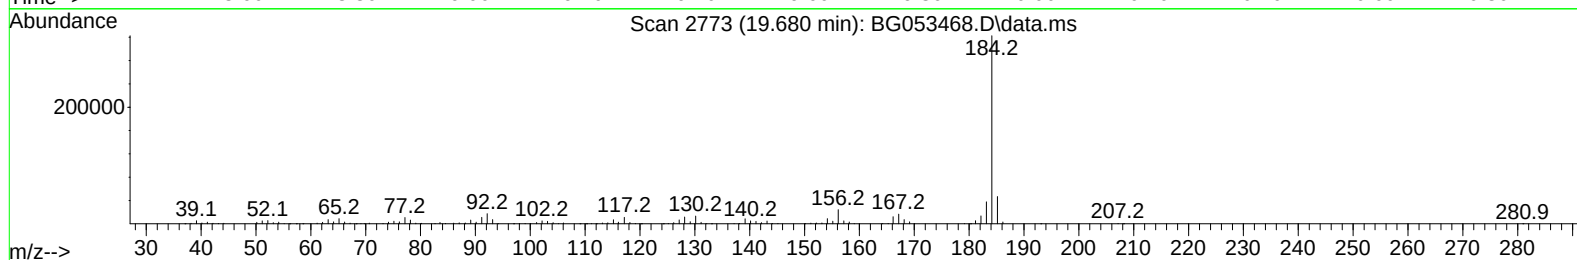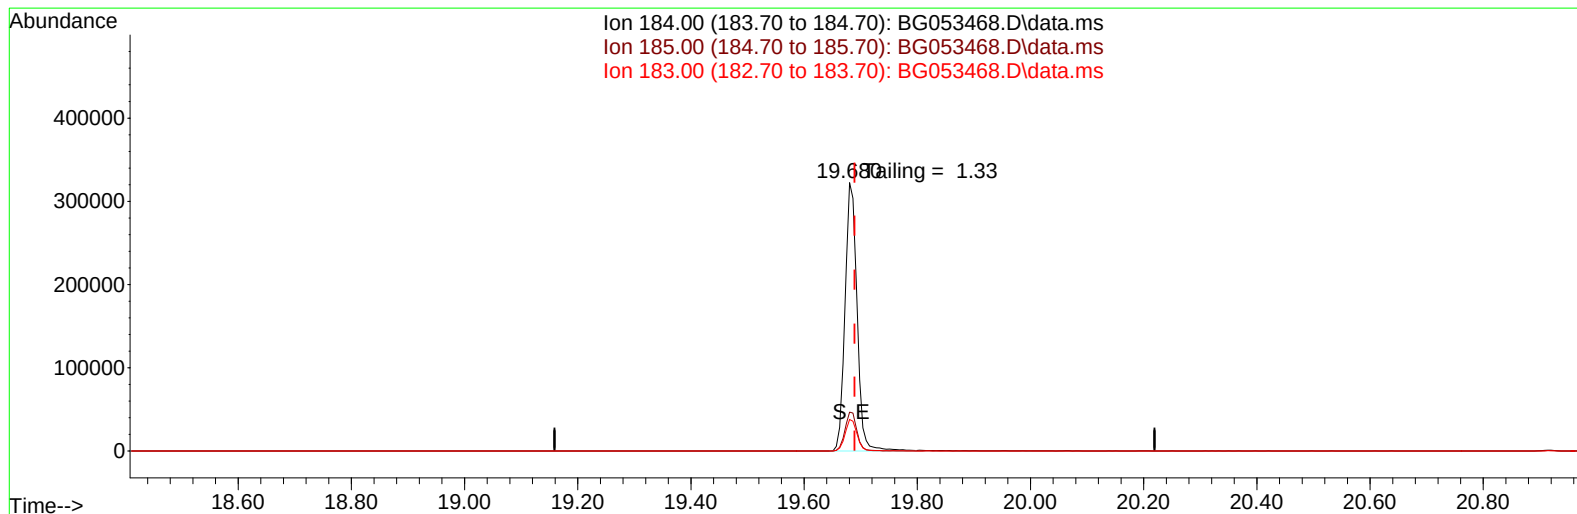

TIC: BG053468.D\data.ms

(77) Benzidine

19.680min (-0.008) 0.00 ng

response 477383

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.51
183.00	11.10	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2022	BNA_G	BG053468.D
Compound Name	Response	Retention Time
DDT	253088	20.914
DDD	3519	20.473
DDE	109	19.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3628	256716	1.41

Instrument :
BNA_G
ClientSampleId :
DFTPP