
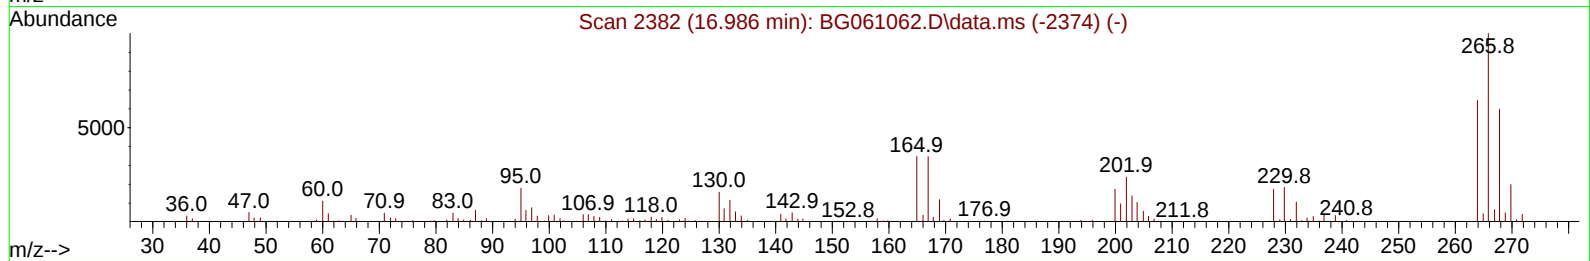
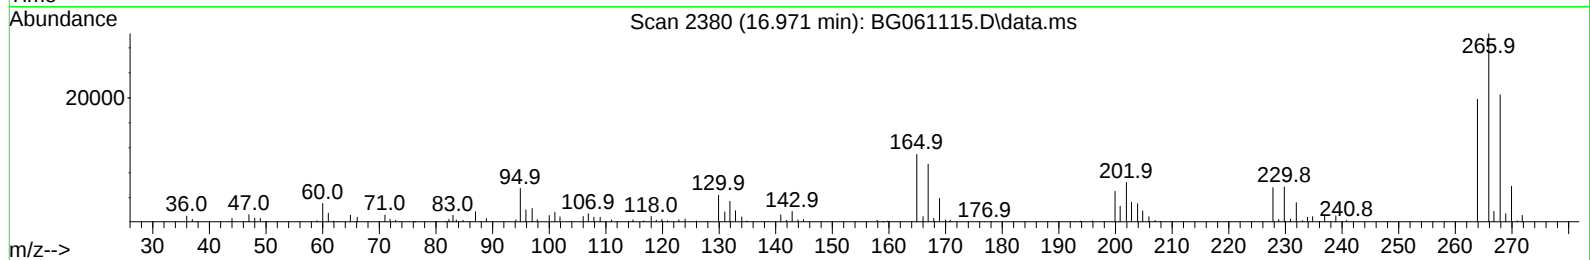


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061115.D
Acq On : 6 May 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:06:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

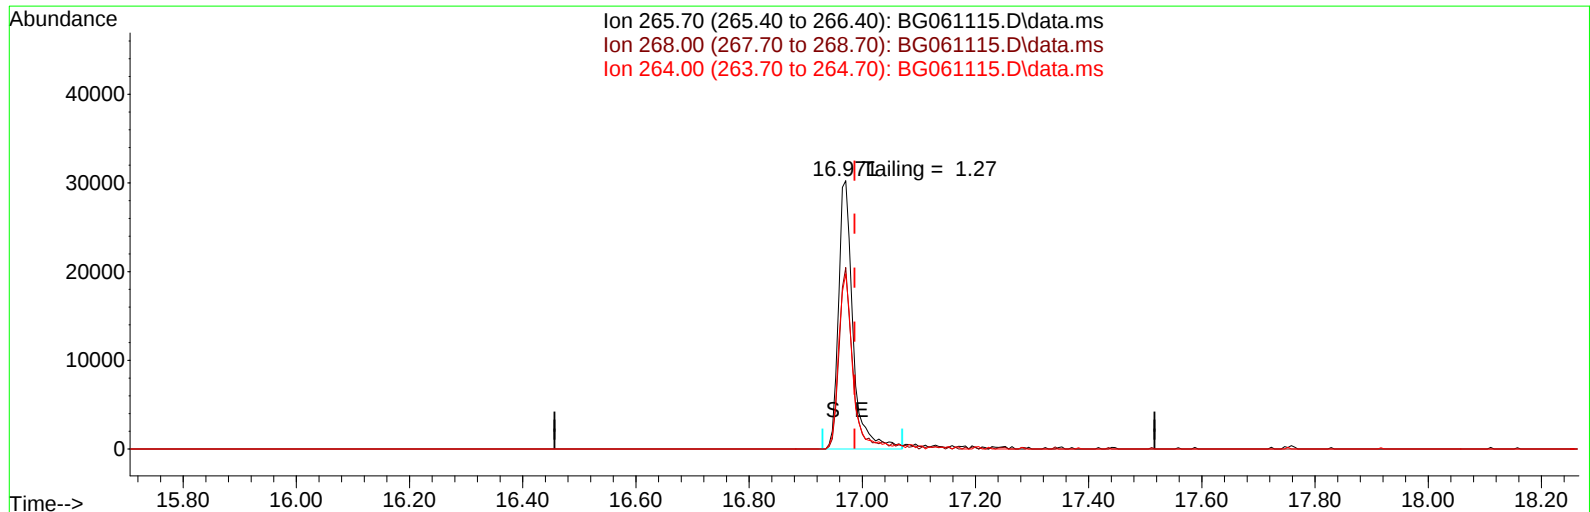

TIC: BG061115.D\data.ms

(70) Pentachlorophenol (C)




16.971min (-0.015) 10686.92 ng

response 53812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	67.62
264.00	64.40	65.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061115.D
Acq On : 6 May 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 06 11:06:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

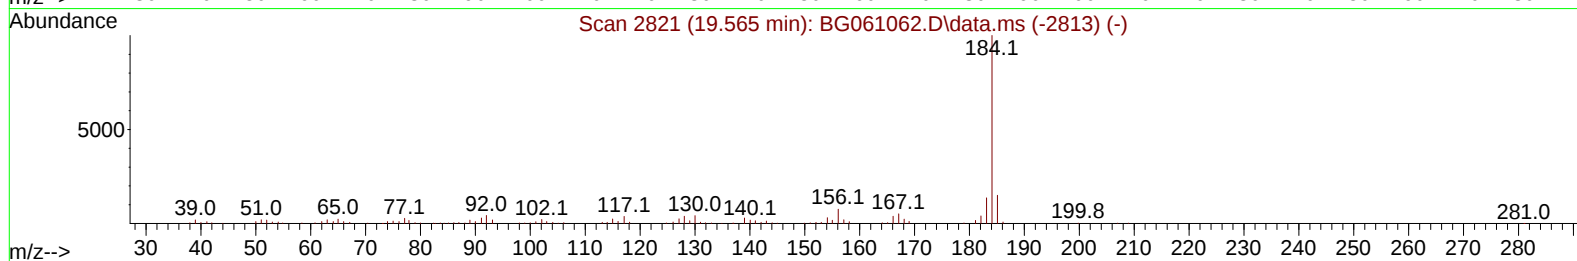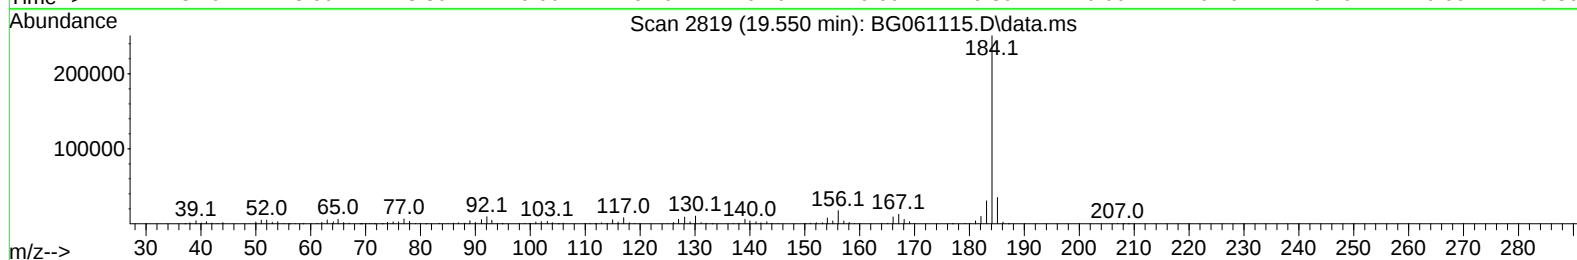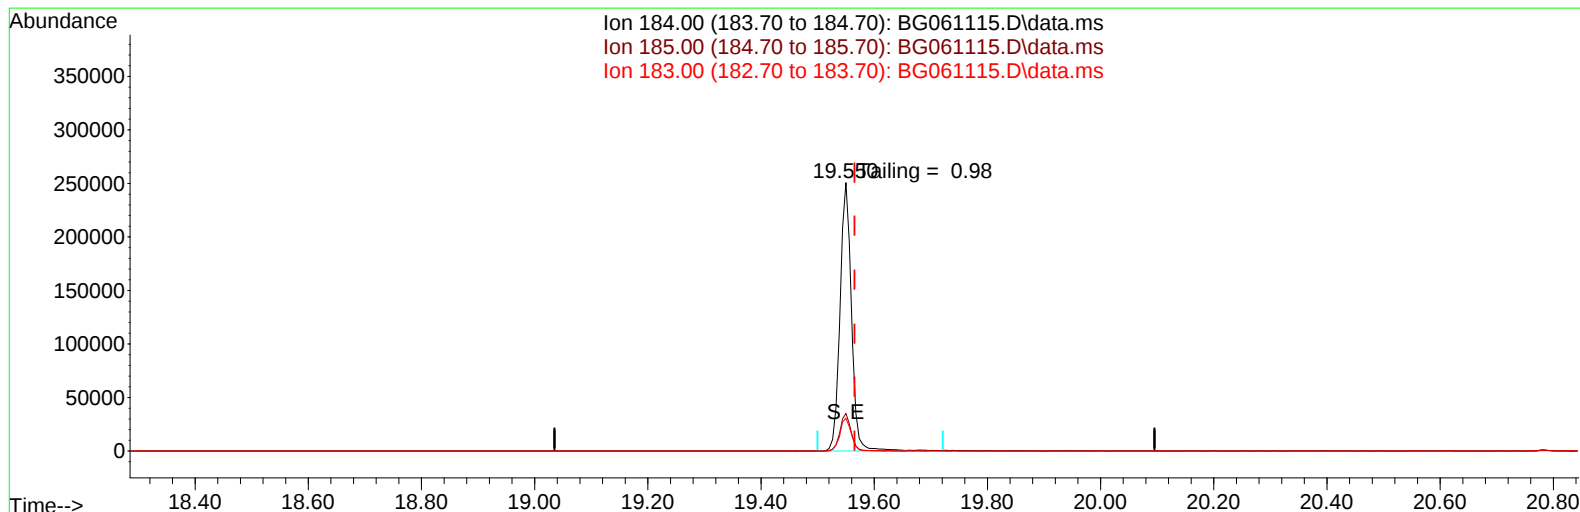

TIC: BG061115.D\data.ms

(77) Benzidine

19.550min (-0.015) 296822.38 ng m

response 353853

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.02
183.00	13.60	12.23
0.00	0.00	0.00