

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
 Data File : BG061117.D
 Acq On : 6 May 2024 12:16
 Operator : MA/JU
 Sample : PB160699BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB160699BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	425	432	440	rBV	388844	596924	22.72%	7.081%
2	7.114	694	702	711	rBV	391758	667594	25.42%	7.919%
3	7.936	835	842	849	rBV	69040	113370	4.32%	1.345%
4	9.094	1031	1039	1048	rBV	237356	422495	16.08%	5.012%
5	10.733	1310	1318	1326	rBV	86290	153498	5.84%	1.821%
6	13.189	1728	1736	1744	rBV	694748	1051596	40.03%	12.475%
7	14.564	1963	1970	1976	rBV	164322	249736	9.51%	2.963%
8	16.056	2217	2224	2241	rBV	703122	1110726	42.29%	13.176%
9	17.314	2431	2438	2447	rBV	258707	387441	14.75%	4.596%
10	19.934	2878	2884	2890	rBV	2094442	2626754	100.00%	31.160%
11	21.568	3156	3162	3170	rBV	315773	519614	19.78%	6.164%
12	24.699	3684	3695	3708	rVB2	182452	530036	20.18%	6.288%




Sum of corrected areas: 8429784

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061117.D
Acq On : 6 May 2024 12:16
Operator : MA/JU
Sample : PB160699BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160699BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

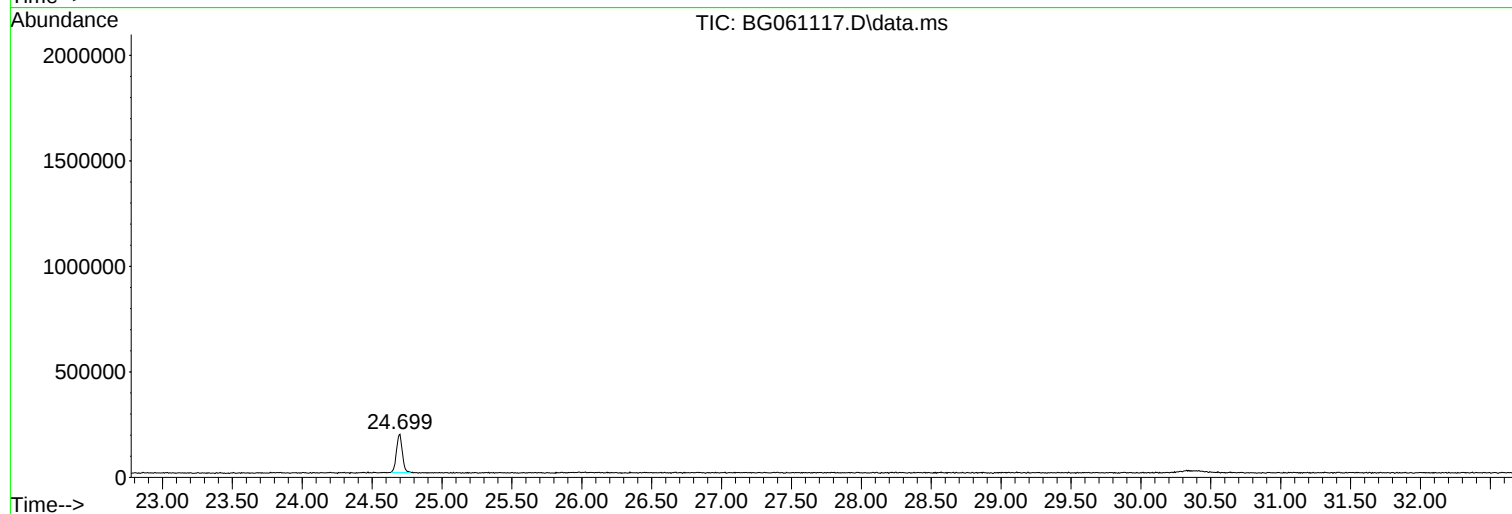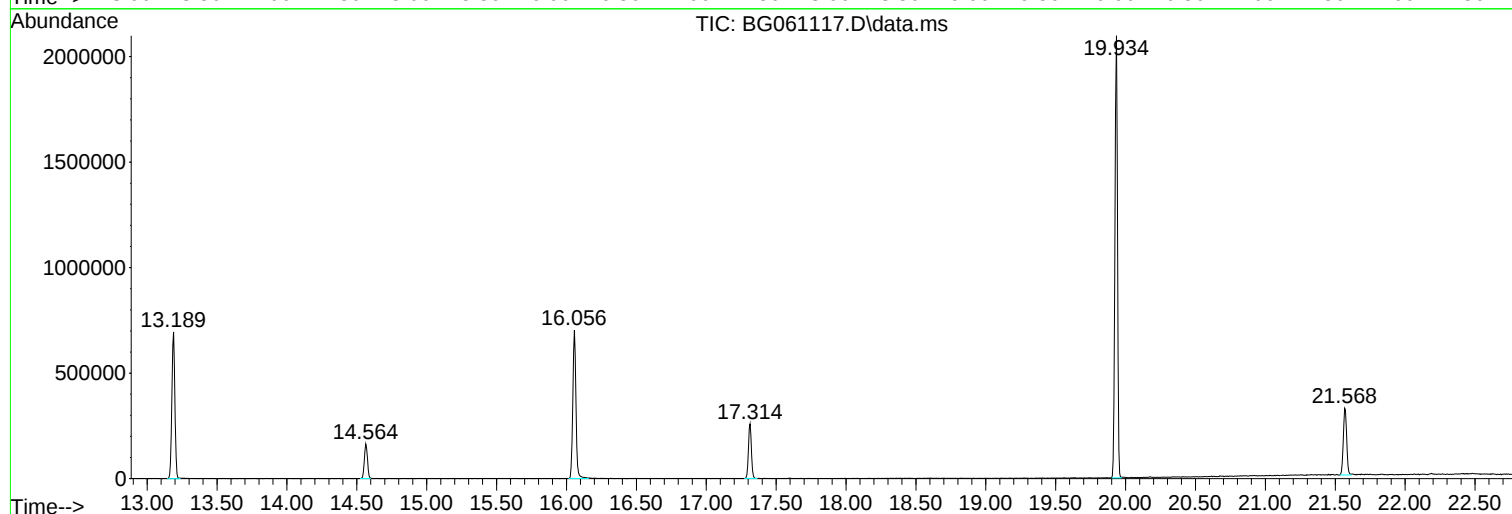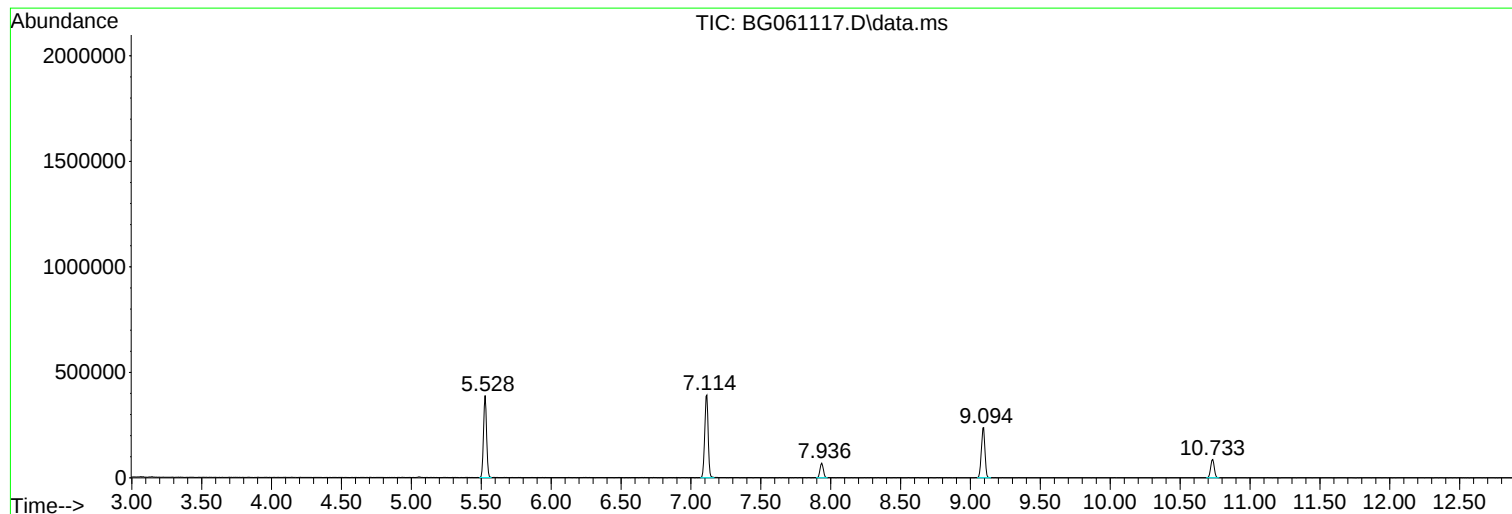

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061117.D
Acq On : 6 May 2024 12:16
Operator : MA/JU
Sample : PB160699BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160699BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061117.D
Acq On : 6 May 2024 12:16
Operator : MA/JU
Sample : PB160699BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB160699BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------