
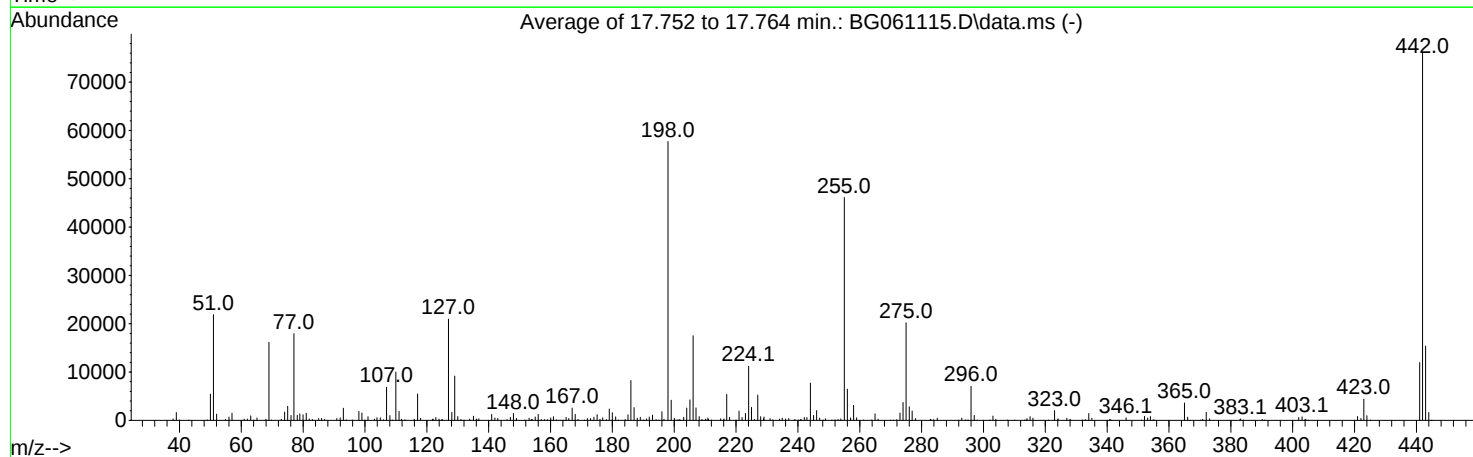


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061115.D
Acq On : 6 May 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 05:11:25 2024

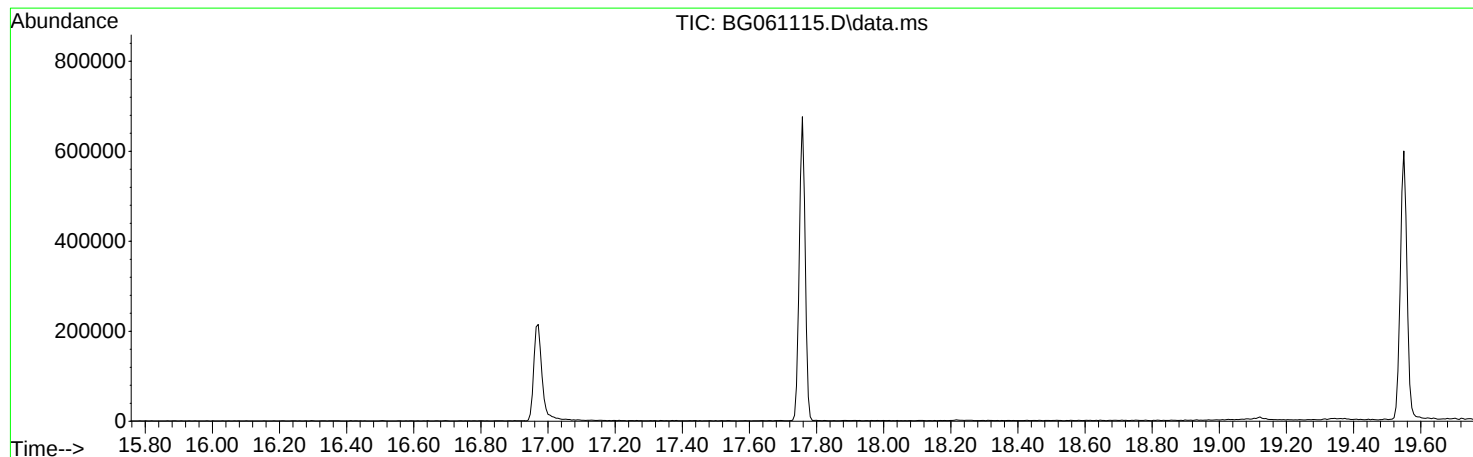




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	21877	PASS
68	69	0.00	2	1.4	228	PASS
69	198	0.00	100	28.0	16161	PASS
70	69	0.00	2	0.5	80	PASS
127	198	10	80	36.4	20981	PASS
197	198	0.00	2	0.4	229	PASS
198	198	100	100	100.0	57717	PASS
199	198	5	9	7.2	4171	PASS
275	198	10	60	35.0	20208	PASS
365	198	1	100	6.3	3626	PASS
441	198	0.01	100	20.7	11966	PASS
442	442	50	100	100.0	76139	PASS
443	442	15	24	20.2	15375	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061115.D
Acq On : 6 May 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 11:06:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

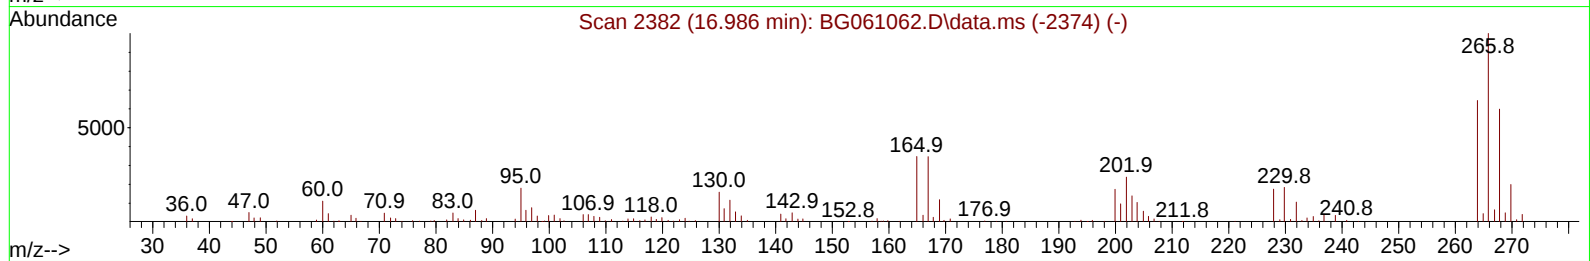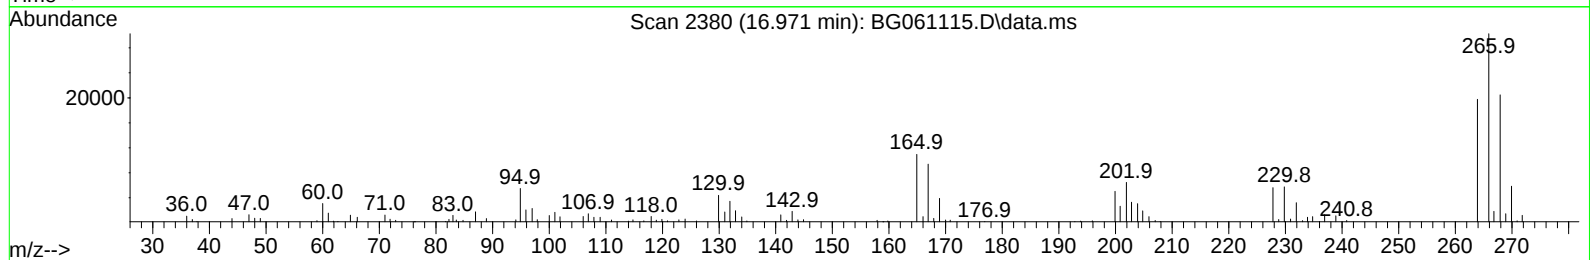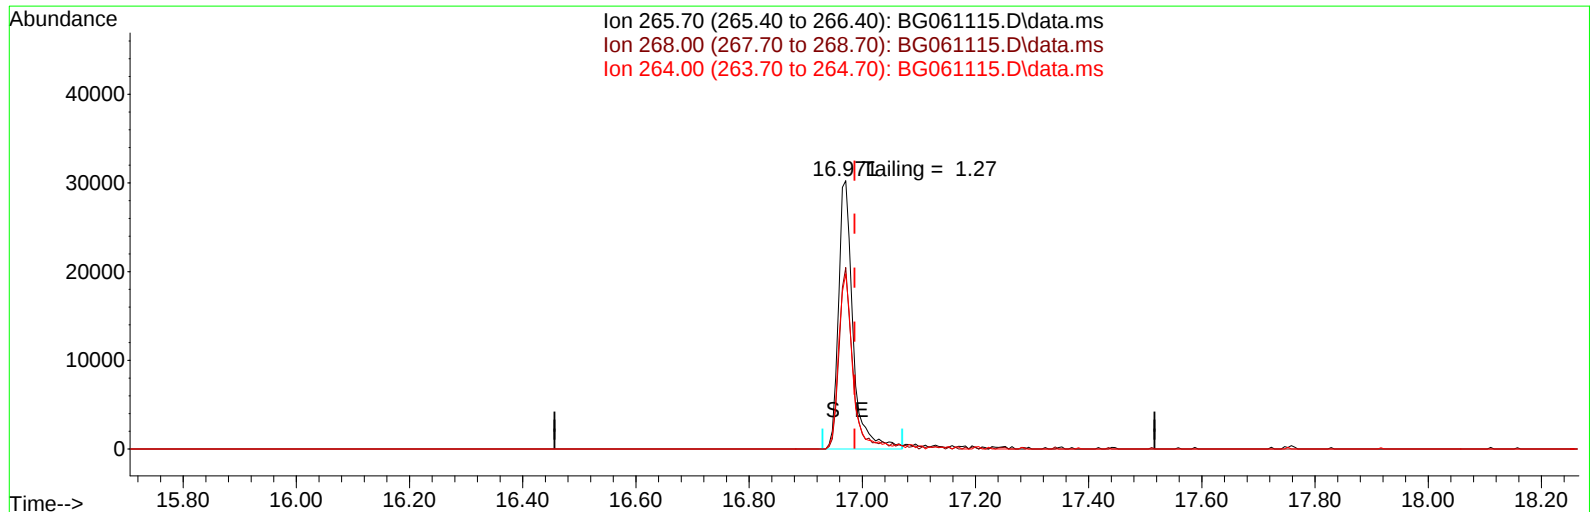

TIC: BG061115.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.015) 10686.92 ng




response 53812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	67.62
264.00	64.40	65.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050624\
Data File : BG061115.D
Acq On : 6 May 2024 10:01
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: May 06 11:06:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

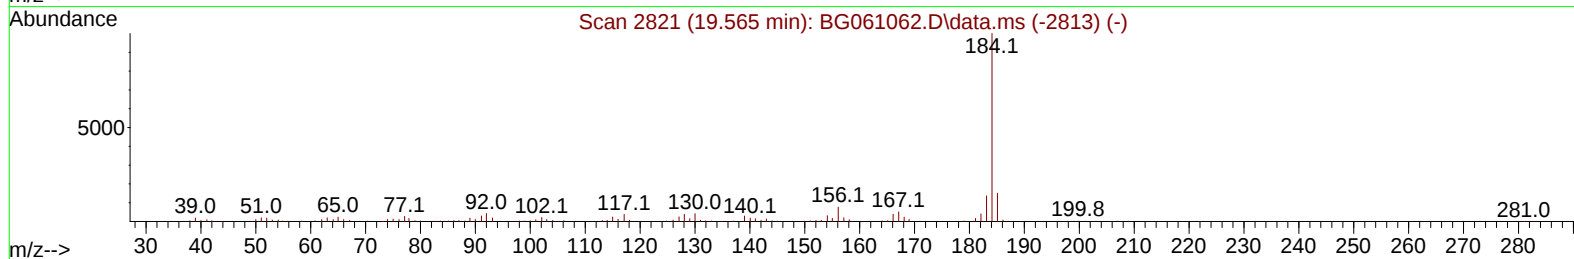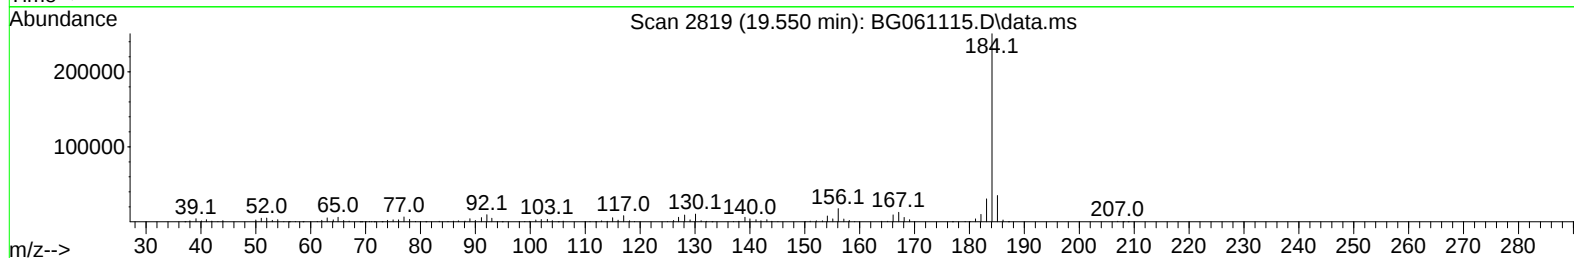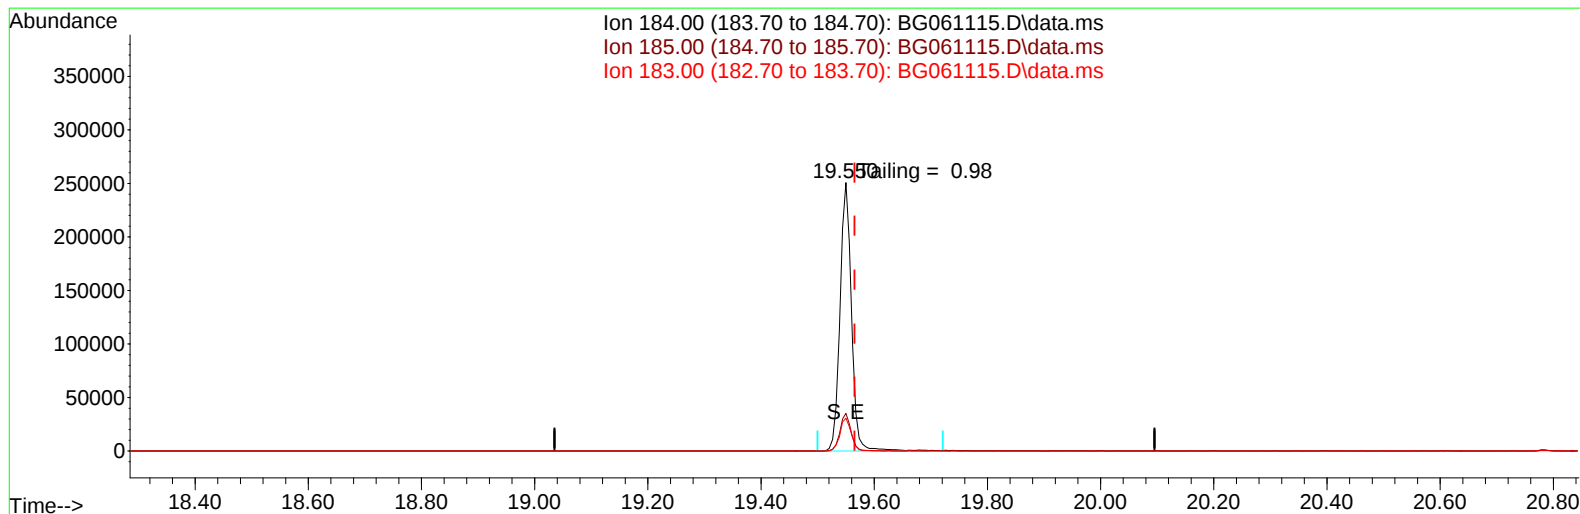

TIC: BG061115.D\data.ms

(77) Benzidine

19.550min (-0.015) 296822.38 ng m

response 353853

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.02
183.00	13.60	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/6/2024	BNA_G	<u>BG061115.D</u>
Compound Name	Response	Retention Time
DDT	215427	20.784
DDD	6811	20.349
DDE	342	19.838
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7153	222580	3.21

Instrument :
BNA_G
ClientSampleId :
DFTPP