

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050715\
 Data File : BG016934.D
 Acq On : 7 May 2015 23:33
 Operator : TP/IZ
 Sample : G2038-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01

Quant Time: May 08 04:18:36 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 08 04:04:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	82728	20.00	ng	0.00
21) Naphthalene-d8	10.66	136	384601	20.00	ng	0.07
38) Acenaphthene-d10	14.44	164	219105	20.00	ng	0.00
63) Phenanthrene-d10	17.18	188	436016	20.00	ng	0.00
75) Chrysene-d12	21.36	240	440140	20.00	ng	0.00
86) Perylene-d12	23.66	264	420421	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	335573	70.63	ng	0.01
7) Phenol-d6	6.97	99	333283	49.10	ng	0.00
23) Nitrobenzene-d5	8.96	82	722248	91.74	ng	0.00
41) 2,4,6-Tribromophenol	15.93	330	352953	160.46	ng	0.00
44) 2-Fluorobiphenyl	13.06	172	1385127	95.40	ng	0.00
78) Terphenyl-d14	19.81	244	1695866	90.32	ng	0.00


Target Compounds				Qvalue		
9) Benzaldehyde	6.95	77	360170	Below Cal	#	1
10) Phenol	6.99	94	67596	9.29	ng	97
17) 2-Methylphenol	8.24	107	21497	4.19	ng	85
18) Hexachloroethane	8.91	117	79854	31.60	ng	1
20) 3+4-Methylphenols	8.56	107	48994	6.94	ng	91
22) Acetophenone	8.62	105	295231	32.23	ng	97
27) 2,4-Dimethylphenol	9.79	122	159802	27.28	ng	96
31) Naphthalene	10.76	128	21227578	1109.69	ng	1
32) Benzoic acid	10.07	122	139246	41.34	ng	30
33) 4-Chloroaniline	10.76	127	11284578	1277.33	ng	23
36) 4-Chloro-3-methylphenol	11.94	107	125956	17.77	ng	21
37) 2-Methylnaphthalene	12.27	142	3040485	208.68	ng	91
45) 1,1'-Biphenyl	13.27	154	637873	40.66	ng	97
48) Acenaphthylene	14.16	152	402733	18.61	ng	97
51) Acenaphthene	14.50	154	1191056	92.49	ng	97
54) Dibenzofuran	14.84	168	854948	46.75	ng	97
55) 4-Nitrophenol	14.50	139	12205	3.72	ng	53
57) Fluorene	15.49	166	707385	43.69	ng	99
61) 4-Nitroaniline	15.49	138	11123	2.48	ng	21
70) Phenanthrene	17.23	178	1094460	48.78	ng	99
71) Anthracene	17.31	178	147467	6.51	ng	96
72) Carbazole	17.59	167	2140304	99.46	ng	92
74) Fluoranthene	19.24	202	147512	5.67	ng	96
77) Pyrene	19.60	202	95189	3.66	ng	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050715\
Data File : BG016934.D
Acq On : 7 May 2015 23:33
Operator : TP/IZ
Sample : G2038-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBMW-01

Quant Time: May 08 04:18:36 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 08 04:04:43 2015
Response via : Initial Calibration

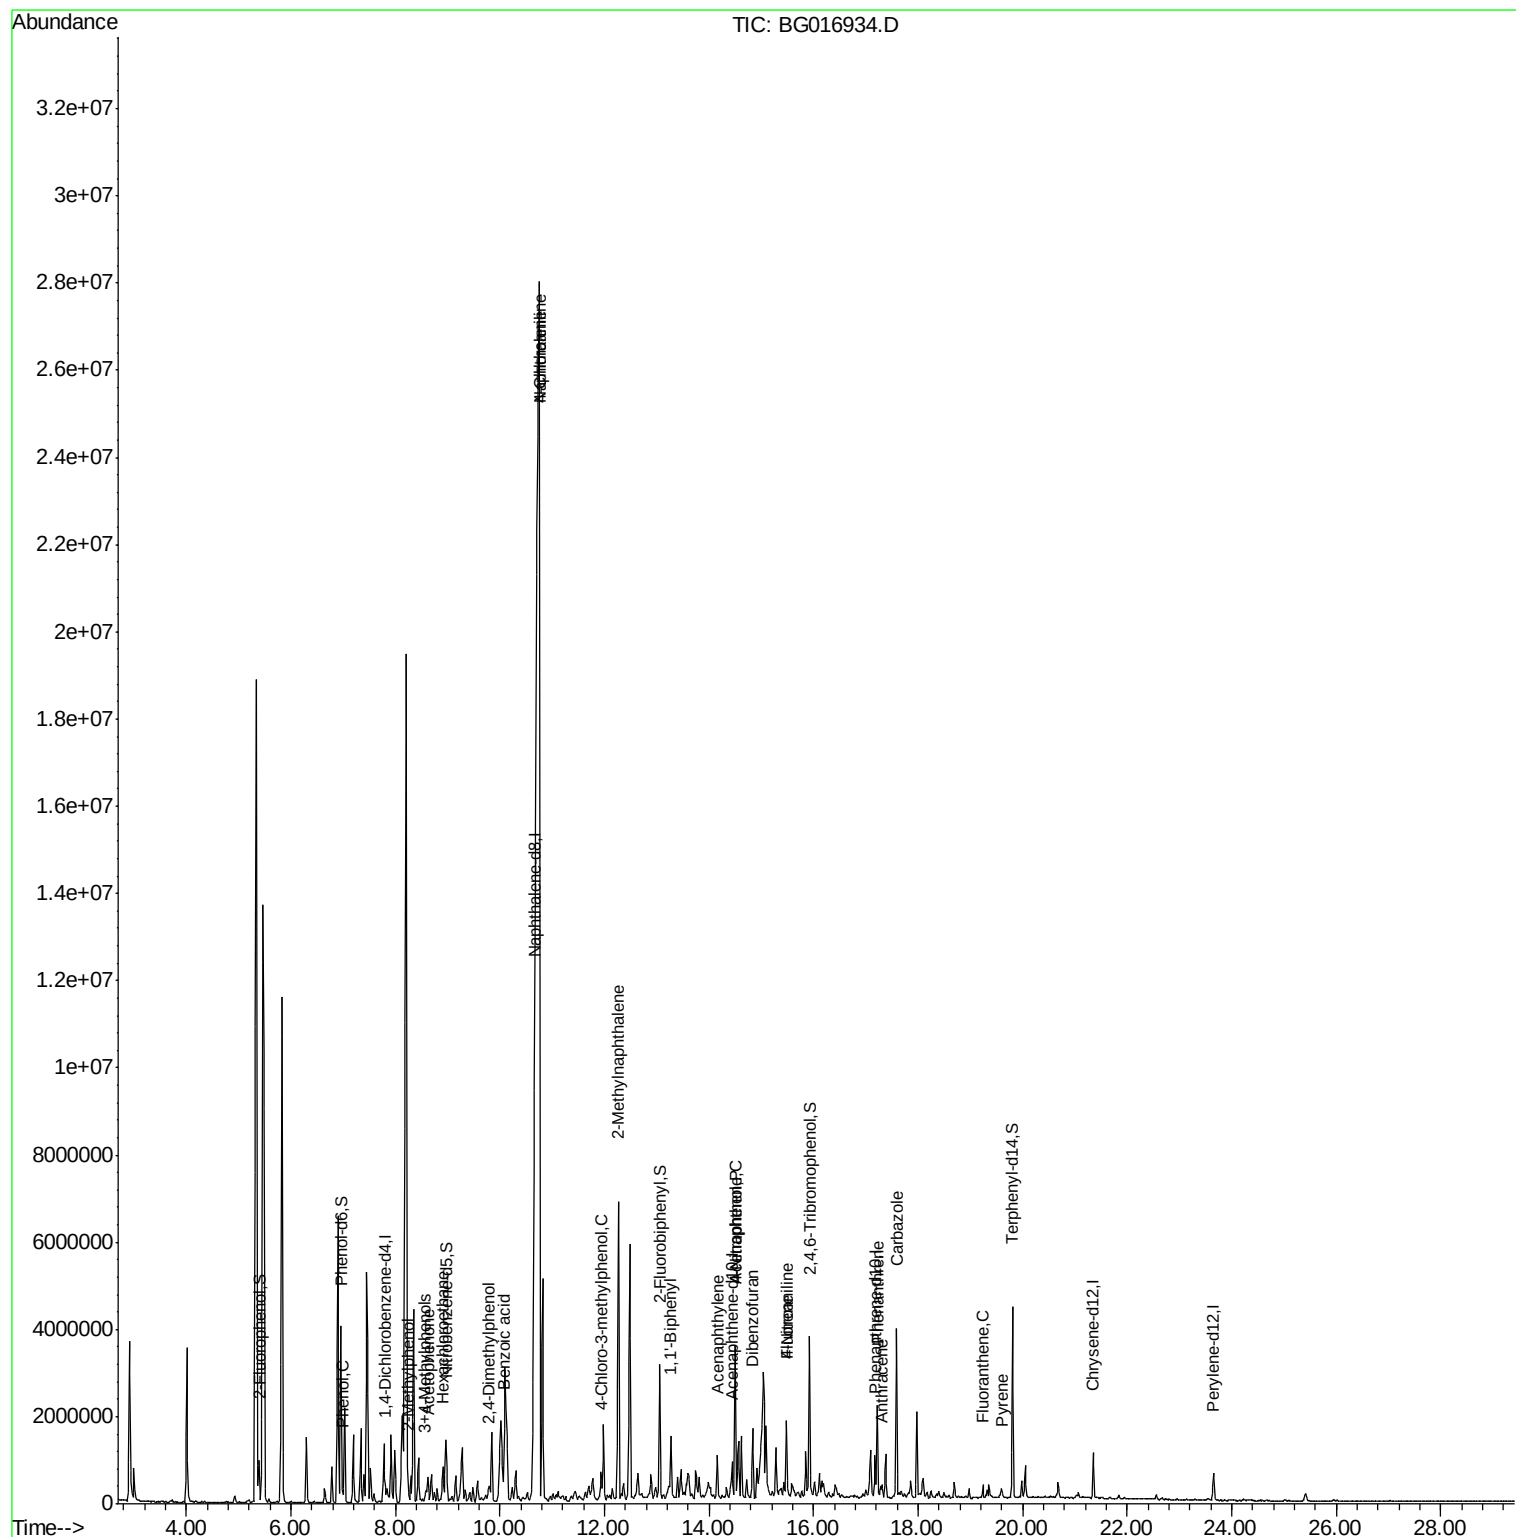

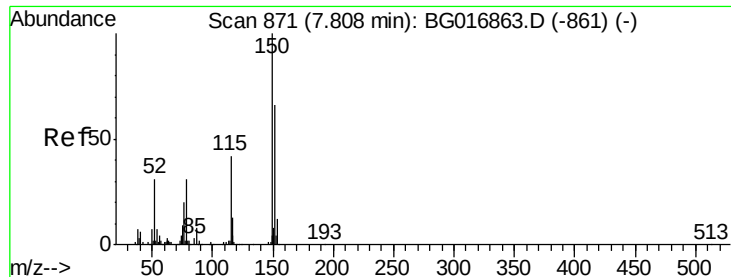


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.81 min Scan# 871
Delta R.T. 0.01 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Instrument :
BNA_G
ClientSampleId :
DBMW-01

Tgt Ion:152 Resp: 82728
Ion Ratio Lower Upper
152 100
150 155.2 121.0 181.4
115 60.2 50.5 75.7




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

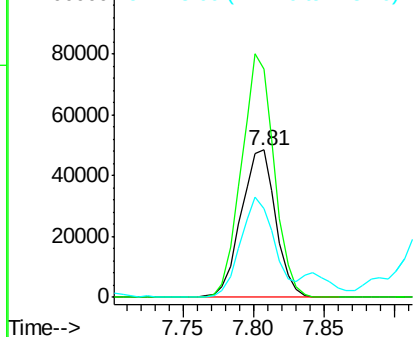



#5


2-Fluorophenol
Concen: 70.63 ng
RT: 5.39 min Scan# 460
Delta R.T. 0.01 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion:112 Resp: 335573
Ion Ratio Lower Upper
112 100
64 67.5 51.4 77.2
63 39.9 28.1 42.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

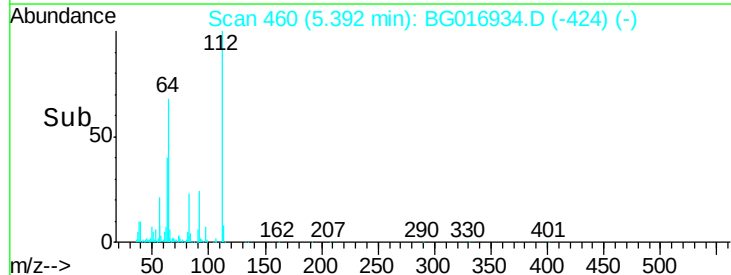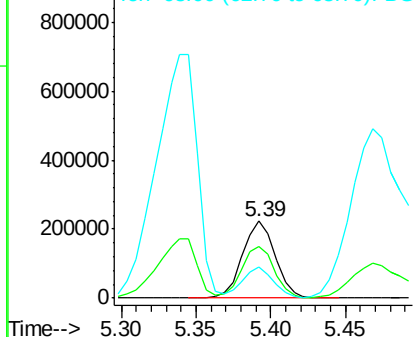



#7

Phenol-d6

Concen: 49.10 ng

RT: 6.97 min Scan# 728

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion: 99 Resp: 333283

Ion Ratio Lower Upper




99 100

42 28.4 22.1 33.1

71 45.4 33.4 50.0



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

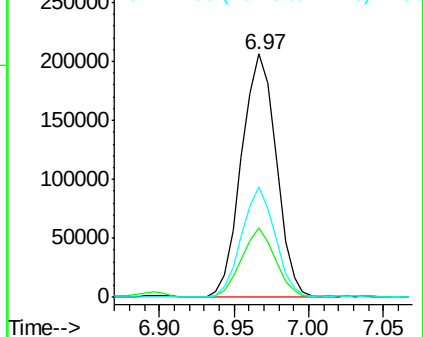

#9

Benzaldehyde

Concen: Below Cal

RT: 6.95 min Scan# 726

Delta R.T. 0.01 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion: 77 Resp: 360170

Ion Ratio Lower Upper



77 100


105 511.7 71.6 111.6#

106 73.7 71.5 111.5



Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 105.00 (104.70 to 105.70): BGC
Ion 106.00 (105.70 to 106.70): BGC

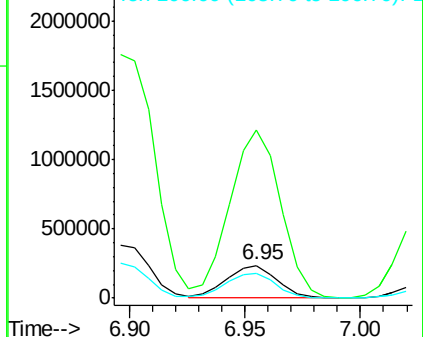



#10

Phenol

Concen: 9.29 ng

RT: 6.99 min Scan# 732

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion: 94 Resp: 67596

Ion Ratio Lower Upper




94 100

65 33.0 14.3 54.3

66 49.1 26.9 66.9



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

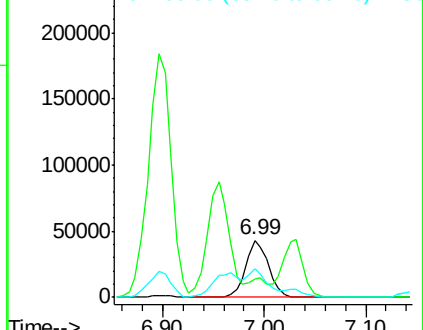

#17

2-Methylphenol

Concen: 4.19 ng

RT: 8.24 min Scan# 945

Delta R.T. 0.01 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Tgt Ion: 107 Resp: 21497


Ion Ratio Lower Upper

107 100



108 97.7 85.9 128.9


77 76.4 43.8 65.6#

79 57.4 39.8 59.6



Abundance Ion 107.00 (106.70 to 107.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC
Ion 79.00 (78.70 to 79.70): BGC

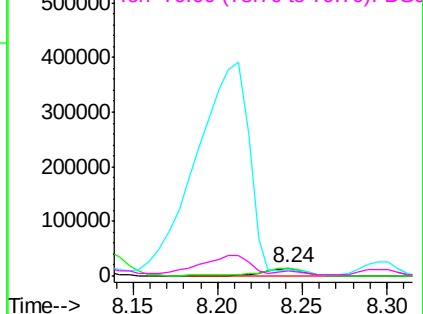



#18

Hexachloroethane

Concen: 31.60 ng

RT: 8.91 min Scan# 1058

Delta R.T. 0.03 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion:117 Resp: 79854

Ion Ratio Lower Upper

117 100

119 468.1 74.8 112.2#




201 0.0 72.1 108.1#



Abundance Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E

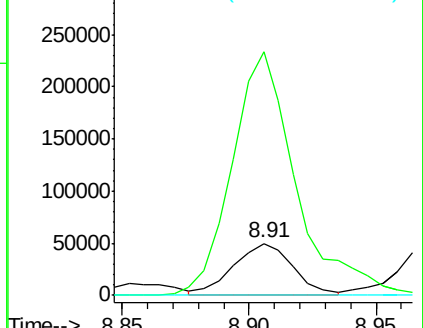

#20

3+4-Methylphenols

Concen: 6.94 ng

RT: 8.56 min Scan# 1000

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Tgt Ion:107 Resp: 48994


Ion Ratio Lower Upper

107 100

108 87.7 76.6 116.6

77 33.4 19.0 59.0

79 38.7 15.0 55.0






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BGC

Ion 79.00 (78.70 to 79.70): BGC



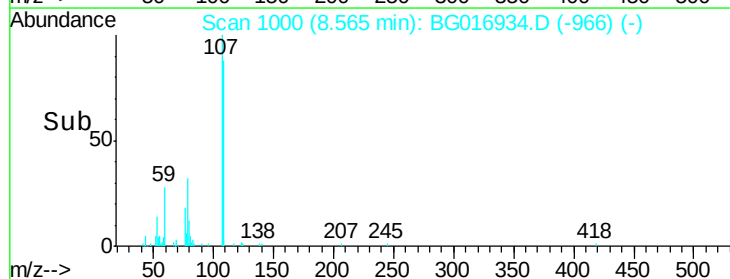
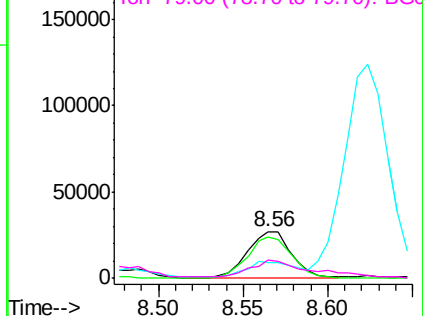




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.66 min Scan# 1356
Delta R.T. 0.07 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion:	136	Resp:	384601
Ion	Ratio	Lower	Upper
136	100		
137	11.7	9.8	14.8
54	11.7	8.7	13.1
68	5.5	5.0	7.4

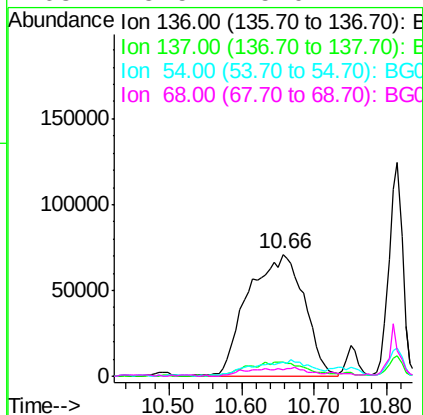

#22
Acetophenone
Concen: 32.23 ng
RT: 8.62 min Scan# 1010
Delta R.T. 0.01 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion:	105	Resp:	295231
Ion	Ratio	Lower	Upper
105	100		
71	0.7	2.8	4.2#
51	38.6	29.4	44.2
120	27.2	22.2	33.4



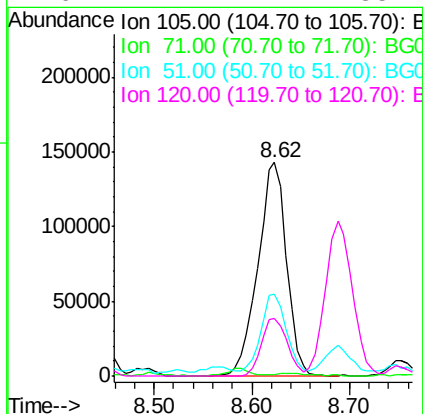





#23
Nitrobenzene-d5
Concen: 91.74 ng
RT: 8.96 min Scan# 1068
Delta R.T. 0.01 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion	Ratio	Lower	Upper
82	100		
128	41.2	33.2	49.8
54	61.2	48.6	72.8

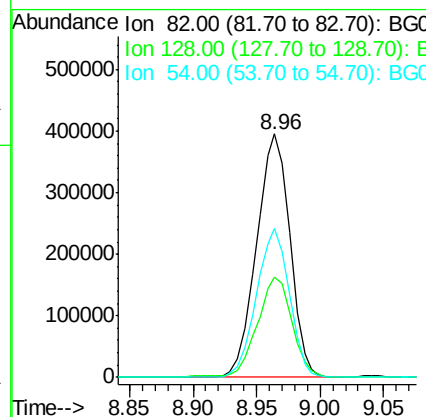

#27
2,4-Dimethylphenol
Concen: 27.28 ng
RT: 9.79 min Scan# 1208
Delta R.T. 0.02 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion	Ratio	Lower	Upper
122	100		
107	126.6	97.6	146.4
121	56.7	48.4	72.6



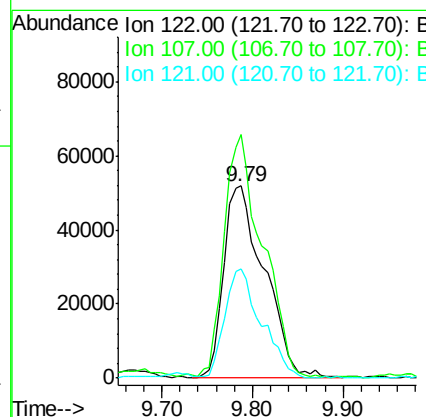





#31
Naphthalene
Concen: 1109.69 ng
RT: 10.76 min Scan# 1373
Delta R.T. 0.11 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion:128 Resp:21227578
Ion Ratio Lower Upper
128 100
129 64.6 9.1 13.7#
127 67.0 10.9 16.3#

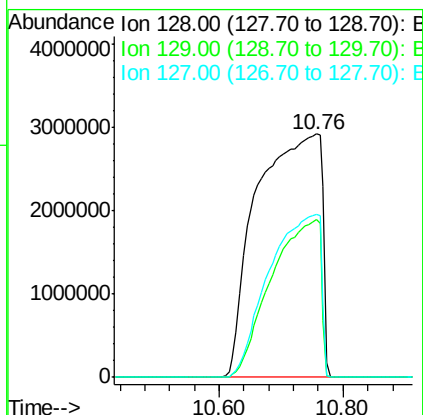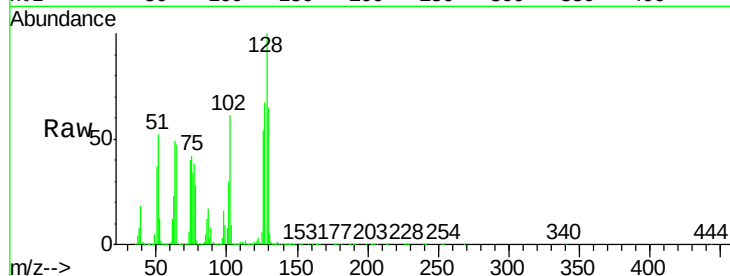

#32
Benzoic acid
Concen: 41.34 ng
RT: 10.07 min Scan# 1257
Delta R.T. 0.18 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion:122 Resp: 139246
Ion Ratio Lower Upper
122 100
105 8.5 123.2 163.2#
77 91.1 93.0 133.0#



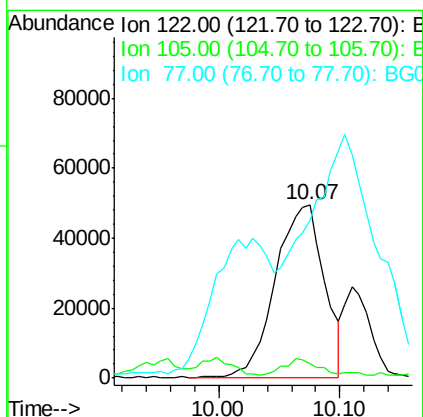





#33
 4-Chloroaniline
 Concen: 1277.33 ng
 RT: 10.76 min Scan# 1373
 Delta R.T. 0.01 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33




Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01


Tgt Ion:127 Resp:11284578
 Ion Ratio Lower Upper
 127 100
 129 96.4 25.8 38.6#
 65 0.0 28.2 42.2#
 92 0.1 15.6 23.4#

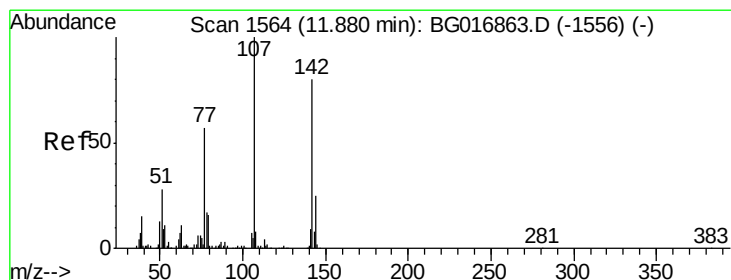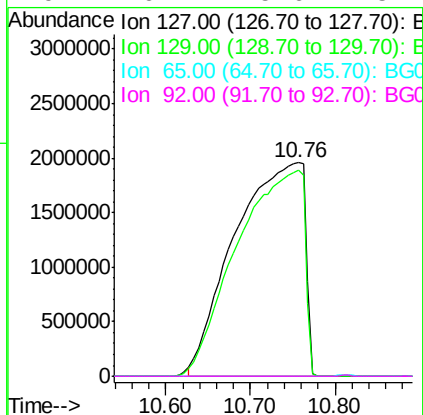

#36
 4-Chloro-3-methylphenol
 Concen: 17.77 ng
 RT: 11.94 min Scan# 1574
 Delta R.T. 0.07 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33

Tgt Ion:107 Resp: 125956
 Ion Ratio Lower Upper
 107 100
 144 0.6 20.2 30.2#
 142 1.9 64.2 96.2#



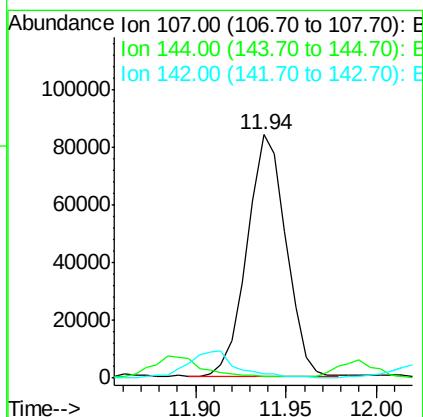
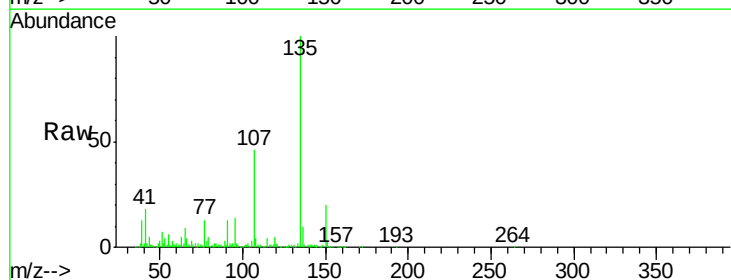




#37
 2-Methylnaphthalene
 Concen: 208.68 ng
 RT: 12.27 min Scan# 1630
 Delta R.T. 0.01 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33




Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01


Tgt Ion:142 Resp: 3040485
 Ion Ratio Lower Upper
 142 100
 141 90.6 69.9 104.9
 115 50.0 29.8 44.8#

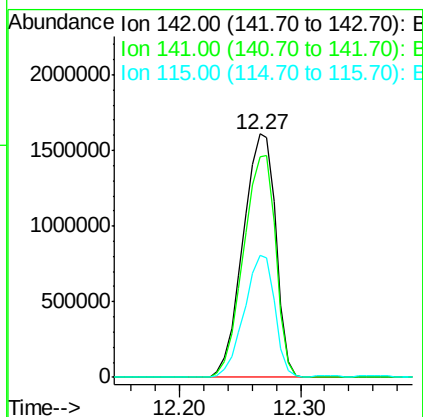

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.44 min Scan# 2000
 Delta R.T. 0.00 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33

Tgt Ion:164 Resp: 219105
 Ion Ratio Lower Upper
 164 100
 162 98.5 74.0 111.0
 160 45.3 34.7 52.1

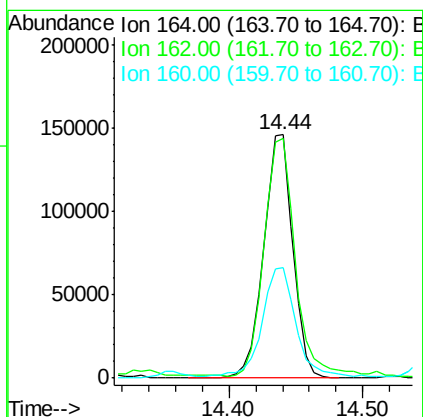



#41

2,4,6-Tribromophenol

Concen: 160.46 ng

RT: 15.93 min Scan# 2253

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion:330 Resp: 352953

Ion Ratio Lower Upper

330 100

332 95.6 0.0 0.0#




141 49.5 0.0 0.0#

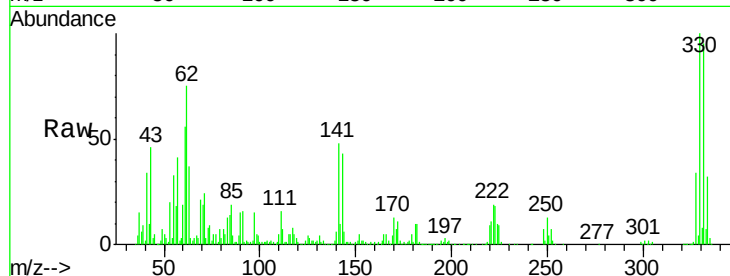

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

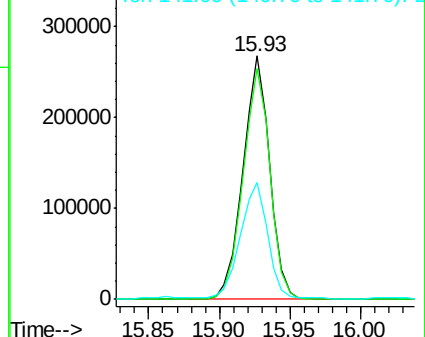

#44

2-Fluorobiphenyl

Concen: 95.40 ng

RT: 13.06 min Scan# 1765

Delta R.T. -0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion:172 Resp: 1385127

Ion Ratio Lower Upper

172 100

171 38.3 29.0 43.4



170 25.6 19.0 28.4




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E




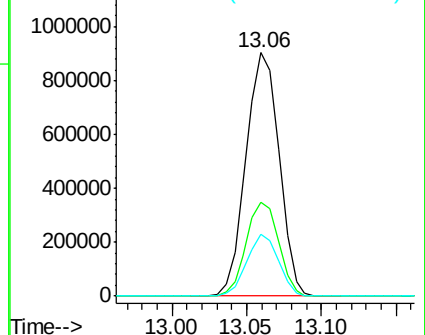




#45
 1,1'-Biphenyl
 Concen: 40.66 ng
 RT: 13.27 min Scan# 1801
 Delta R.T. 0.00 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33




Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01


Tgt Ion:154 Resp: 637873
 Ion Ratio Lower Upper
 154 100
 153 43.5 22.0 62.0
 76 14.7 0.0 33.3

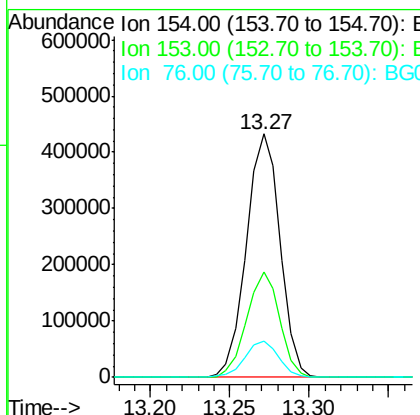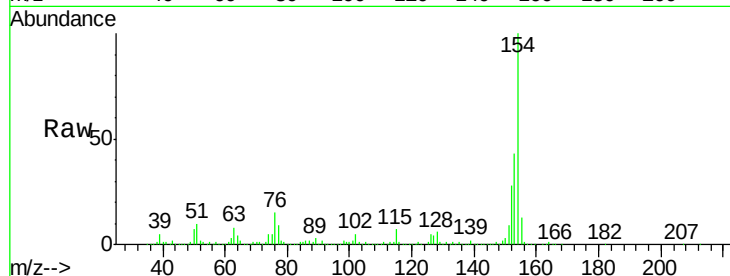

#48
 Acenaphthylene
 Concen: 18.61 ng
 RT: 14.16 min Scan# 1952
 Delta R.T. -0.00 min
 Lab File: BG016934.D
 Acq: 7 May 2015 23:33

Tgt Ion:152 Resp: 402733
 Ion Ratio Lower Upper
 152 100
 151 21.6 17.0 25.4
 153 16.3 10.7 16.1#

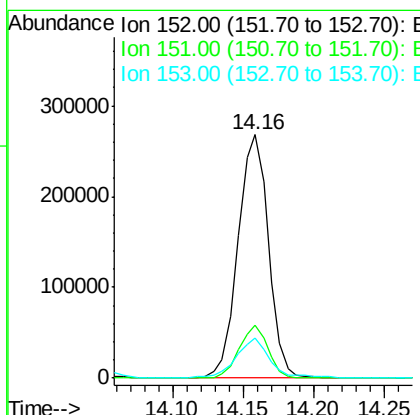



#51

Acenaphthene

Concen: 92.49 ng

RT: 14.50 min Scan# 2011

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampled :

DBMW-01


Tgt Ion:154 Resp: 1191056

Ion Ratio Lower Upper

154 100

153 107.3 84.2 126.4




152 53.6 40.2 60.2



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

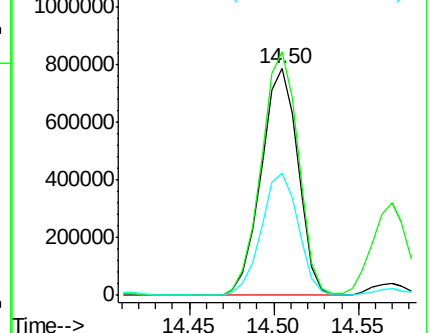

#54

Dibenzofuran

Concen: 46.75 ng

RT: 14.84 min Scan# 2068

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion:168 Resp: 854948

Ion Ratio Lower Upper

168 100

139 42.8 32.5 48.7



169 13.4 10.4 15.6




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E




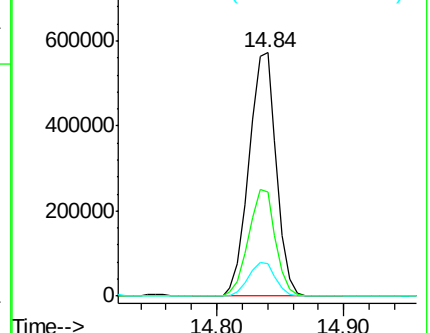




#55
4-Nitrophenol
Concen: 3.72 ng
RT: 14.50 min Scan# 2010
Delta R.T. -0.14 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion:139 Resp: 12205
Ion Ratio Lower Upper
139 100
109 32.6 61.8 101.8#
65 71.7 96.8 136.8#

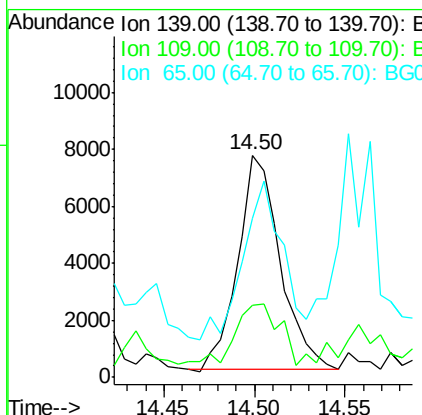

#57
Fluorene
Concen: 43.69 ng
RT: 15.49 min Scan# 2178
Delta R.T. 0.00 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion:166 Resp: 707385
Ion Ratio Lower Upper
166 100
165 93.6 76.1 114.1
167 14.1 11.4 17.2


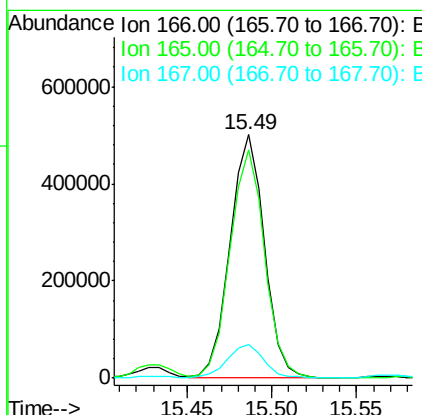






#61
4-Nitroaniline
Concen: 2.48 ng
RT: 15.49 min Scan# 2178
Delta R.T. -0.02 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion:138 Resp: 11123
Ion Ratio Lower Upper
138 100
92 8.0 31.8 71.8#
108 6.7 70.6 110.6#

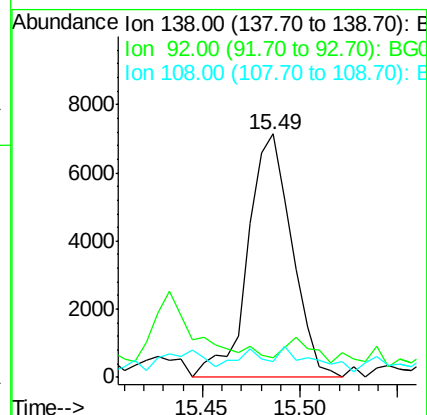

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.18 min Scan# 2466
Delta R.T. -0.00 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion:188 Resp: 436016
Ion Ratio Lower Upper
188 100
94 9.4 8.2 12.4
80 12.1 8.8 13.2

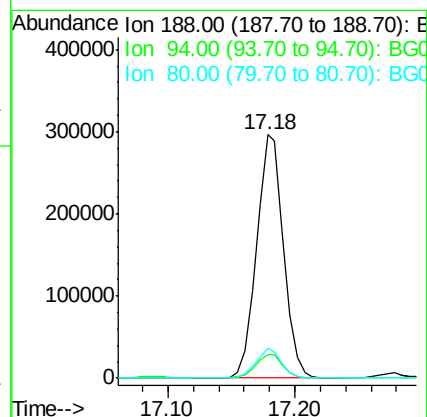



#70

Phenanthrene

Concen: 48.78 ng

RT: 17.23 min Scan# 2474

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion:178 Resp: 1094460

Ion Ratio Lower Upper

178 100

176 20.7 16.0 24.0




179 16.4 13.0 19.6



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

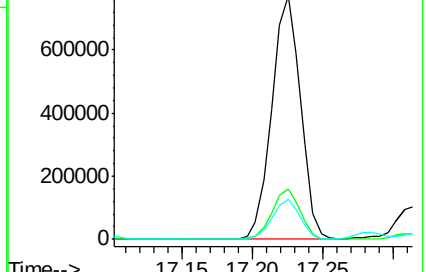

#71

Anthracene

Concen: 6.51 ng

RT: 17.31 min Scan# 2489

Delta R.T. -0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion:178 Resp: 147467

Ion Ratio Lower Upper

178 100

176 17.4 16.2 24.4



179 15.6 13.1 19.7




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

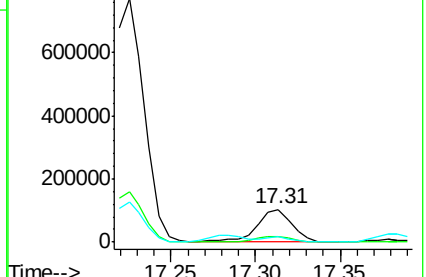



#72

Carbazole

Concen: 99.46 ng

RT: 17.59 min Scan# 2536

Delta R.T. 0.01 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion:167 Resp: 2140304

Ion Ratio Lower Upper

167 100

166 27.0 18.4 27.6




139 18.0 12.2 18.4



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

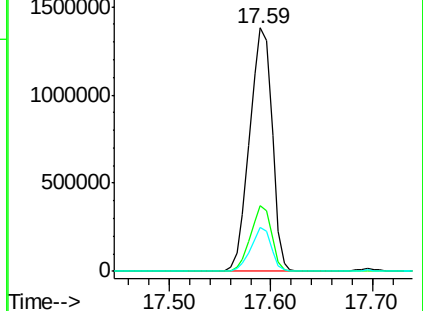

#74

Fluoranthene

Concen: 5.67 ng

RT: 19.24 min Scan# 2817

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion:202 Resp: 147512

Ion Ratio Lower Upper

202 100

101 12.9 0.0 31.5



203 16.0 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E




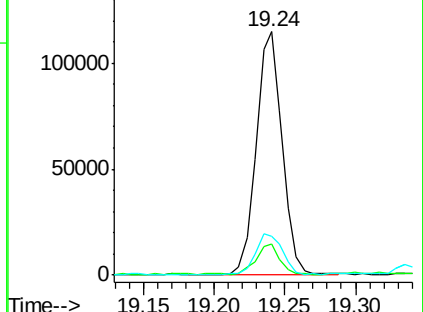




#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.36 min Scan# 3177
Delta R.T. -0.00 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33




Instrument :
BNA_G
ClientSampleId :
DBMW-01


Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.7	9.1	13.7
236	25.0	20.2	30.4

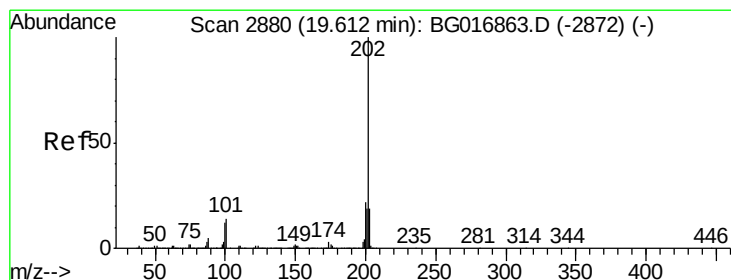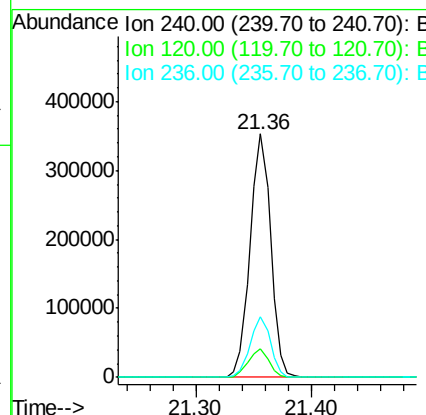

#77
Pyrene
Concen: 3.66 ng
RT: 19.60 min Scan# 2878
Delta R.T. -0.00 min
Lab File: BG016934.D
Acq: 7 May 2015 23:33

Tgt Ion	Ratio	Lower	Upper
202	100		
200	18.5	17.9	26.9
203	19.5	15.2	22.8

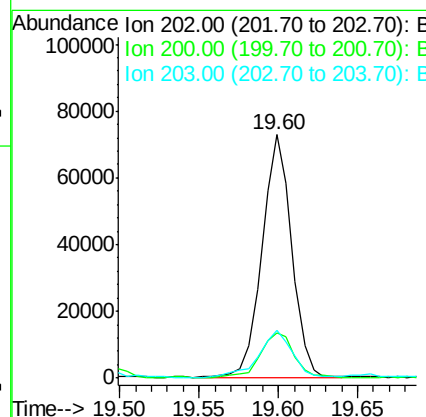



#78

Terphenyl-d14

Concen: 90.32 ng

RT: 19.81 min Scan# 2914

Delta R.T. 0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33

Instrument :

BNA_G

ClientSampleId :

DBMW-01


Tgt Ion:244 Resp: 1695866

Ion Ratio Lower Upper

244 100

212 9.0 7.0 10.6




122 13.0 10.4 15.6



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

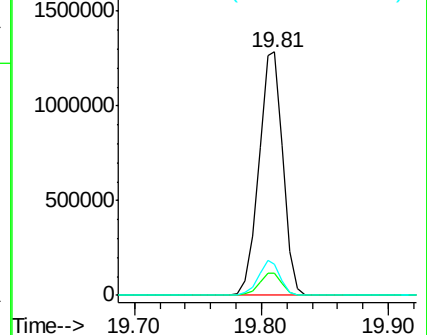

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.66 min Scan# 3569

Delta R.T. -0.00 min

Lab File: BG016934.D

Acq: 7 May 2015 23:33


Tgt Ion:264 Resp: 420421

Ion Ratio Lower Upper

264 100

260 23.5 19.5 29.3

265 22.4 18.5 27.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

