
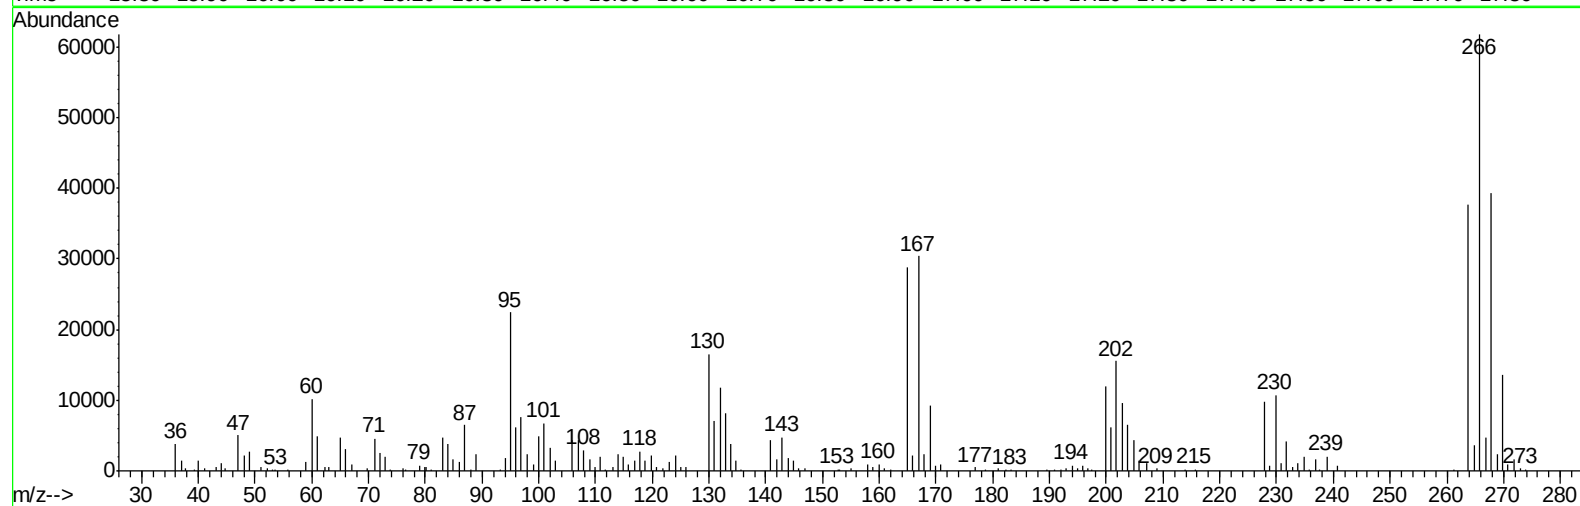


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050715\
Data File : BG016912.D
Acq On : 7 May 2015 8:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 06:47:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 08 04:04:43 2015
Response via : Initial Calibration

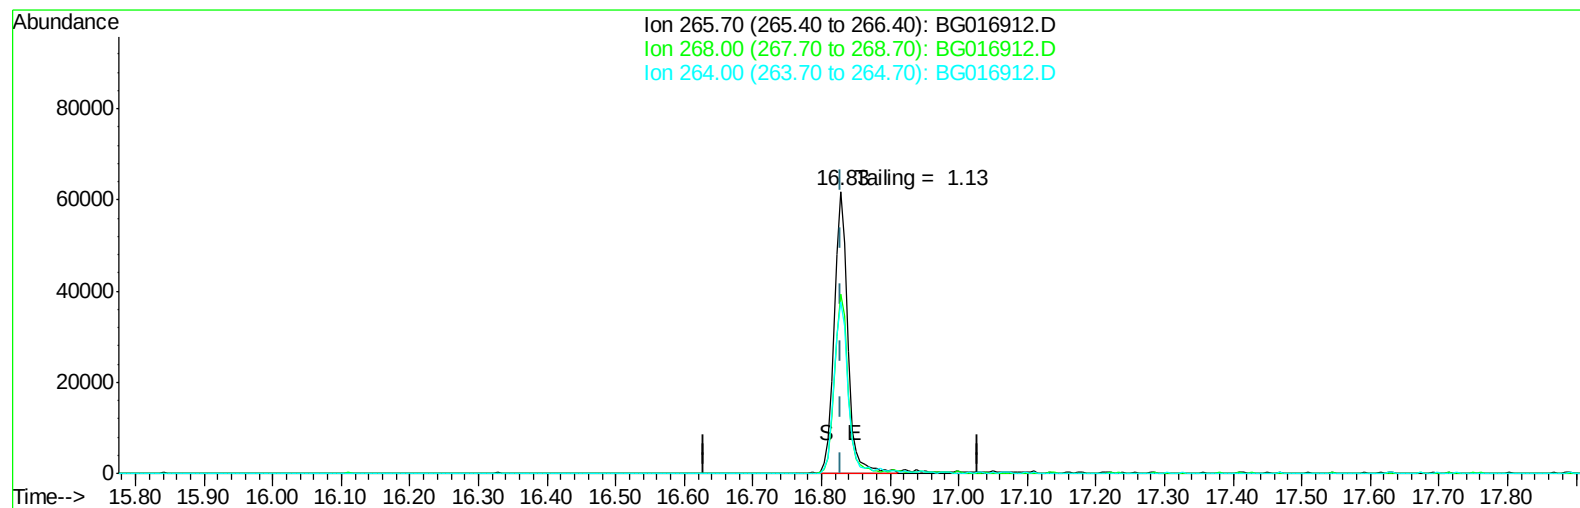

TIC: BG016912.D

(69) Pentachlorophenol (C)



16.827min (-0.002) 41770.22ng

response 85539

Ion	Exp%	Act%
265.70	100	100
268.00	69.00	63.62
264.00	64.20	61.02
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050715\
Data File : BG016912.D
Acq On : 7 May 2015 8:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 08 06:47:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 08 04:04:43 2015
Response via : Initial Calibration

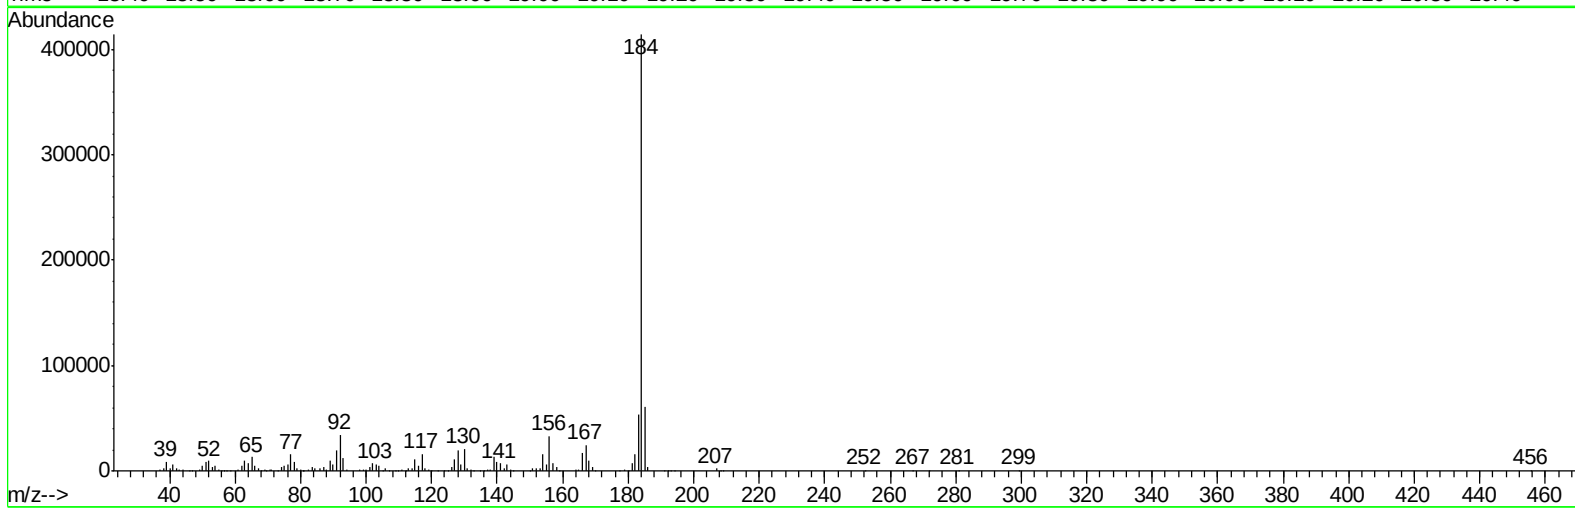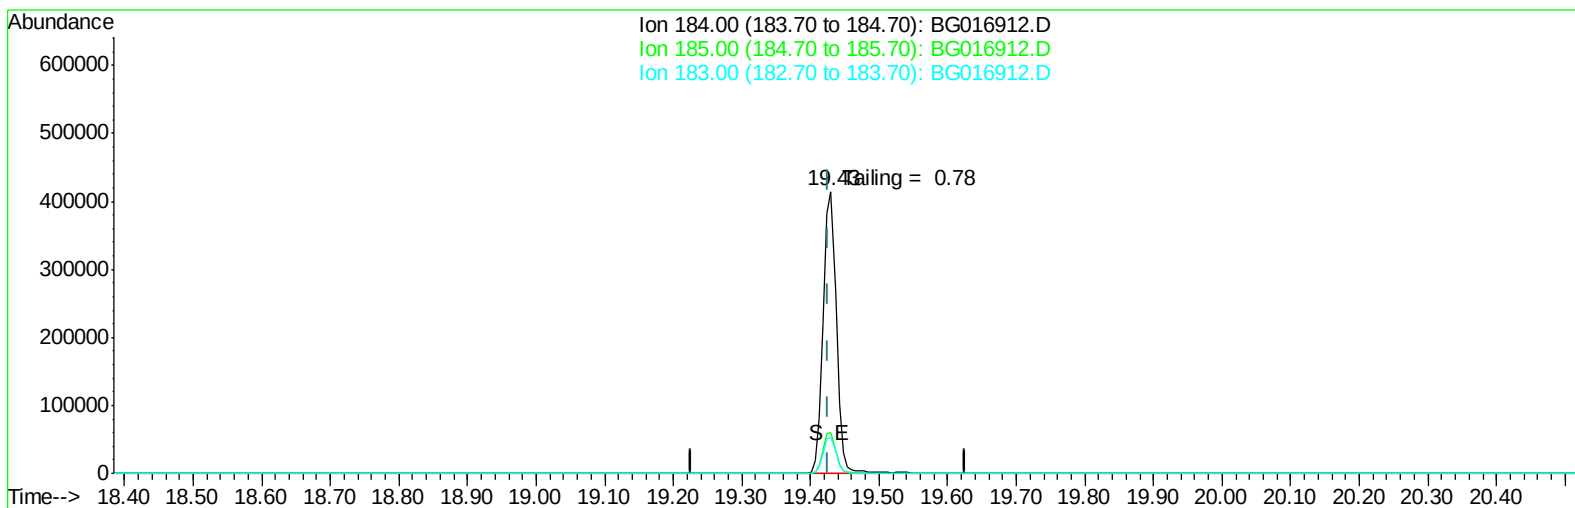

TIC: BG016912.D

(76) Benzidine

19.430min (+0.004) 17272.36ng

response 548743

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.66
183.00	13.20	12.86
0.00	0.00	0.00