

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050715\
 Data File : BG016937.D
 Acq On : 8 May 2015 1:18
 Operator : TP/IZ
 Sample : G2038-03MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.907	32	37	49	rBV	3310608	5654105	4.01%	0.975%
2	4.006	218	224	241	rBV	3186347	4891449	3.47%	0.844%
3	5.340	441	451	456	rBV	18205260	35531621	25.18%	6.128%
4	5.392	456	460	465	rVV	944322	1430609	1.01%	0.247%
5	5.469	465	473	487	rVB	12515566	32015020	22.69%	5.521%
6	5.827	523	534	542	rBV	10350767	18061184	12.80%	3.115%
7	6.297	607	614	624	rVB	1291839	1962767	1.39%	0.339%
8	6.897	707	716	721	rVV	6044219	9872796	7.00%	1.703%
9	6.955	721	726	732	rVV2	3654072	6315211	4.48%	1.089%
10	7.026	734	738	749	rVB	2004170	3074145	2.18%	0.530%
11	7.190	760	766	770	rBV	1381582	2198338	1.56%	0.379%
12	7.337	780	791	795	rBV	1586772	2952572	2.09%	0.509%
13	7.455	805	811	819	rVV2	4824700	9396213	6.66%	1.621%
14	7.778	860	866	873	rVV2	1118510	2417443	1.71%	0.417%
15	7.837	873	876	882	rVV2	846112	1457278	1.03%	0.251%
16	7.919	884	890	896	rVV	1416911	2437361	1.73%	0.420%
17	7.989	896	902	908	rVB	1128190	1994206	1.41%	0.344%
18	8.130	918	926	929	rVV2	1845539	3819991	2.71%	0.659%
19	8.207	929	939	943	rVV	18875383	45697923	32.38%	7.881%
20	8.342	957	962	969	rVB	4881530	8328936	5.90%	1.436%
21	8.436	969	978	984	rBV	907028	1517833	1.08%	0.262%
22	8.624	1005	1010	1016	rVV	1869229	3479125	2.47%	0.600%
23	8.971	1062	1069	1083	rVB3	1292314	4109838	2.91%	0.709%
24	9.276	1114	1121	1127	rVB	1054077	2227034	1.58%	0.384%
25	9.564	1162	1170	1180	rBV3	918339	2124557	1.51%	0.366%
26	9.793	1202	1209	1213	rVV2	878410	1926449	1.37%	0.332%
27	9.846	1213	1218	1224	rVB	1437356	2401270	1.70%	0.414%
28	10.022	1233	1248	1256	rBV7	1872555	7008274	4.97%	1.209%
29	10.105	1256	1262	1275	rVB	2924926	8907563	6.31%	1.536%
30	10.299	1287	1295	1301	rVB2	668801	2069053	1.47%	0.357%
31	10.751	1342	1372	1376	rBV	27322118	141115258	100.00%	24.337%
32	10.810	1376	1382	1387	rVB	4742192	6879117	4.87%	1.186%
33	10.945	1399	1405	1413	rBV3	834506	1691603	1.20%	0.292%
34	11.879	1558	1564	1570	rBV	868869	1504089	1.07%	0.259%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050715\
 Data File : BG016937.D
 Acq On : 8 May 2015 1:18
 Operator : TP/IZ
 Sample : G2038-03MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBMW-01MSD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.991	1578	1583	1590	rVB	1584641	2630054	1.86%	0.454%
36	12.267	1621	1630	1636	rVB	7519296	13172155	9.33%	2.272%
37	12.490	1657	1668	1673	rVB	6328443	10961820	7.77%	1.891%
38	12.625	1681	1691	1699	rBV7	1450543	4347430	3.08%	0.750%
39	12.866	1724	1732	1735	rBV	1020400	1630091	1.16%	0.281%
40	12.925	1735	1742	1749	rVV3	1550399	4265744	3.02%	0.736%
41	13.060	1760	1765	1771	rVB	2996514	4401231	3.12%	0.759%
42	13.271	1796	1801	1805	rVV	2870606	4530473	3.21%	0.781%
43	13.313	1805	1808	1814	rVB	1348233	1888231	1.34%	0.326%
44	13.612	1854	1859	1867	rVB7	581052	1447561	1.03%	0.250%
45	13.812	1888	1893	1901	rVV2	1060715	1739542	1.23%	0.300%
46	13.900	1901	1908	1913	rVV	1327106	2061736	1.46%	0.356%
47	13.953	1913	1917	1921	rVV	866558	1496994	1.06%	0.258%
48	14.018	1921	1928	1937	rVV2	1182300	2434047	1.72%	0.420%
49	14.165	1948	1953	1962	rVB	2446018	3816041	2.70%	0.658%
50	14.511	2005	2012	2016	rBV	4646224	7411621	5.25%	1.278%
51	14.552	2016	2019	2027	rVB2	1122064	2322430	1.65%	0.401%
52	14.629	2027	2032	2035	rBV	1378982	2421945	1.72%	0.418%
53	14.840	2064	2068	2075	rVB	2969734	4365997	3.09%	0.753%
54	14.981	2078	2092	2096	rBV2	2083129	4979021	3.53%	0.859%
55	15.058	2098	2105	2109	rVV2	3572545	9194537	6.52%	1.586%
56	15.093	2109	2111	2117	rVB	1470442	1851819	1.31%	0.319%
57	15.269	2136	2141	2151	rBV2	1893231	3560455	2.52%	0.614%
58	15.487	2172	2178	2186	rVB2	4632724	7133234	5.05%	1.230%
59	15.698	2208	2214	2222	rBV	1924353	2717584	1.93%	0.469%
60	15.774	2222	2227	2233	rVV	1584168	2208046	1.56%	0.381%
61	15.857	2235	2241	2245	rVV2	1023987	1502019	1.06%	0.259%
62	15.927	2245	2253	2263	rVV	3745989	5306969	3.76%	0.915%
63	16.374	2324	2329	2333	rBV2	1427165	1924967	1.36%	0.332%
64	16.485	2343	2348	2354	rVB	1348706	1880286	1.33%	0.324%
65	16.662	2371	2378	2383	rBV	1150829	1621167	1.15%	0.280%
66	16.832	2402	2407	2414	rVB	2137295	2936065	2.08%	0.506%
67	17.096	2443	2452	2458	rVV2	1091256	2369047	1.68%	0.409%
68	17.226	2470	2474	2480	rVV	3678146	5511309	3.91%	0.951%
69	17.314	2480	2489	2495	rVV	2146018	3458589	2.45%	0.596%
70	17.596	2529	2537	2542	rVB	4903049	7444070	5.28%	1.284%
71	18.154	2627	2632	2641	rVB	2098656	2817475	2.00%	0.486%

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050715\
Data File : BG016937.D
Acq On : 8 May 2015 1:18
Operator : TP/IZ
Sample : G2038-03MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBMW-01MSD

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	19.241	2811	2817	2823	rBV	2413048	3136485	2.22%	0.541%
73	19.605	2869	2879	2886	rBV	2426925	3276106	2.32%	0.565%
74	19.805	2908	2913	2922	rBV	3901408	5121730	3.63%	0.883%
75	20.504	3027	3032	3036	rBV	2268478	2568620	1.82%	0.443%
76	20.575	3039	3044	3049	rVV	2885326	3130344	2.22%	0.540%
77	21.274	3159	3163	3169	rVB	2653271	3107979	2.20%	0.536%
78	21.350	3169	3176	3180	rBV2	2470966	4264526	3.02%	0.735%
79	21.397	3180	3184	3194	rVB	2355433	2962758	2.10%	0.511%
80	22.173	3311	3316	3323	rVB	2279432	3064662	2.17%	0.529%
81	22.966	3444	3451	3455	rBV	1638848	2976330	2.11%	0.513%
82	23.013	3455	3459	3466	rVB	1729168	2811917	1.99%	0.485%
83	23.565	3545	3553	3560	rBV	1493342	2838880	2.01%	0.490%
84	26.045	3959	3975	3987	rVB3	1786685	5598172	3.97%	0.965%
85	26.762	4083	4097	4109	rBV	831899	2736713	1.94%	0.472%


Sum of corrected areas: 579827255

Data Path : Z:\HPCHEM1\BNA G\DATA\BG050715\
Data File : BG016937.D
Acq On : 8 May 2015 1:18
Operator : TP/IZ
Sample : G2038-03MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBMW-01MSD

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

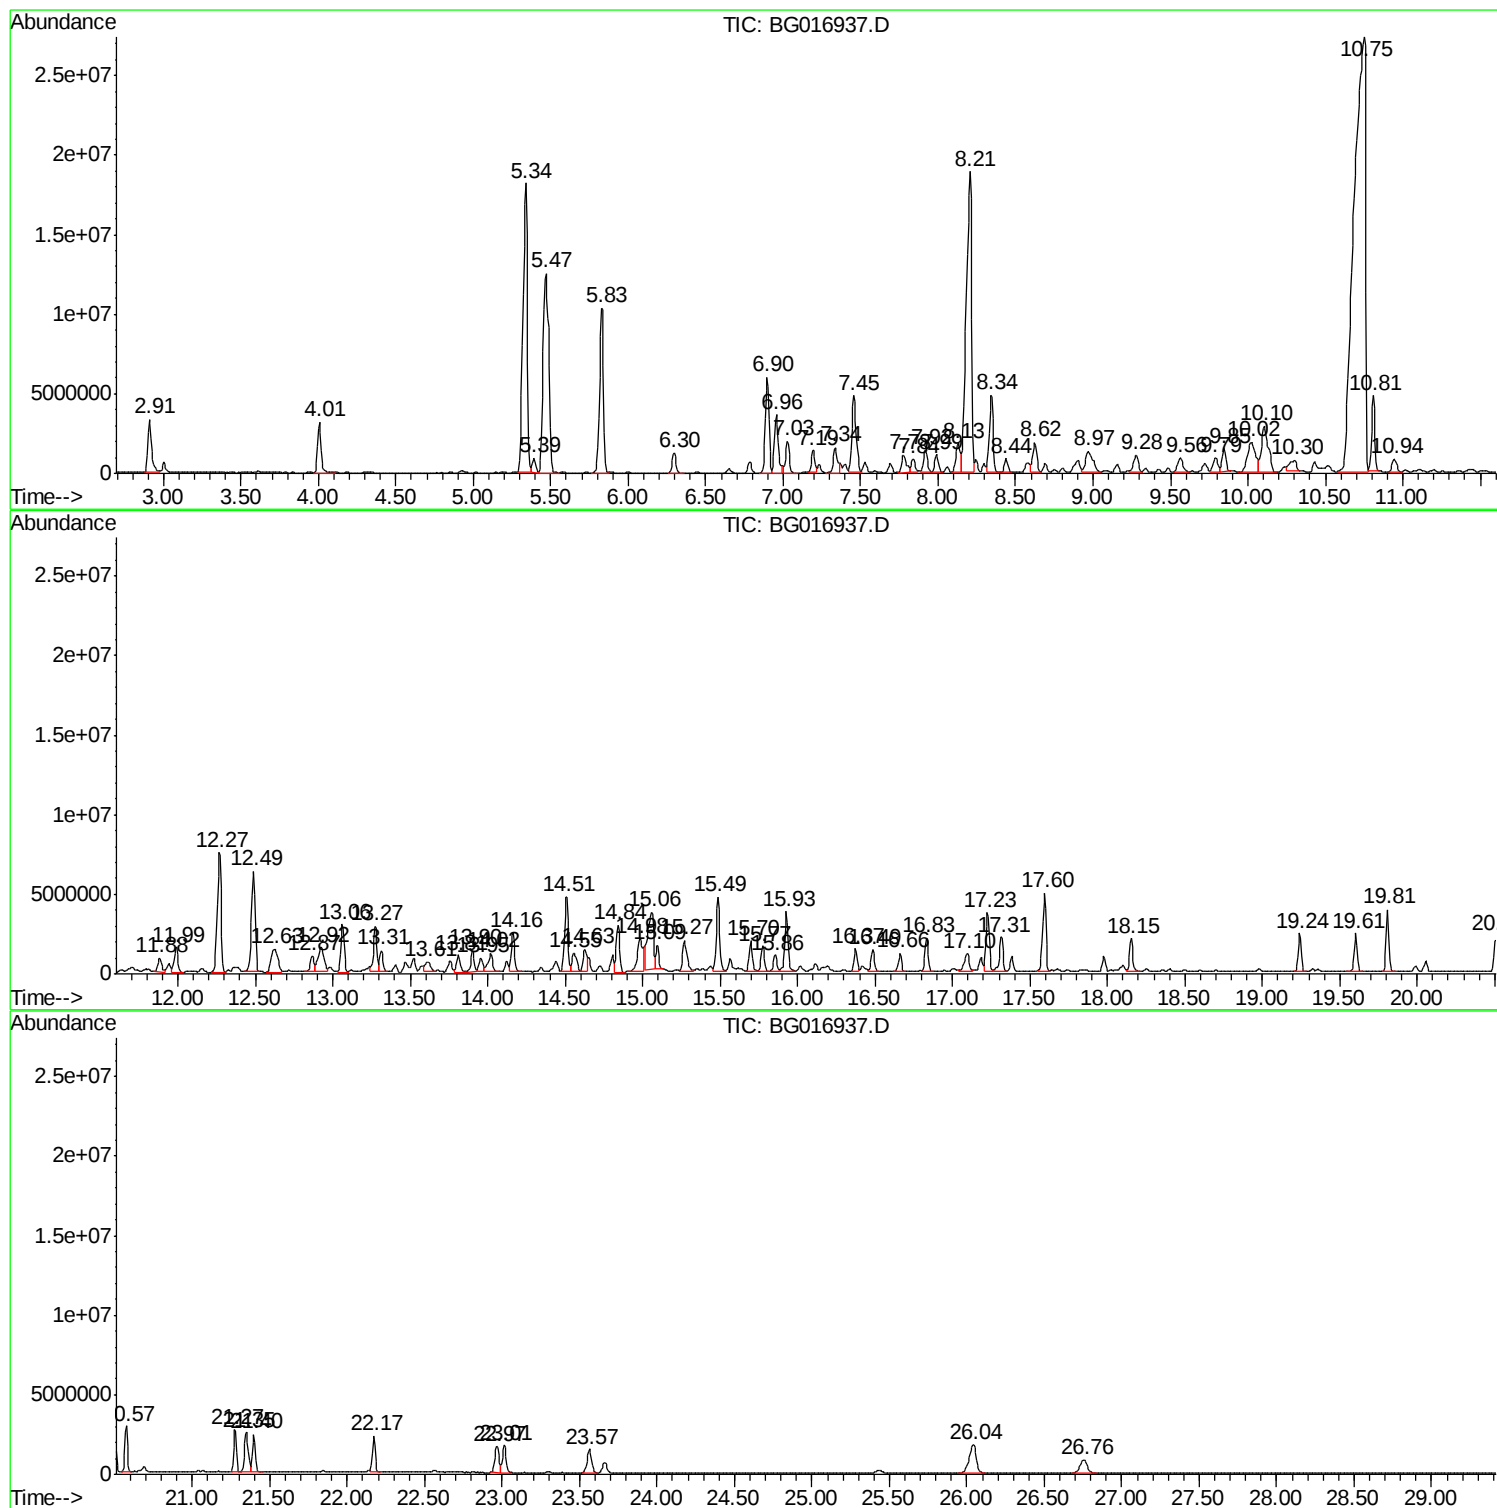

Data_Path : Z:\HPCHEM1\BNA_G\DATA\BG050715\
Data_File : BG016937.D
Acq_On : 8_May,2015 1:188
Operator : TP/IZZ
Sample : G2038-03MSDD
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
DBMW-01MSD

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
