
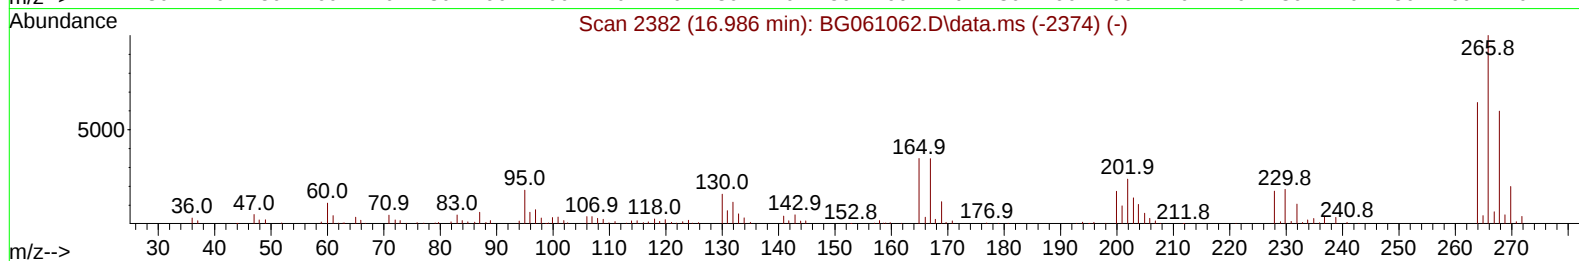
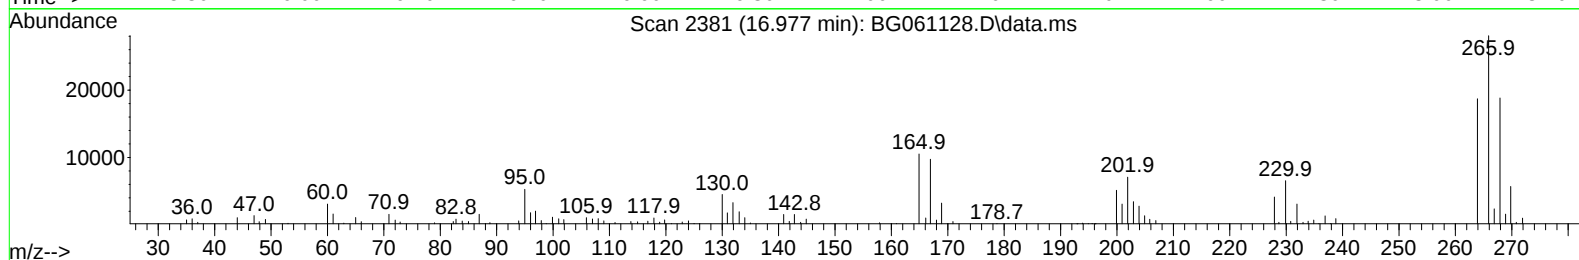


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050724\
Data File : BG061128.D
Acq On : 7 May 2024 11:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:14:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

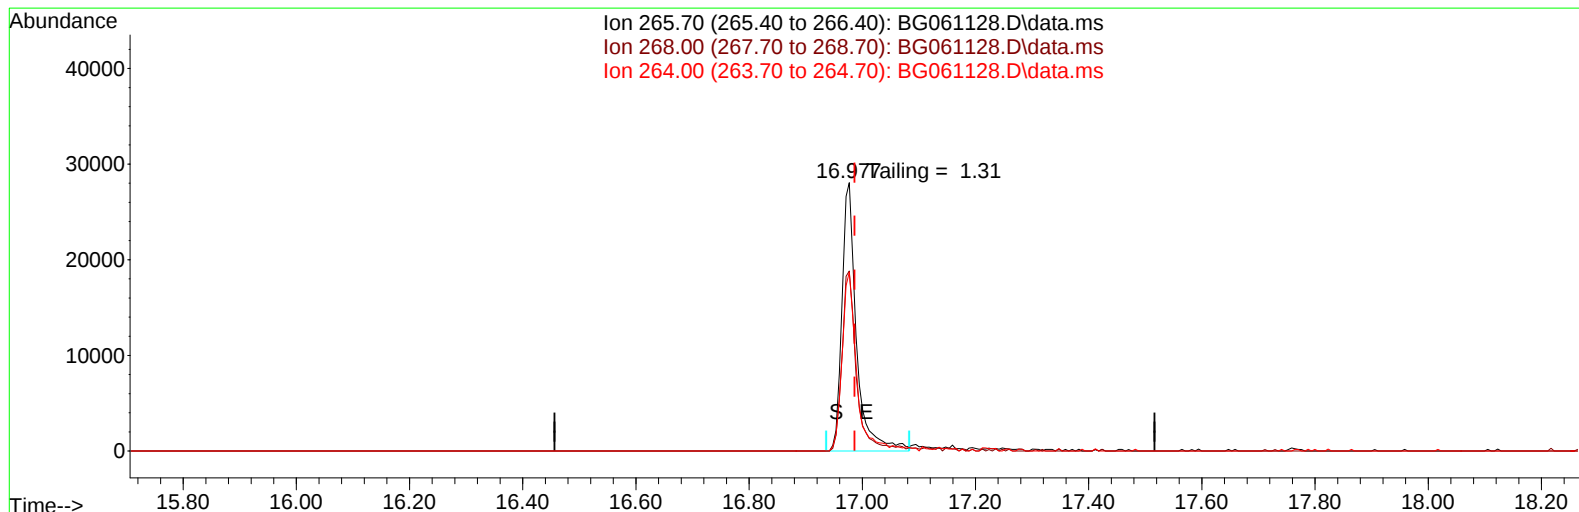

TIC: BG061128.D\data.ms

(70) Pentachlorophenol (C)




16.977min (-0.009) 12438.97 ng m

response 50309

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	59.80	67.05
264.00	64.40	66.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG050724\
Data File : BG061128.D
Acq On : 7 May 2024 11:15
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 07 12:14:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 05:11:25 2024
Response via : Initial Calibration

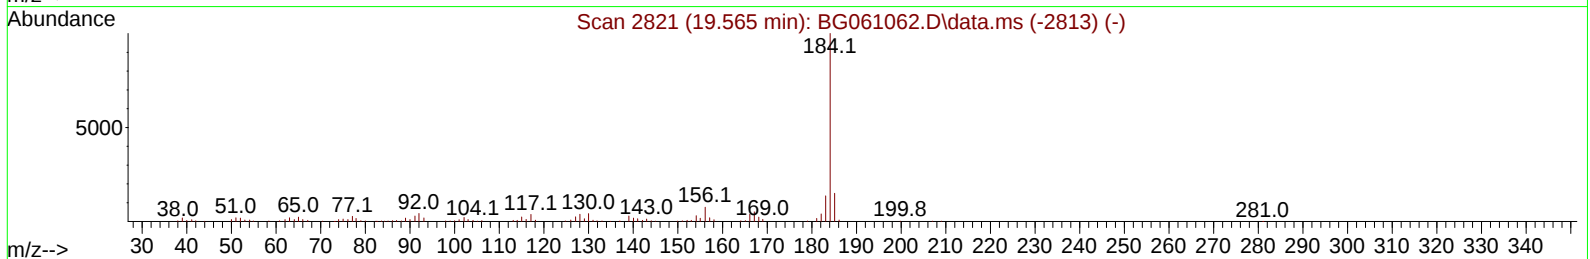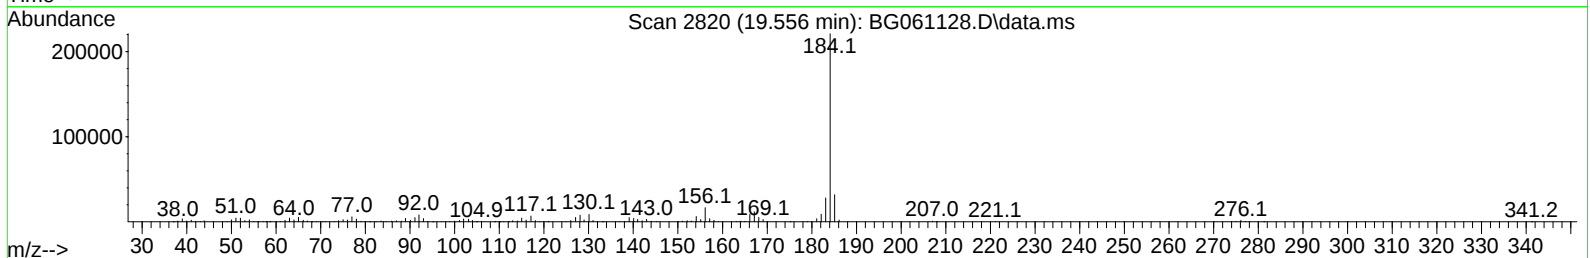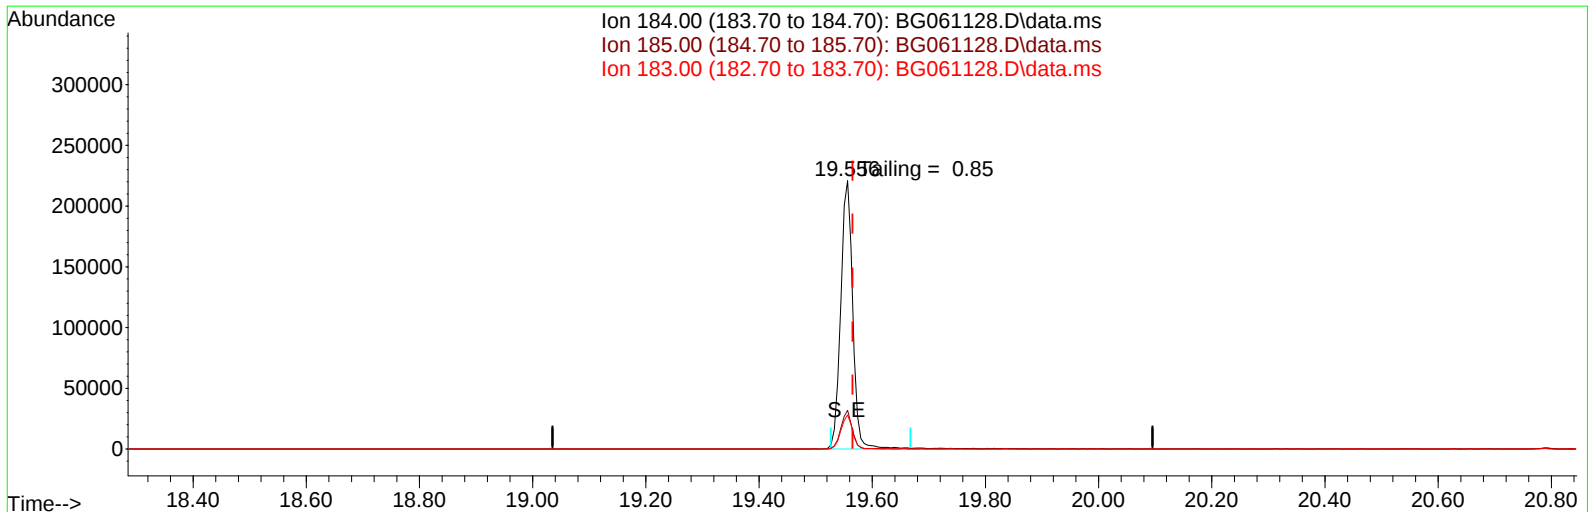

TIC: BG061128.D\data.ms

(77) Benzidine

19.556min (-0.009) 108931.01 ng

response 319144

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.47
183.00	13.60	12.71
0.00	0.00	0.00