

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
 Data File : BG017005.D
 Acq On : 10 May 2015 00:25
 Operator : TP/IZ
 Sample : G2104-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MW-105

Quant Time: May 11 01:24:38 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 05 16:13:58 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	72464	20.00	ng	-0.02
21) Naphthalene-d8	10.58	136	330726	20.00	ng	-0.01
38) Acenaphthene-d10	14.43	164	235610	20.00	ng	-0.02
63) Phenanthrene-d10	17.17	188	565206	20.00	ng	-0.02
75) Chrysene-d12	21.35	240	569921	20.00	ng	-0.02
86) Perylene-d12	23.64	264	555768	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	191079	45.91	ng	-0.01
7) Phenol-d6	6.96	99	197513	33.22	ng	0.00
23) Nitrobenzene-d5	8.95	82	400087	59.10	ng	-0.02
41) 2,4,6-Tribromophenol	15.91	330	271583	114.82	ng	-0.02
44) 2-Fluorobiphenyl	13.05	172	857197	54.90	ng	-0.02
78) Terphenyl-d14	19.80	244	1475018	60.67	ng	-0.02
Target Compounds						
32) Benzoic acid	9.91	122	65	Below Cal	Qvalue #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG050815\
Data File : BG017005.D
Acq On : 10 May 2015 00:25
Operator : TP/IZ
Sample : G2104-03
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MW-105

Quant Time: May 11 01:24:38 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG050515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 05 16:13:58 2015
Response via : Initial Calibration

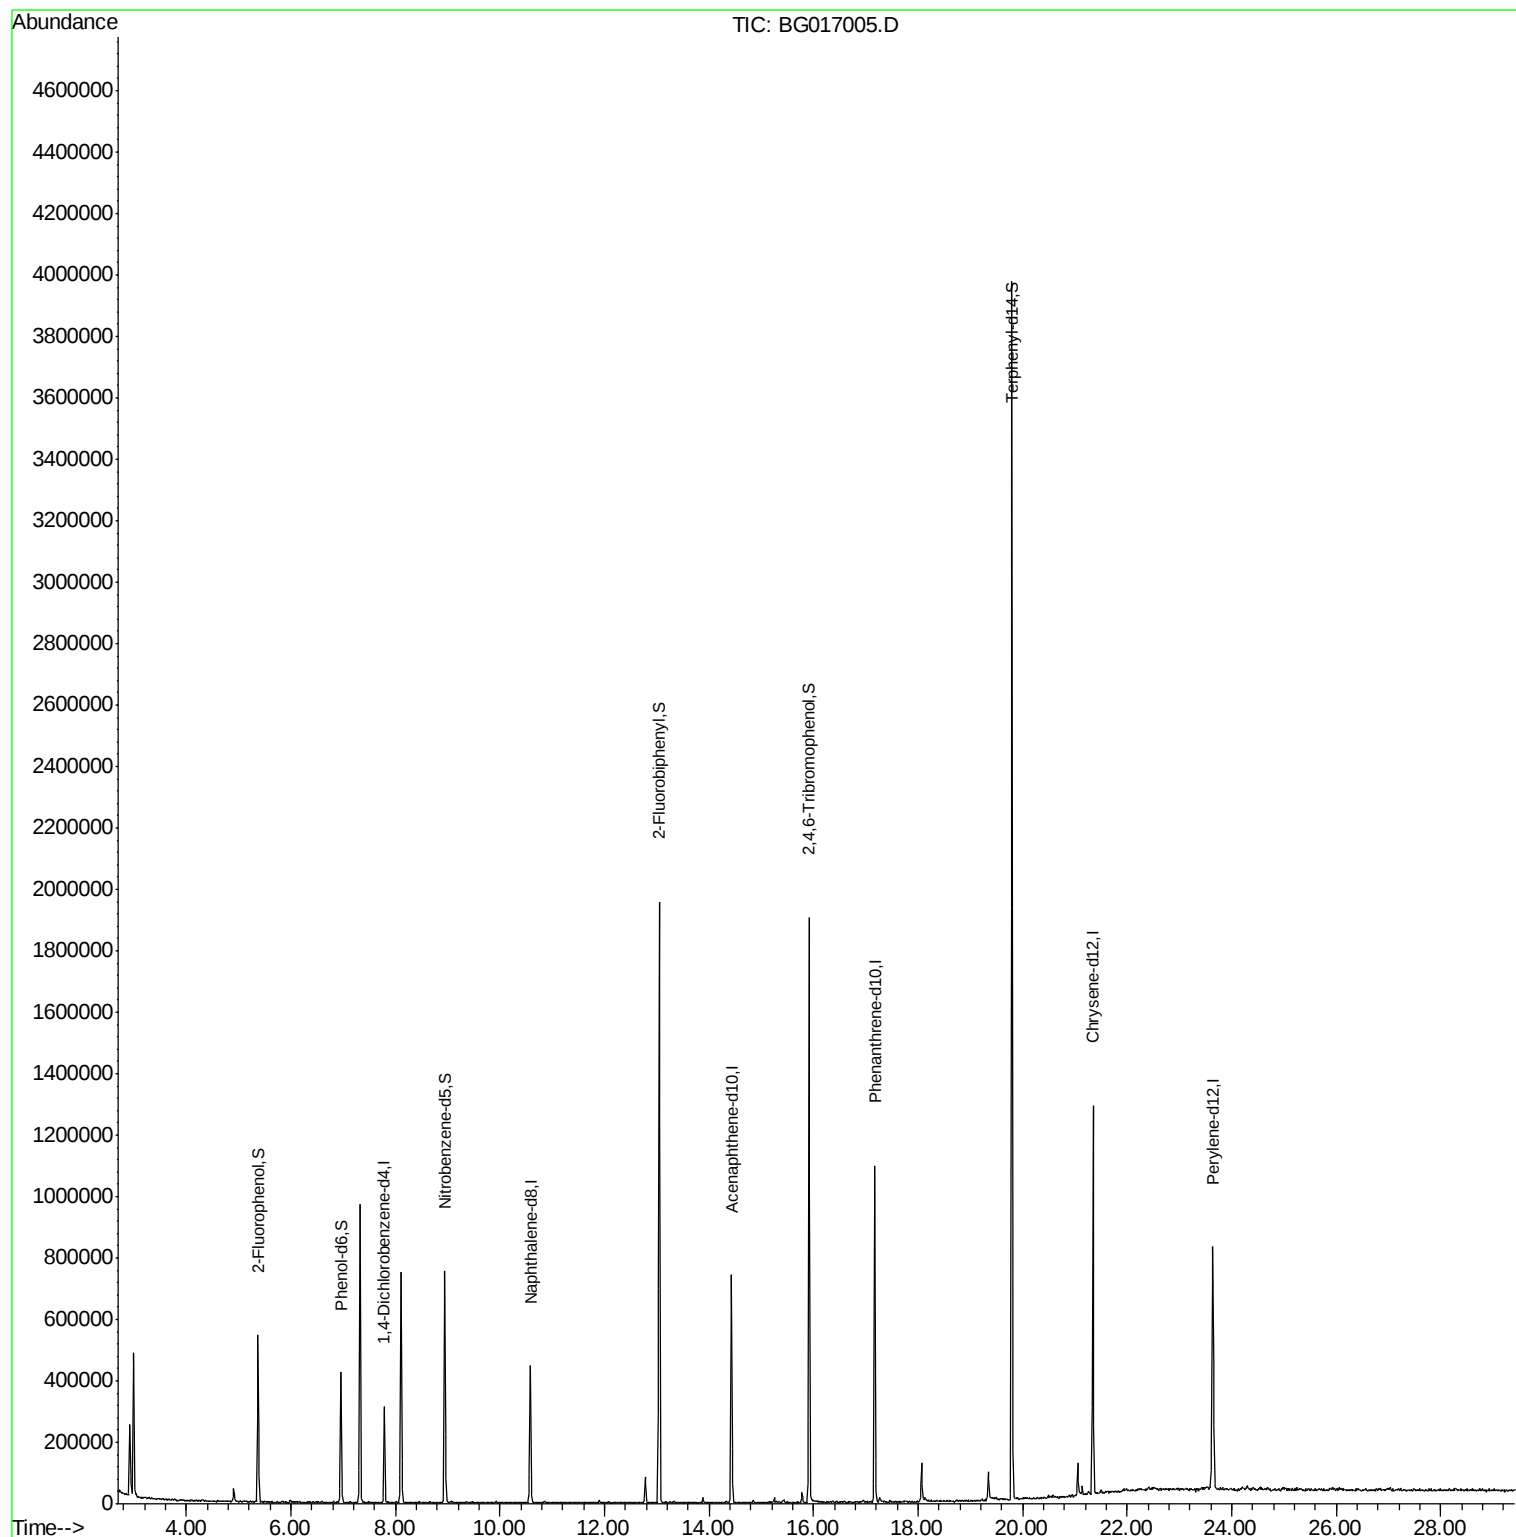



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.79 min Scan# 868

Delta R.T. -0.02 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25

Instrument :

BNA_G

ClientSampleId :

MW-105


Tgt Ion:152 Resp: 72464

Ion Ratio Lower Upper

152 100

150 157.6 121.0 181.4



115 65.2 50.5 75.7

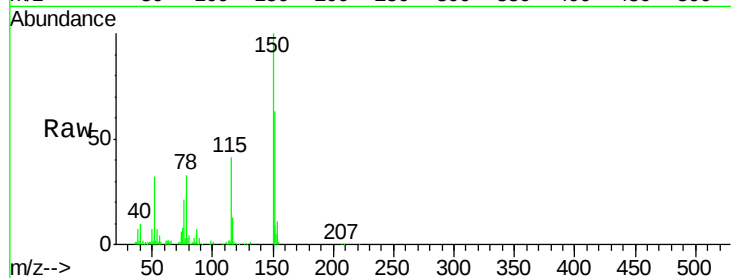

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

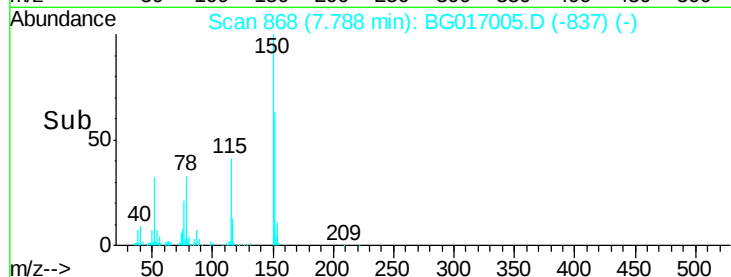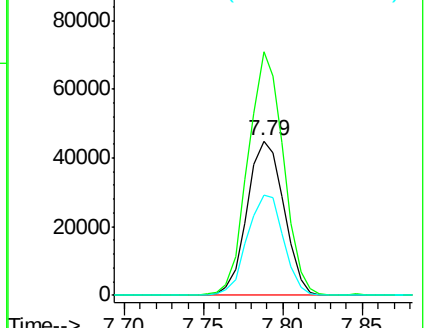

#5

2-Fluorophenol

Concen: 45.91 ng

RT: 5.37 min Scan# 457

Delta R.T. -0.01 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25


Tgt Ion:112 Resp: 191079

Ion Ratio Lower Upper

112 100

64 66.8 51.4 77.2



63 38.1 28.1 42.1

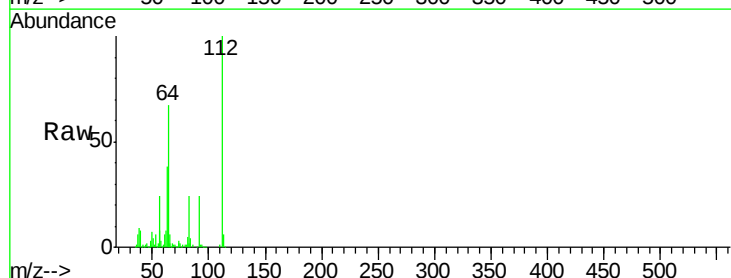

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

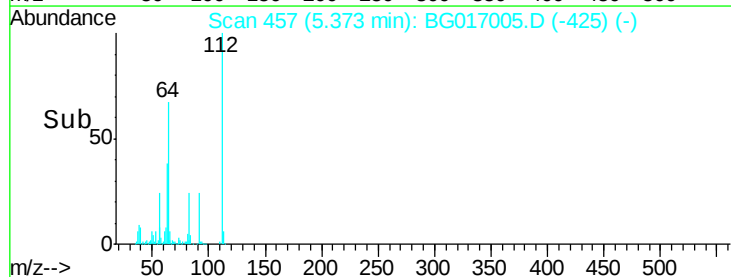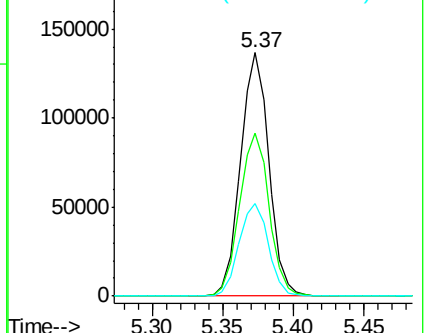



#7

Phenol-d6

Concen: 33.22 ng

RT: 6.96 min Scan# 727

Delta R.T. -0.01 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25

Instrument :

BNA_G

ClientSampleId :

MW-105





Tgt Ion: 99 Resp: 197513

Ion Ratio Lower Upper

99 100

42 27.6 22.1 33.1

71 45.3 33.4 50.0

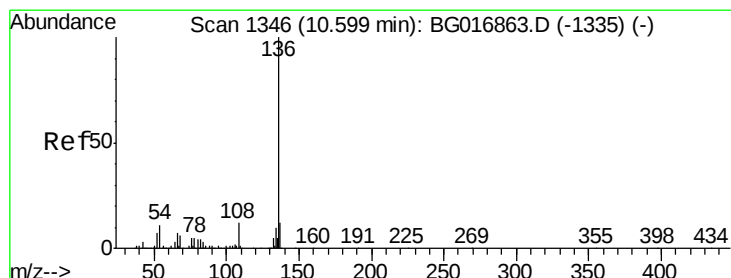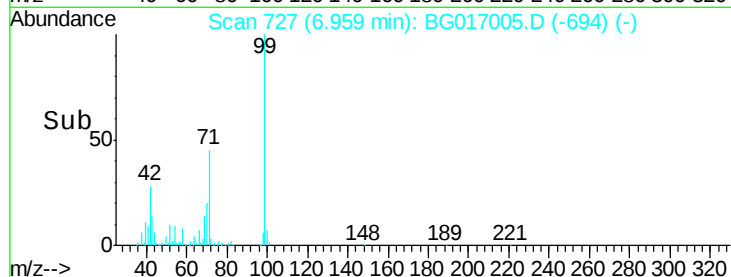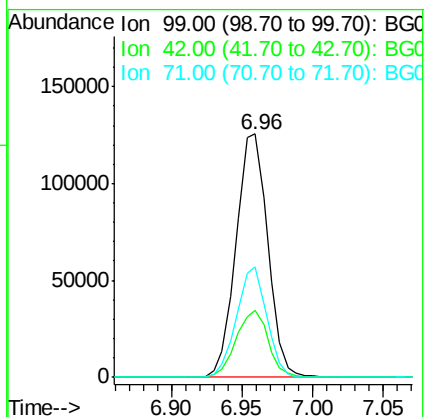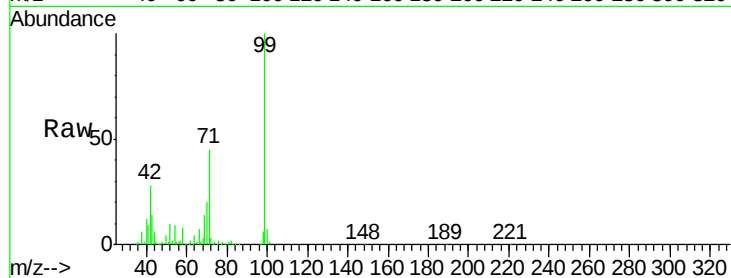

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.58 min Scan# 1344

Delta R.T. -0.01 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25

Tgt Ion: 136 Resp: 330726




Ion Ratio Lower Upper

136 100

137 9.5 9.8 14.8#

54 9.8 8.7 13.1

68 5.9 5.0 7.4


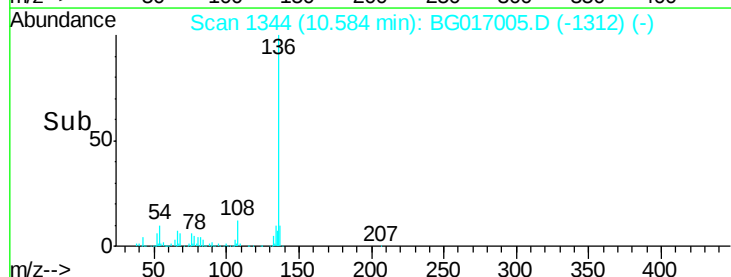
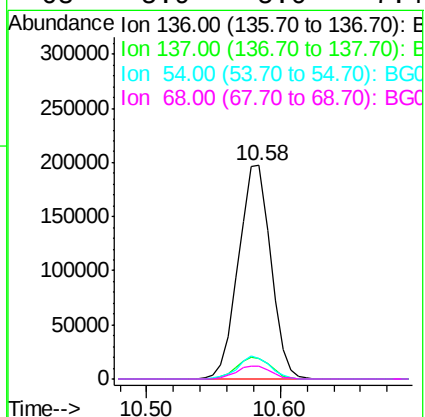
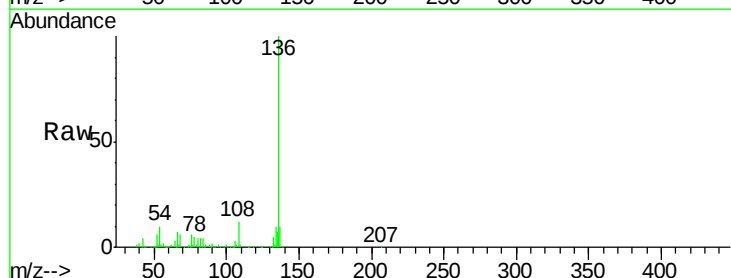




#23
 Nitrobenzene-d5
 Concen: 59.10 ng
 RT: 8.95 min Scan# 1065
 Delta R.T. -0.02 min
 Lab File: BG017005.D
 Acq: 10 May 2015 00:25




Instrument :
 BNA_G
 ClientSampleId :
 MW-105


Tgt Ion: 82 Resp: 400087
 Ion Ratio Lower Upper
 82 100
 128 41.6 33.2 49.8
 54 60.7 48.6 72.8

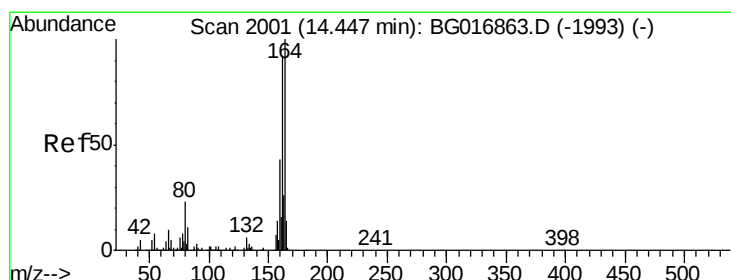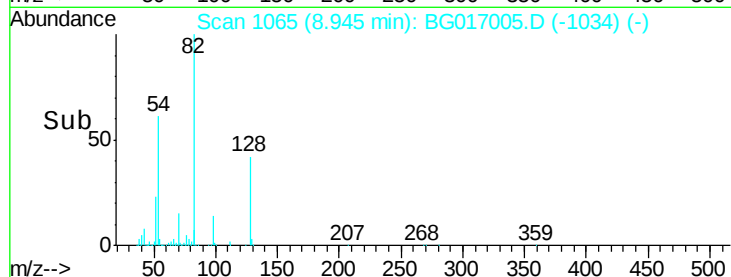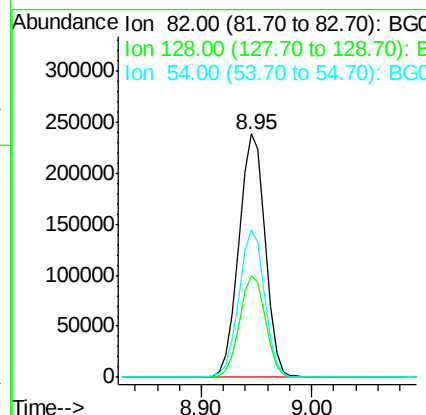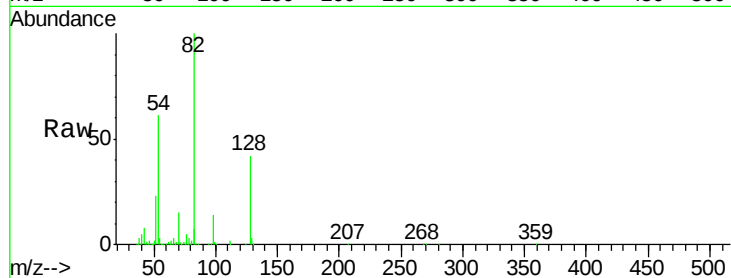

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.43 min Scan# 1998
 Delta R.T. -0.02 min
 Lab File: BG017005.D
 Acq: 10 May 2015 00:25

Tgt Ion: 164 Resp: 235610
 Ion Ratio Lower Upper
 164 100
 162 91.5 74.0 111.0
 160 43.5 34.7 52.1

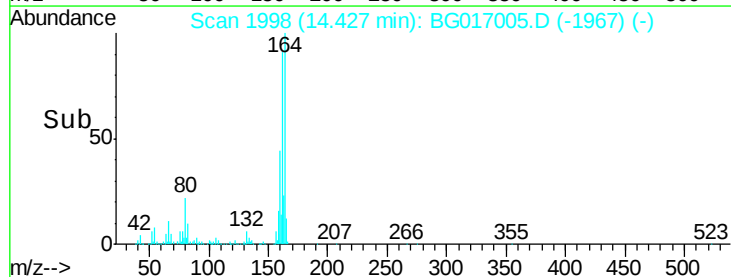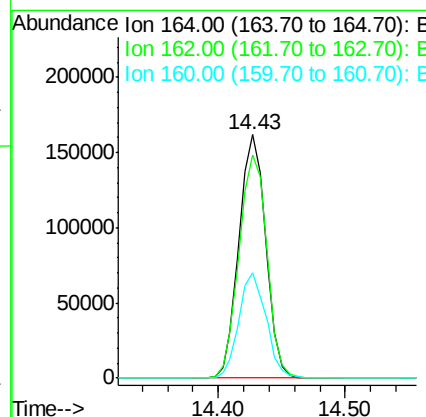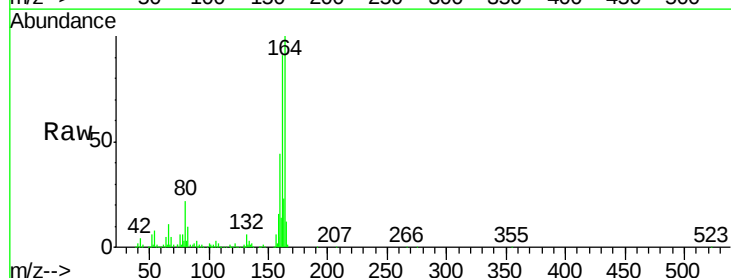


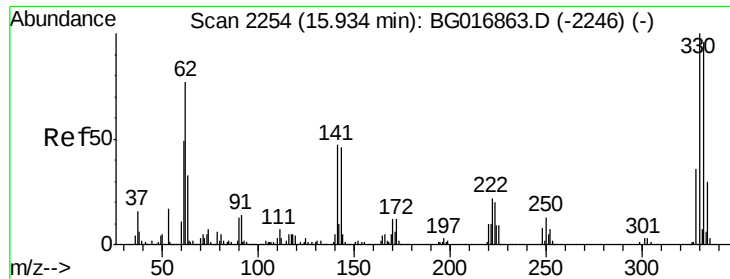




#41
 2,4,6-Tribromophenol
 Concen: 114.82 ng
 RT: 15.91 min Scan# 2251
 Delta R.T. -0.02 min
 Lab File: BG017005.D
 Acq: 10 May 2015 00:25

Instrument :
 BNA_G
 ClientSampleId :
 MW-105

Tgt Ion: 330 Resp: 271583
 Ion Ratio Lower Upper
 330 100
 332 94.8 0.0 0.0#
 141 49.8 0.0 0.0#

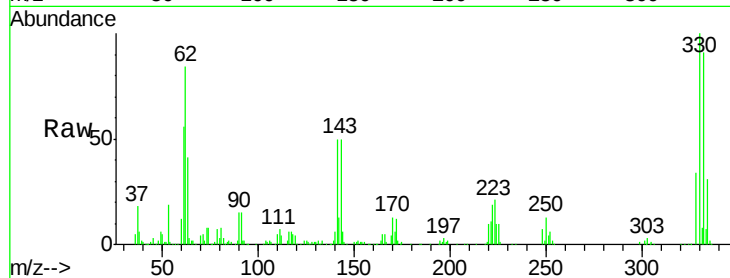


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

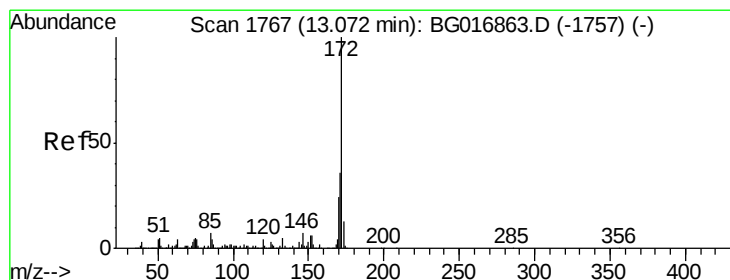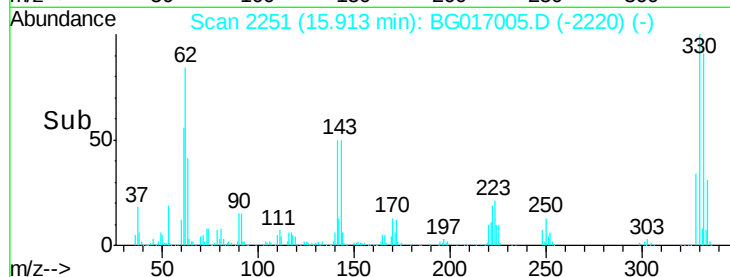
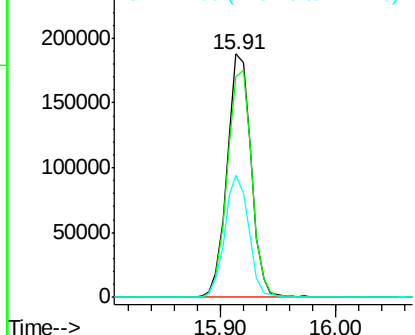



#44
 2-Fluorobiphenyl
 Concen: 54.90 ng
 RT: 13.05 min Scan# 1764
 Delta R.T. -0.02 min
 Lab File: BG017005.D
 Acq: 10 May 2015 00:25

Tgt Ion: 172 Resp: 857197
 Ion Ratio Lower Upper
 172 100
 171 37.1 29.0 43.4
 170 23.7 19.0 28.4

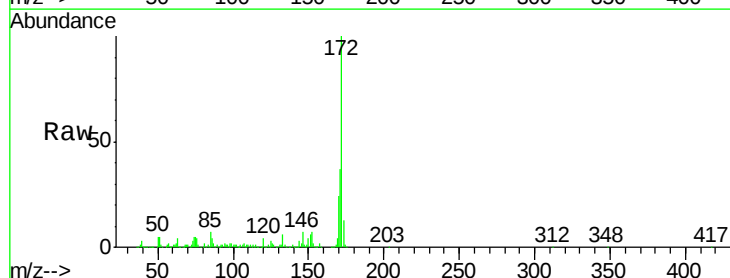

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

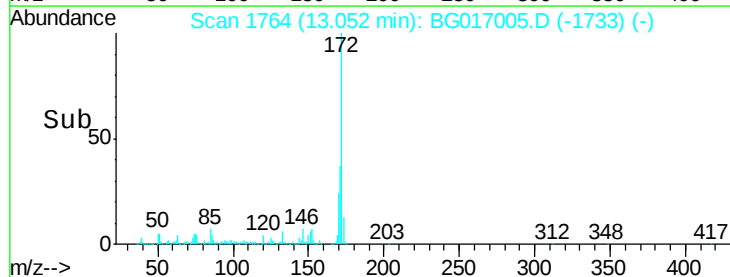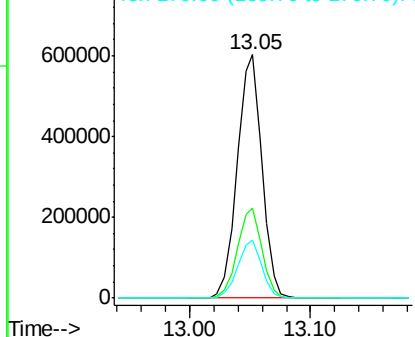


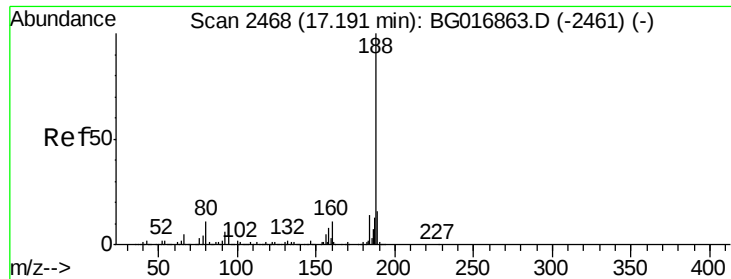

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.17 min Scan# 2465
Delta R.T. -0.02 min
Lab File: BG017005.D
Acq: 10 May 2015 00:25

Instrument :
BNA_G
ClientSampleId :
MW-105




Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.6	8.2	12.4
80	11.2	8.8	13.2

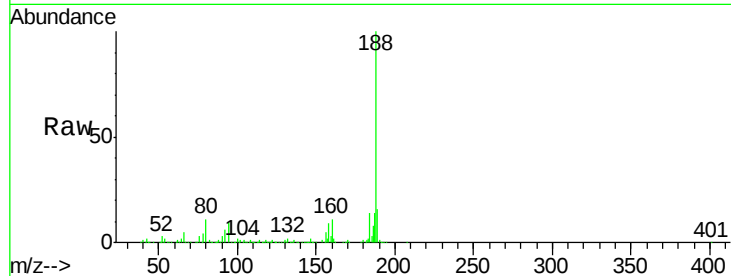

Abundance Ion 188.00 (187.70 to 188.70): E


Ion 94.00 (93.70 to 94.70): B

Ion 80.00 (79.70 to 80.70): B

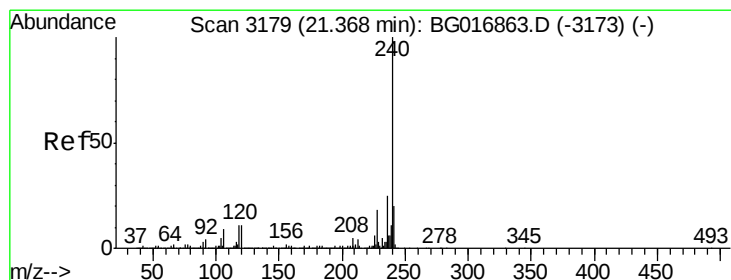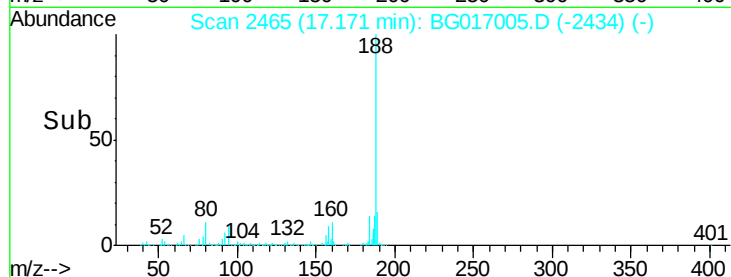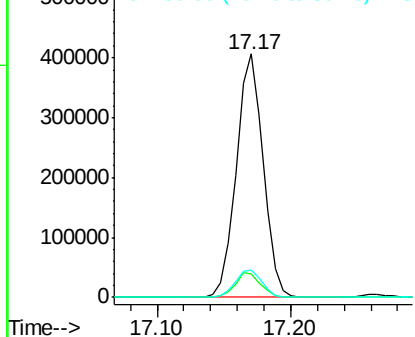

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.35 min Scan# 3176
Delta R.T. -0.02 min
Lab File: BG017005.D
Acq: 10 May 2015 00:25



Tgt Ion	Ratio	Lower	Upper
240	100		
120	9.8	9.1	13.7
236	26.2	20.2	30.4

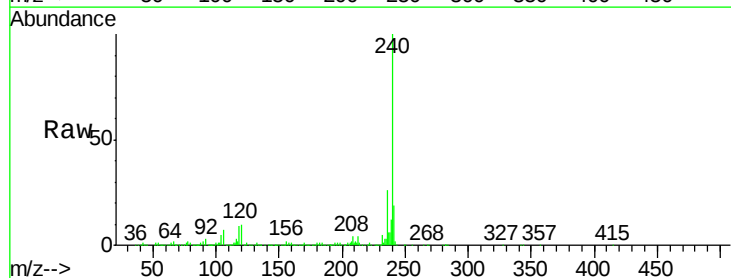


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

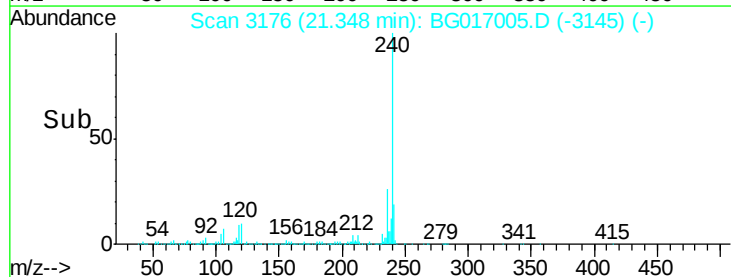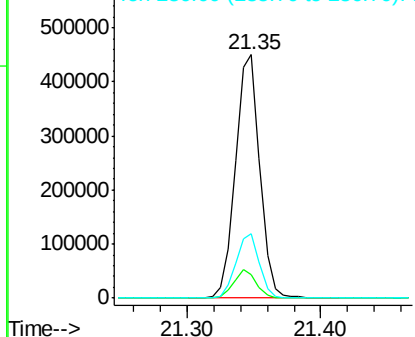

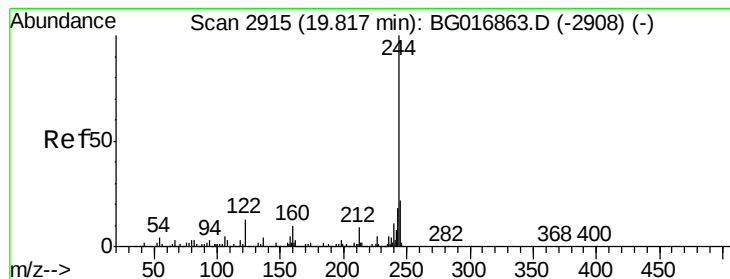

#78

Terphenyl-d14

Concen: 60.67 ng

RT: 19.80 min Scan# 2912

Delta R.T. -0.02 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25

Instrument :

BNA_G

ClientSampleId :

MW-105


Tgt Ion:244 Resp: 1475018

Ion Ratio Lower Upper

244 100

212 9.4 7.0 10.6




122 12.9 10.4 15.6

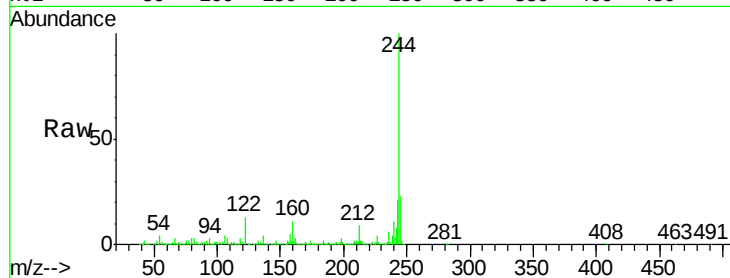

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

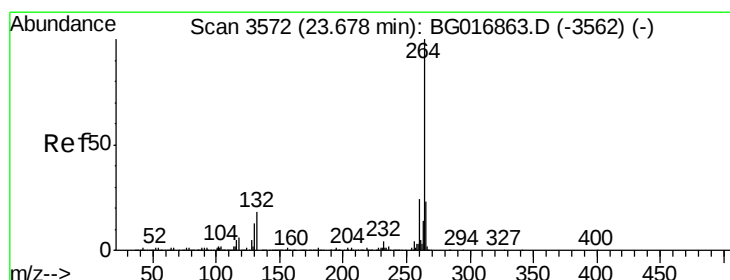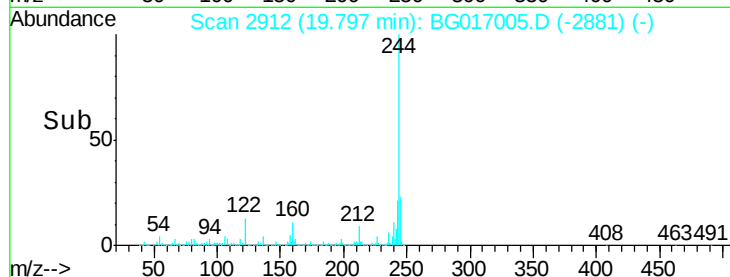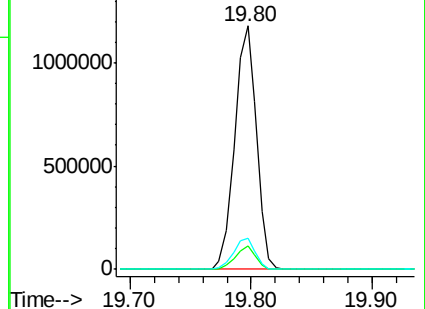

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.64 min Scan# 3566

Delta R.T. -0.04 min

Lab File: BG017005.D

Acq: 10 May 2015 00:25


Tgt Ion:264 Resp: 555768

Ion Ratio Lower Upper

264 100

260 23.8 19.5 29.3

265 23.2 18.5 27.7

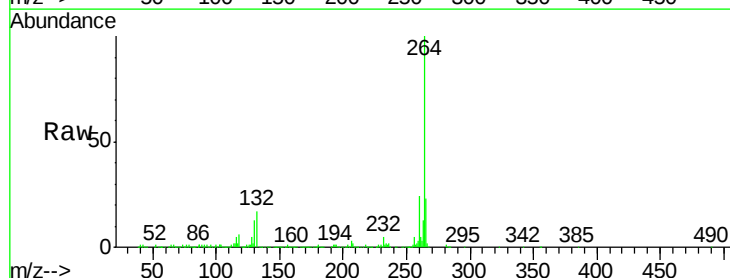

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

